


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011019\
 Data File : BG039053.D
 Acq On : 10 Jan 2019 14:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

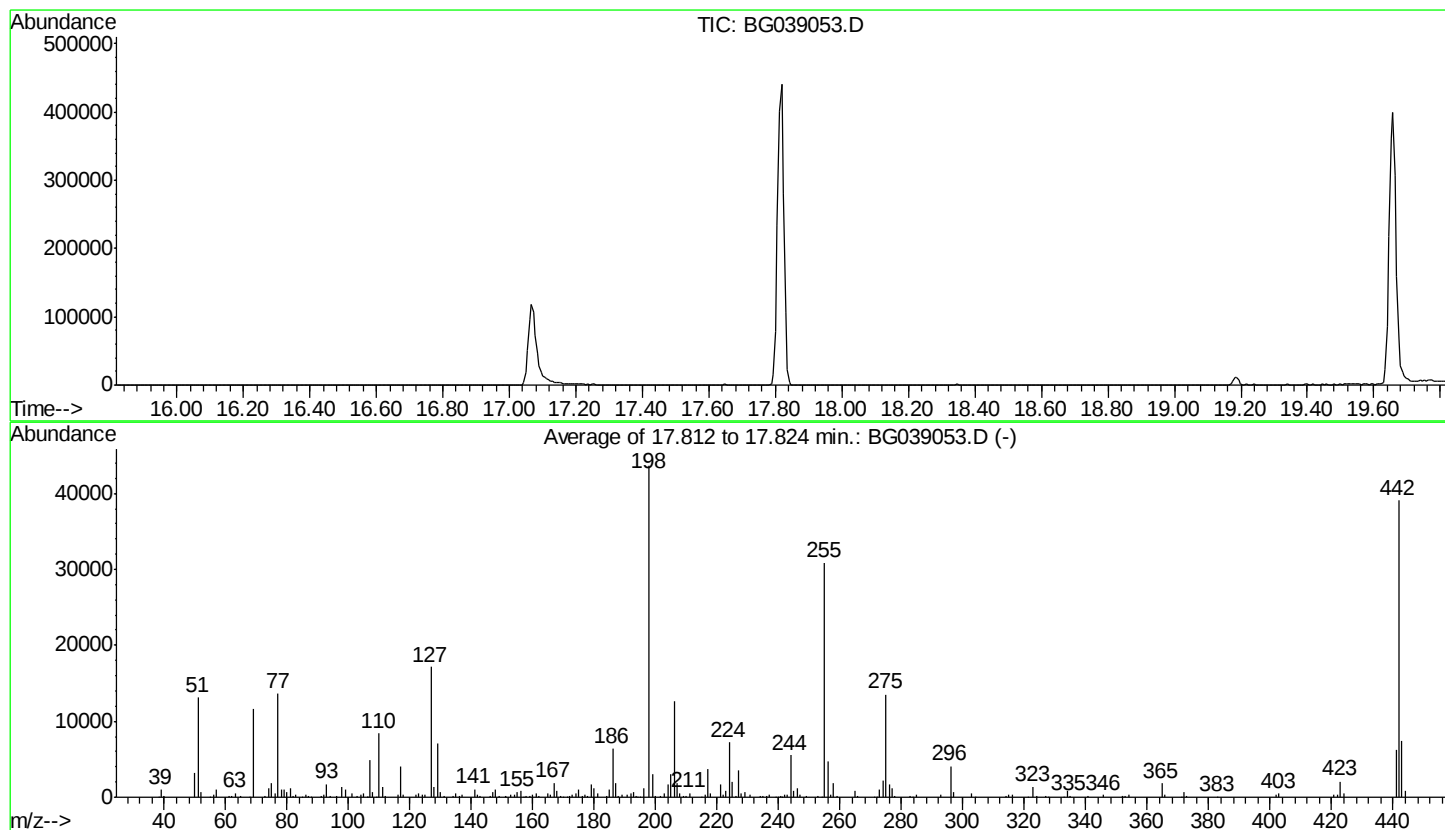

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	13139	PASS
68	69	0.00	2	0.6	71	PASS
69	198	0.00	100	26.7	11671	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	17188	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43656	PASS
199	198	5	9	7.0	3066	PASS
275	198	10	60	31.0	13550	PASS
365	198	1	100	4.1	1798	PASS
441	198	0.01	100	14.4	6273	PASS
442	198	50	100	89.4	39048	PASS
443	442	15	24	18.9	7387	PASS