
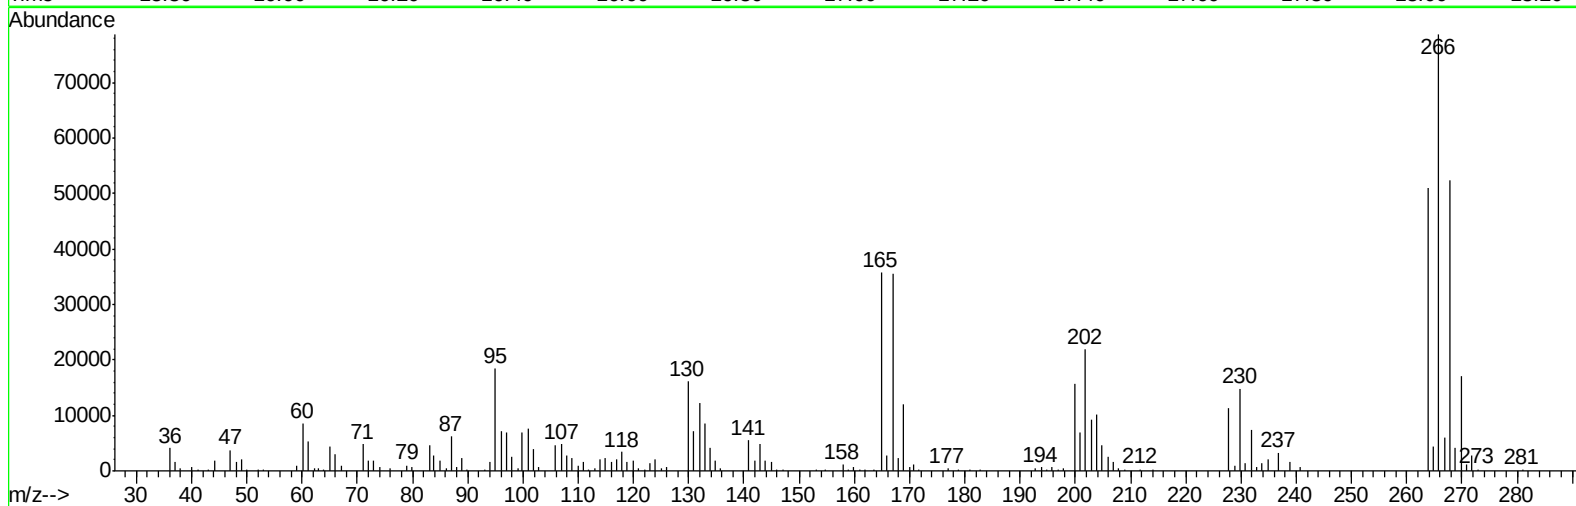


Data File : BG043996.D
Acq On : 10 Jan 2020 10:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 05:58:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

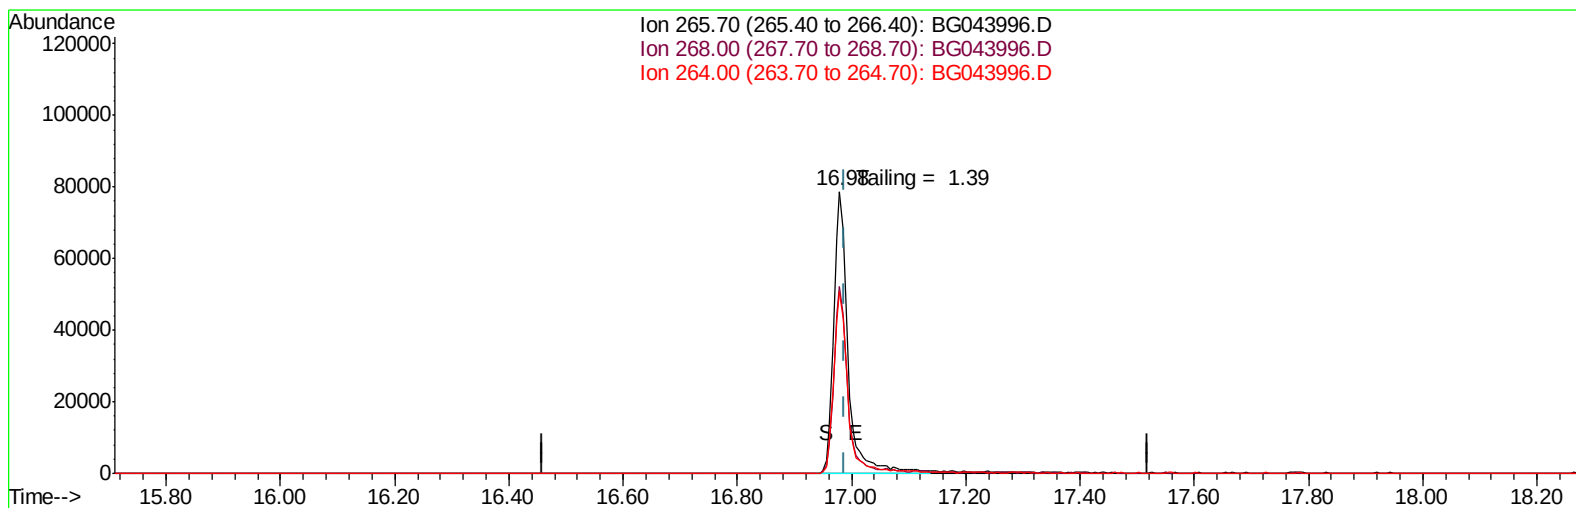

TIC: BG043996.D

(70) Pentachlorophenol (C)



16.979min (-0.010) 23317.22ng

response 134743

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	66.56
264.00	63.50	64.70
0.00	0.00	0.00

Data File : BG043996.D
Acq On : 10 Jan 2020 10:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 05:58:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

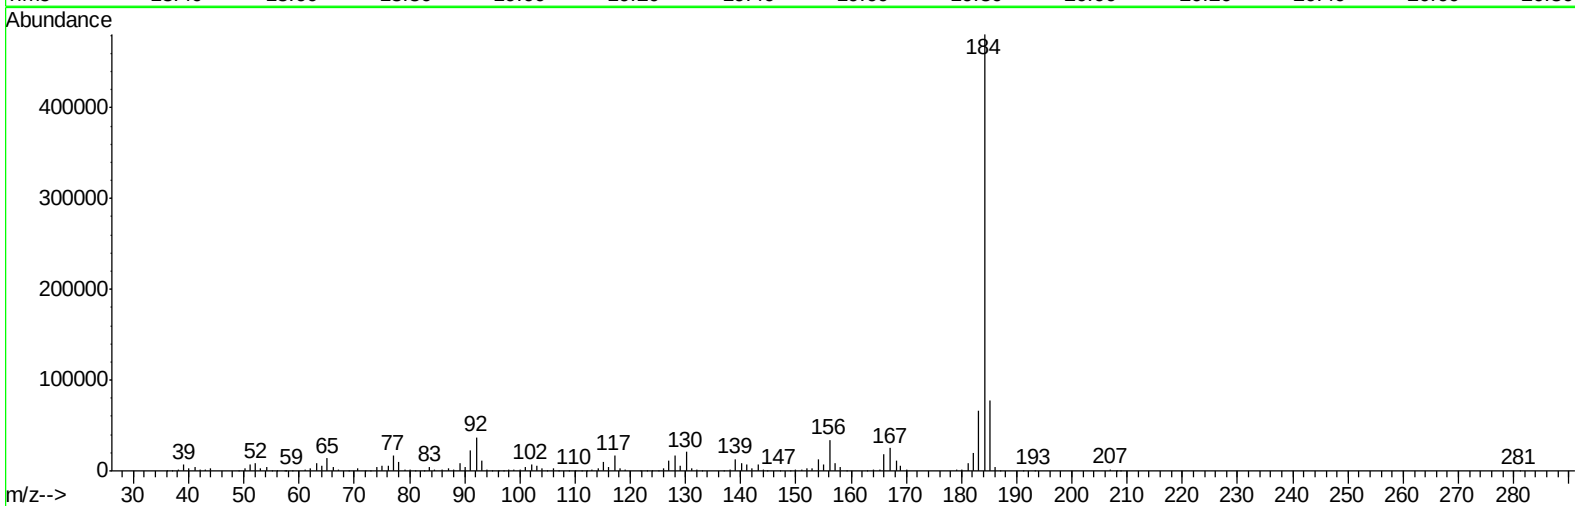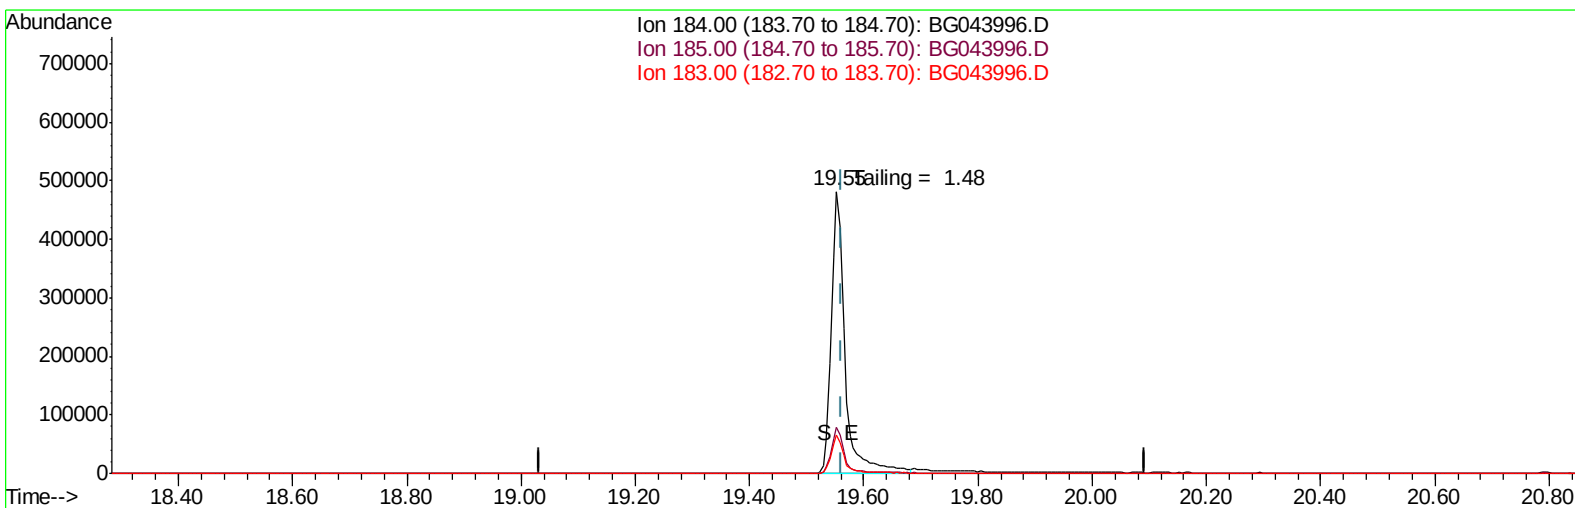

TIC: BG043996.D

(77) Benzidine

19.553min (-0.010) 463454.86ng

response 827096

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.19
183.00	13.20	13.71
0.00	0.00	0.00