


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011020\
 Data File : BG043996.D
 Acq On : 10 Jan 2020 10:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

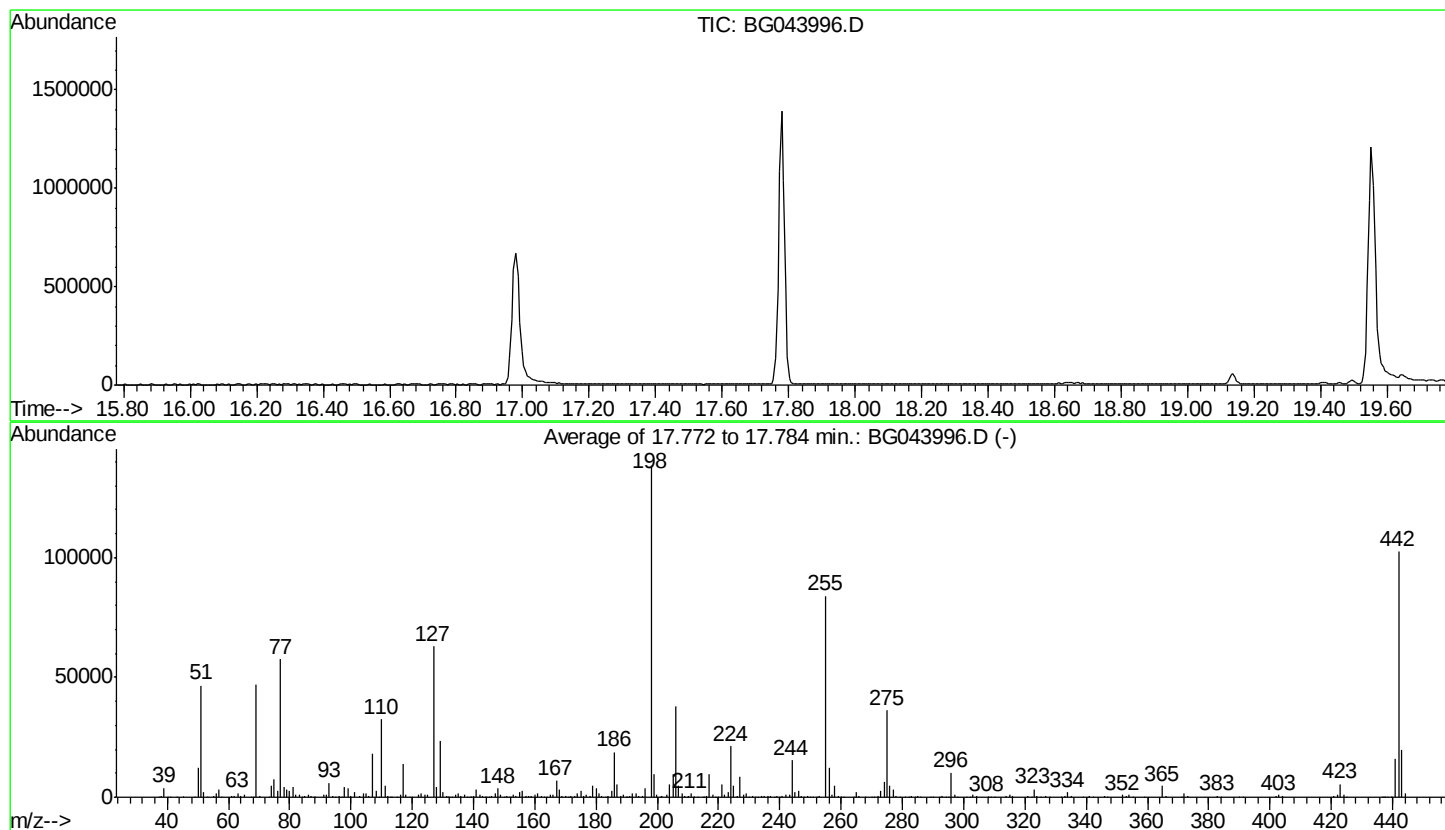

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	46546	PASS
68	69	0.00	2	0.6	265	PASS
69	198	0.00	100	34.1	47245	PASS
70	69	0.00	2	0.7	311	PASS
127	198	10	80	45.5	62954	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	138368	PASS
199	198	5	9	7.0	9653	PASS
275	198	10	60	26.2	36258	PASS
365	198	1	100	3.3	4587	PASS
441	198	0.01	100	11.6	16041	PASS
442	198	50	100	74.0	102341	PASS
443	442	15	24	19.5	19968	PASS