


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011119\
 Data File : BG039104.D
 Acq On : 12 Jan 2019 5:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

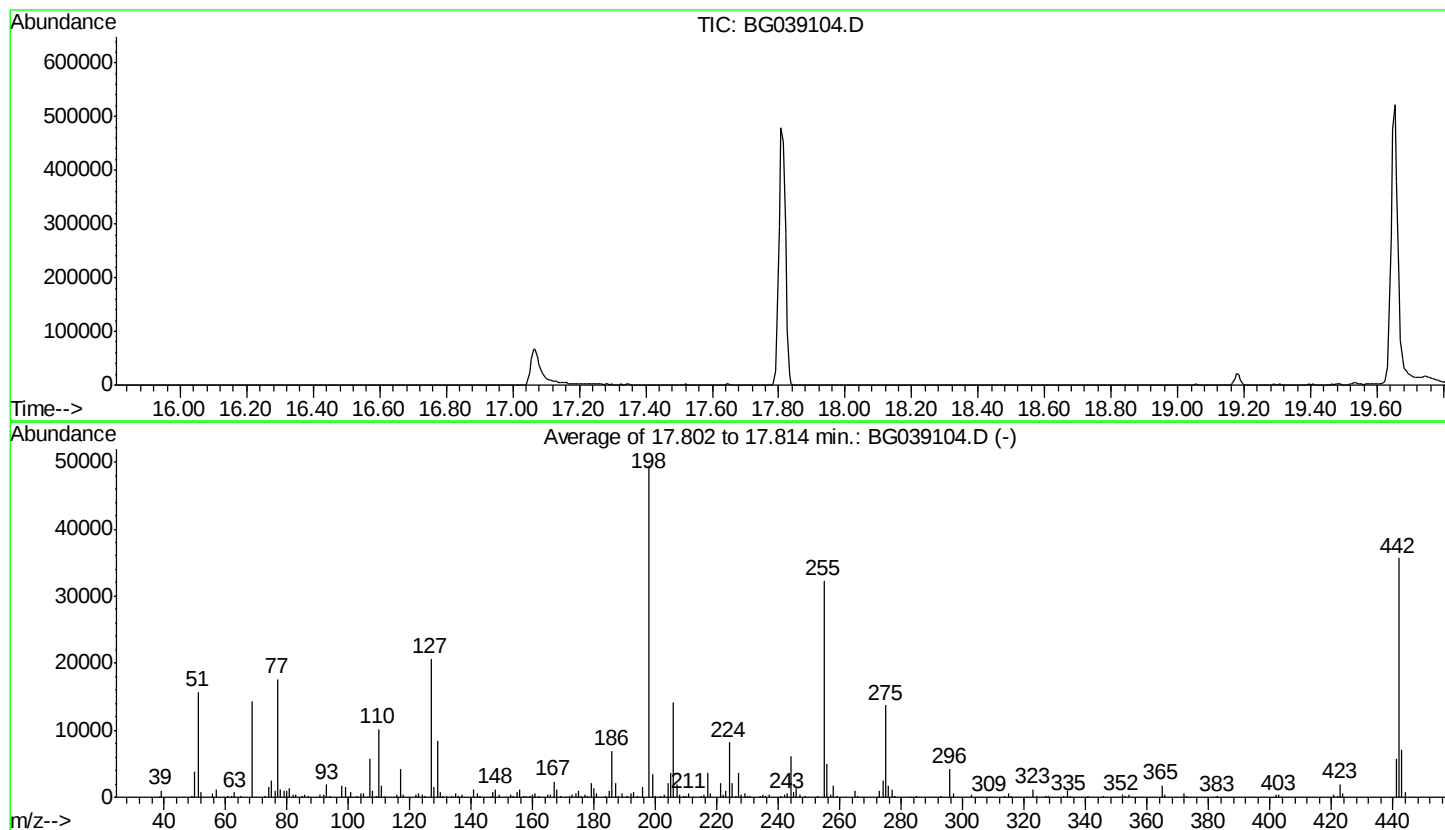

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	15677	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.8	14247	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	20678	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49453	PASS
199	198	5	9	7.1	3504	PASS
275	198	10	60	27.7	13693	PASS
365	198	1	100	3.6	1804	PASS
441	198	0.01	100	11.6	5719	PASS
442	198	50	100	72.1	35680	PASS
443	442	15	24	19.7	7026	PASS