


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011320\
 Data File : BG044014.D
 Acq On : 13 Jan 2020 16:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

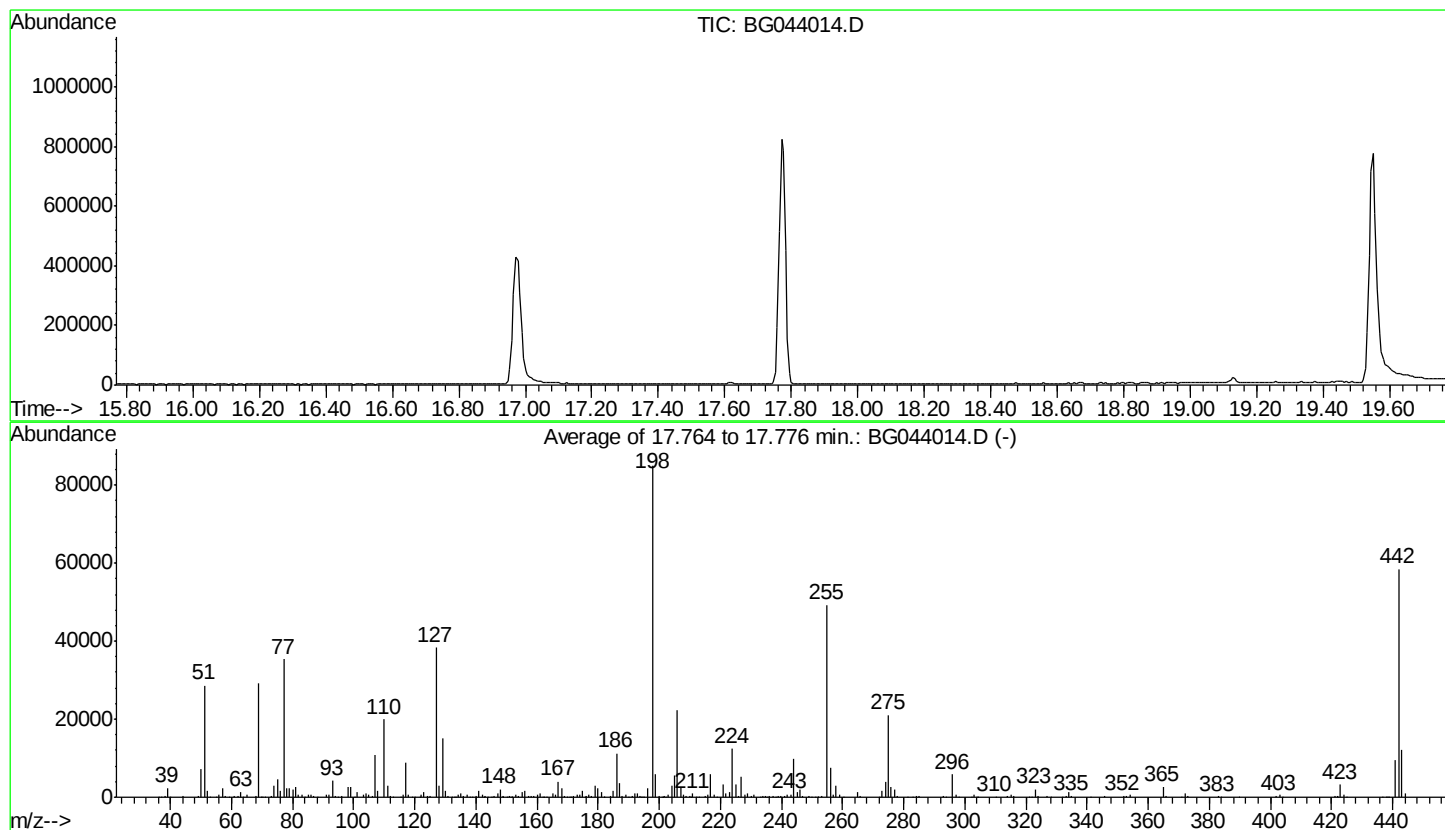

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	28560	PASS
68	69	0.00	2	1.6	472	PASS
69	198	0.00	100	34.5	29338	PASS
70	69	0.00	2	0.5	151	PASS
127	198	10	80	45.1	38312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84981	PASS
199	198	5	9	6.9	5859	PASS
275	198	10	60	24.8	21038	PASS
365	198	1	100	3.1	2674	PASS
441	198	0.01	100	11.2	9541	PASS
442	198	50	100	68.8	58504	PASS
443	442	15	24	20.6	12059	PASS