
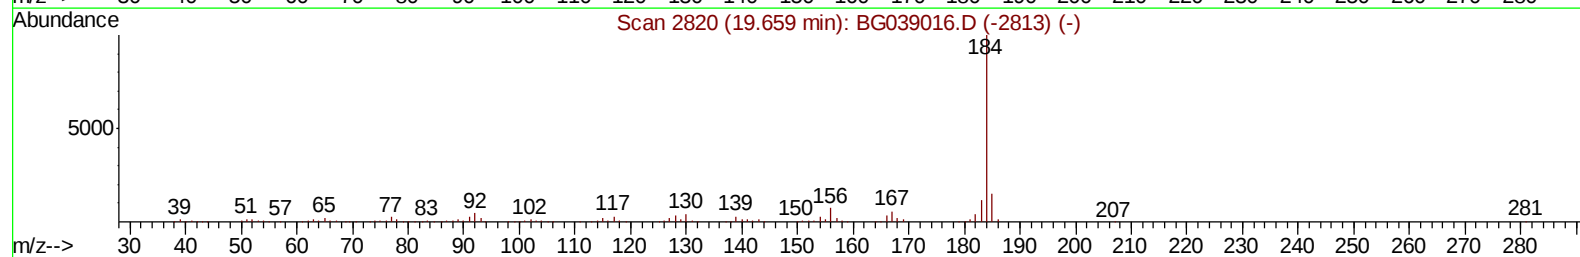
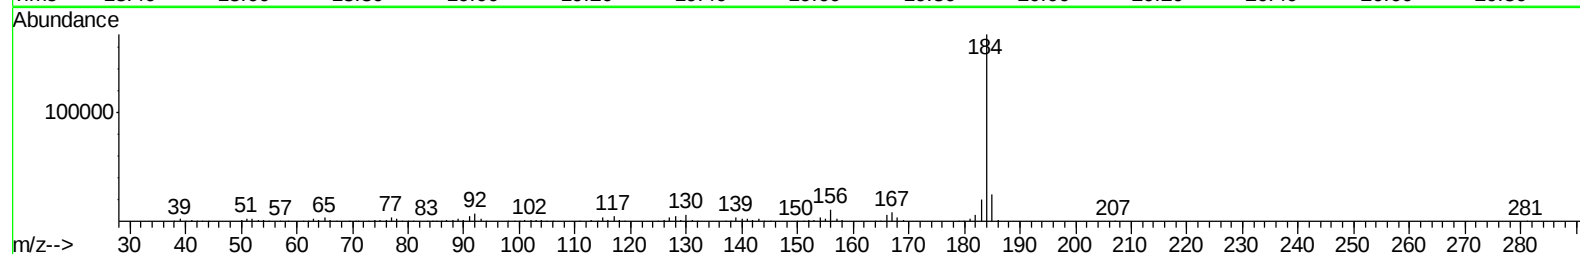


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011419\
Data File : BG039120.D
Acq On : 14 Jan 2019 14:30
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 00:12:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

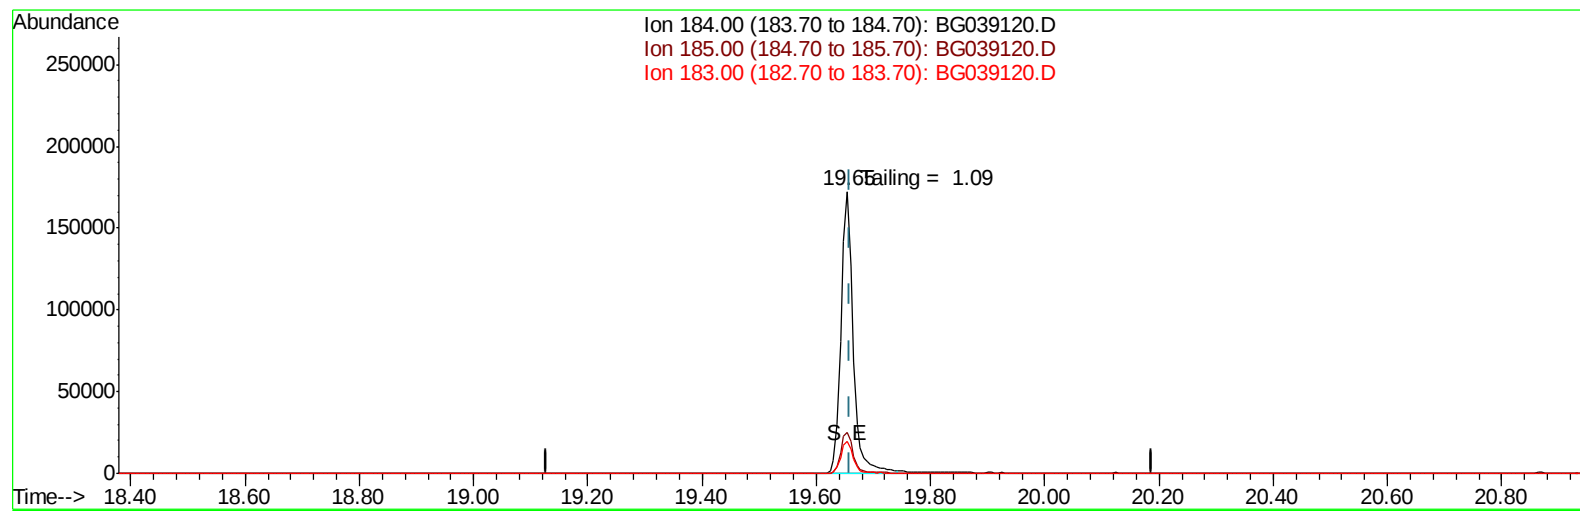

TIC: BG039120.D

(77) Benzidine




19.654min (-0.005) 0.00ng

response 258255

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.60
183.00	11.90	11.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011419\
Data File : BG039120.D
Acq On : 14 Jan 2019 14:30
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 00:12:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

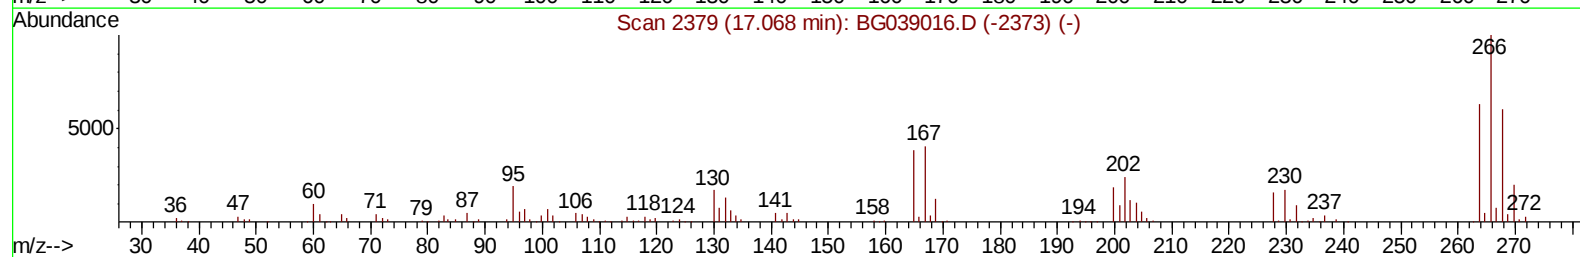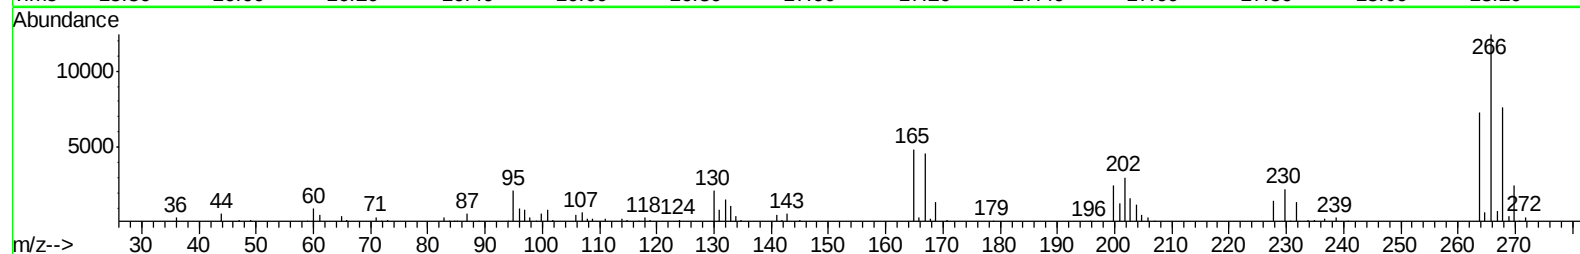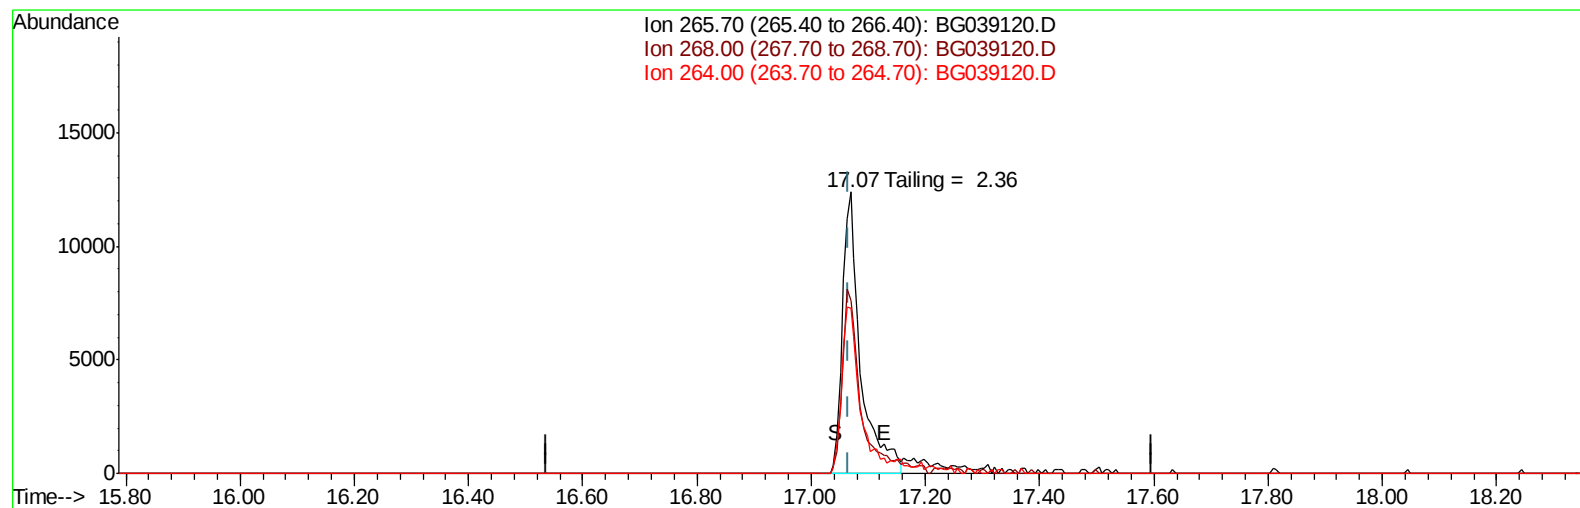

TIC: BG039120.D

(70) Pentachlorophenol (C)

17.069min (+0.002) 19858.36ng

response 27268

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.60
264.00	68.20	64.61
0.00	0.00	0.00