


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011419\  
 Data File : BG039120.D  
 Acq On : 14 Jan 2019 14:30  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG010919.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jan 09 14:23:53 2019

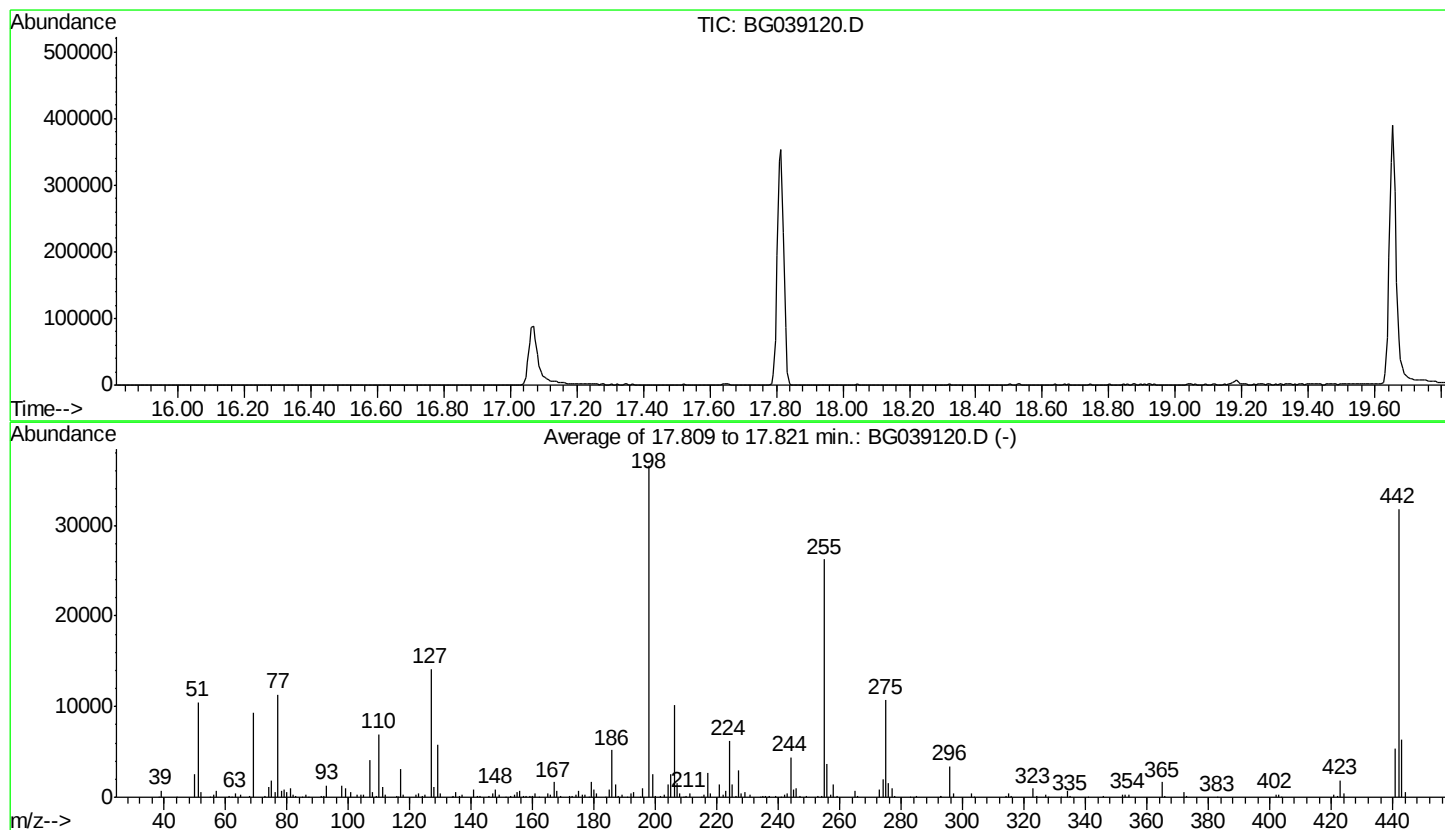

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.7      | 10506   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 129     | PASS             |
| 69          | 198          | 0.00         | 100          | 25.3      | 9270    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 38.8      | 14196   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 36581   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 2508    | PASS             |
| 275         | 198          | 10           | 60           | 29.5      | 10785   | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 1680    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.7      | 5388    | PASS             |
| 442         | 198          | 50           | 100          | 86.9      | 31781   | PASS             |
| 443         | 442          | 15           | 24           | 20.1      | 6376    | PASS             |