
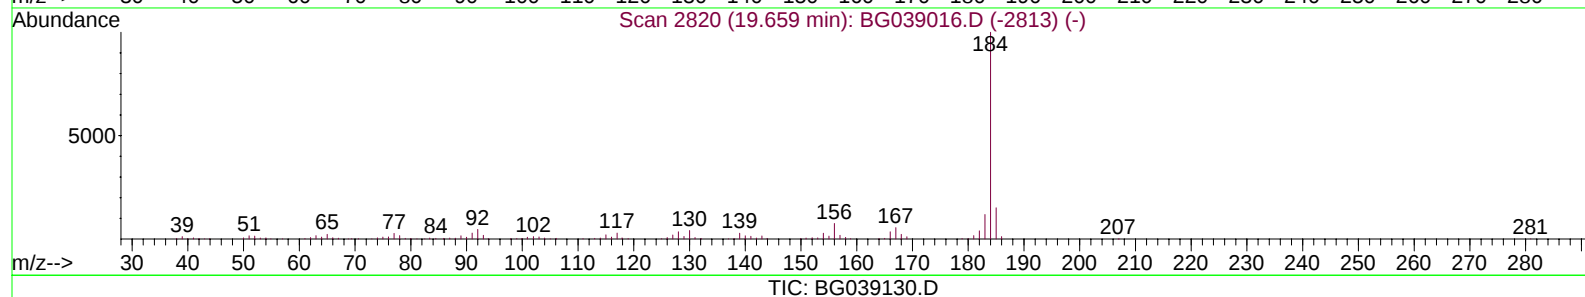
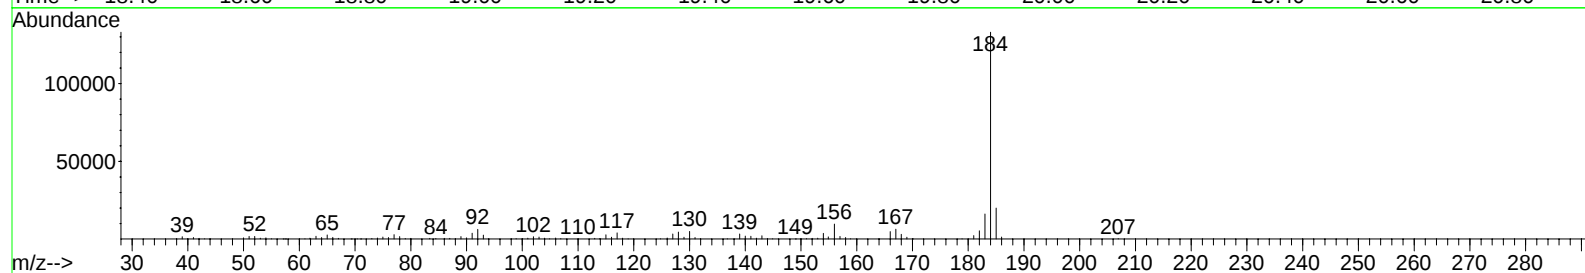


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011519\
 Data File : BG039130.D
 Acq On : 15 Jan 2019 12:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 18:06:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 09 14:23:53 2019
 Response via : Initial Calibration

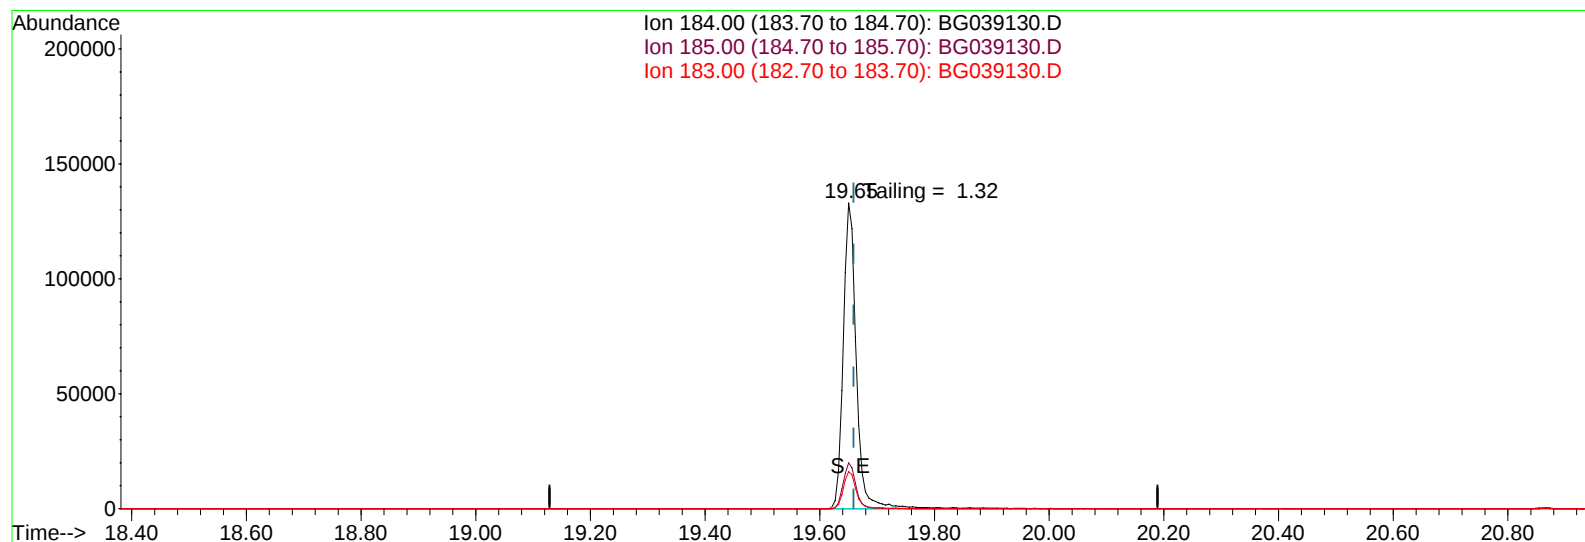

(77) Benzidine




19.650min (-0.009) 0.00ng

response 209488

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.01
183.00	11.90	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011519\
Data File : BG039130.D
Acq On : 15 Jan 2019 12:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 18:06:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

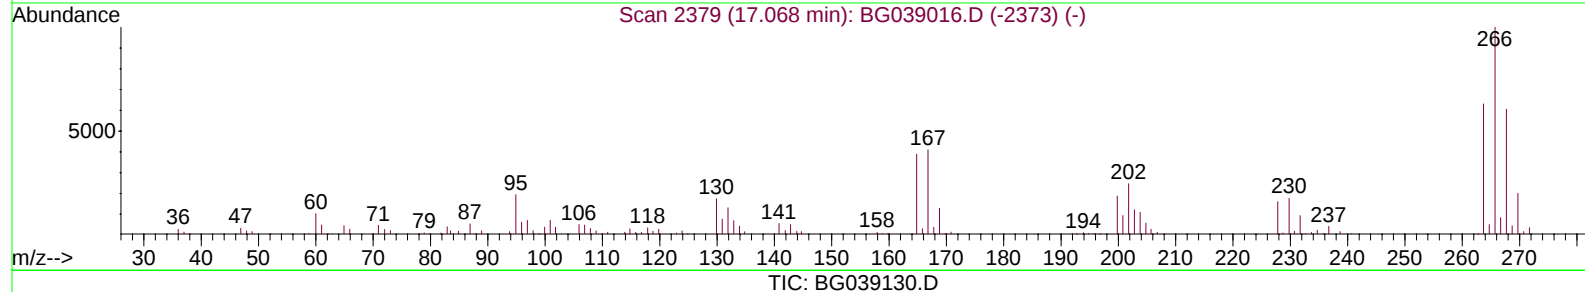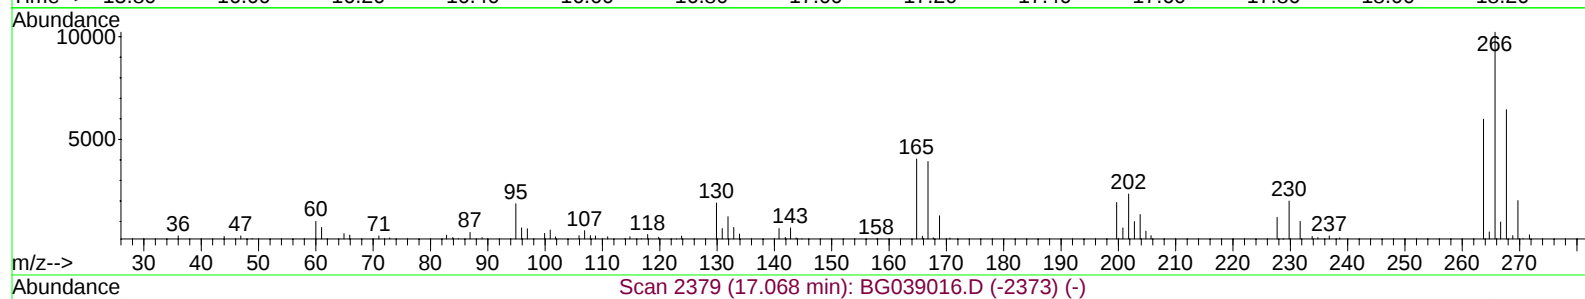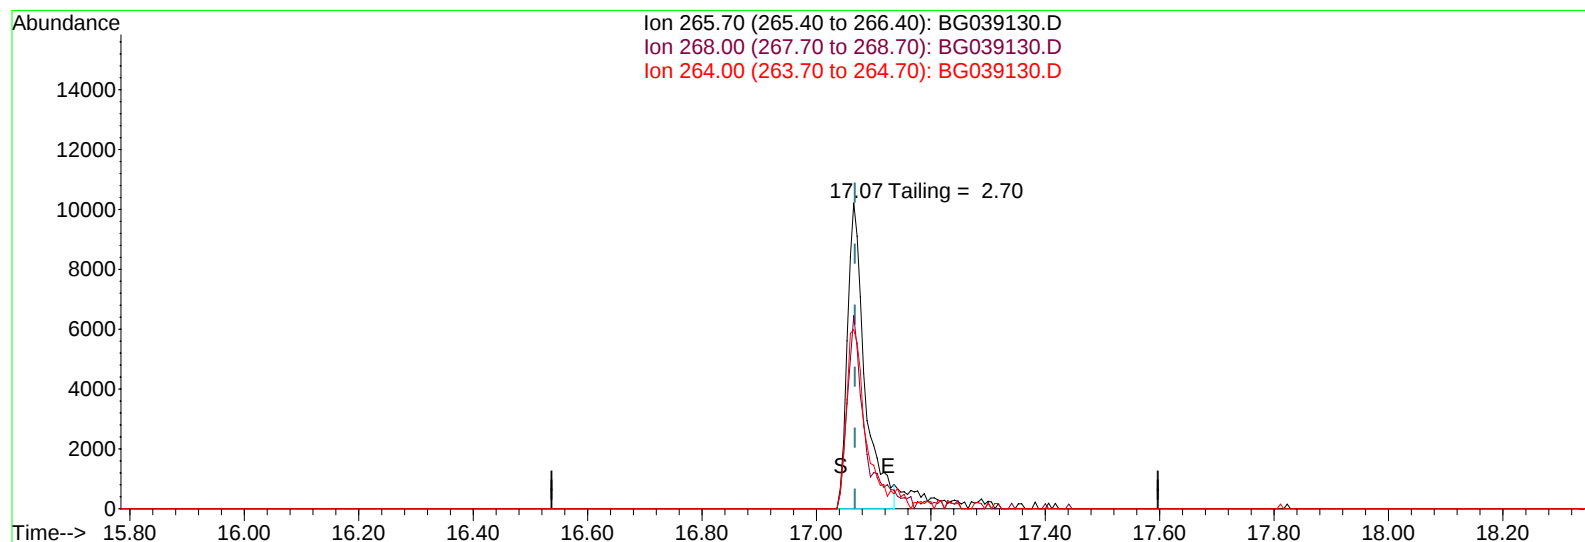

(70) Pentachlorophenol (C)

17.065min (-0.002) 17720.20ng

response 22676

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.13
264.00	68.20	63.45
0.00	0.00	0.00