
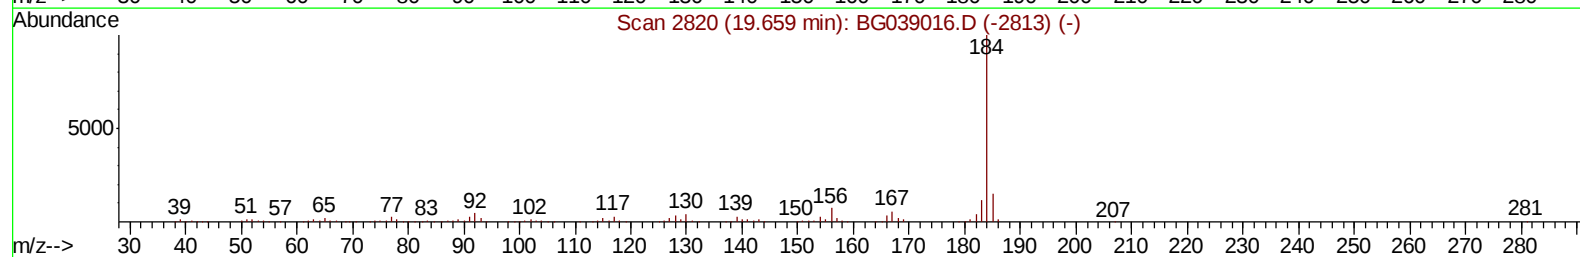
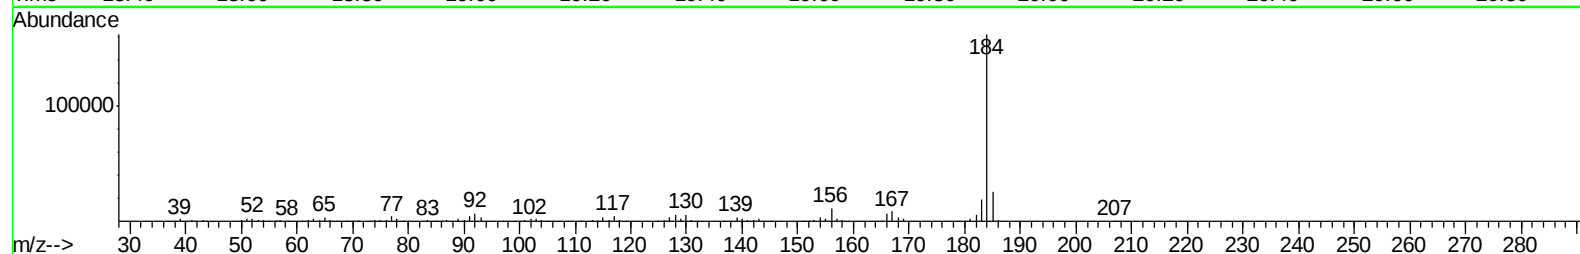


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011519\
Data File : BG039146.D
Acq On : 16 Jan 2019 2:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:44:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

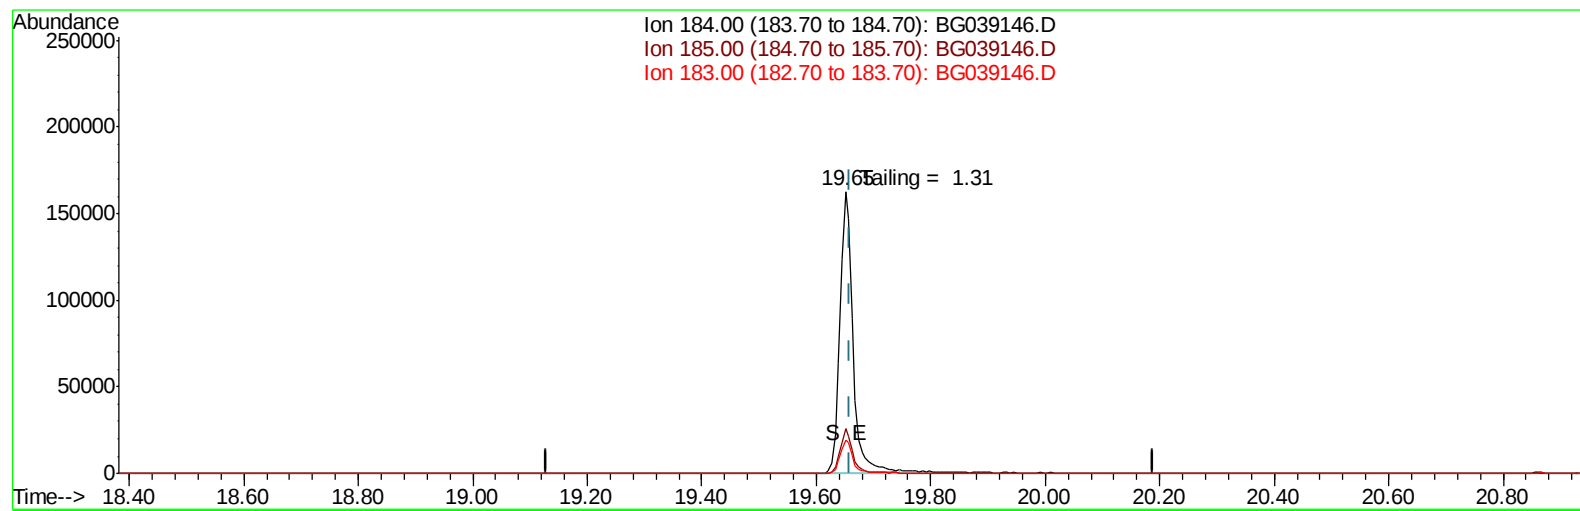

TIC: BG039146.D

(77) Benzidine




19.651min (-0.008) 0.00ng

response 263789

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.84
183.00	11.90	12.06
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011519\
Data File : BG039146.D
Acq On : 16 Jan 2019 2:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:44:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

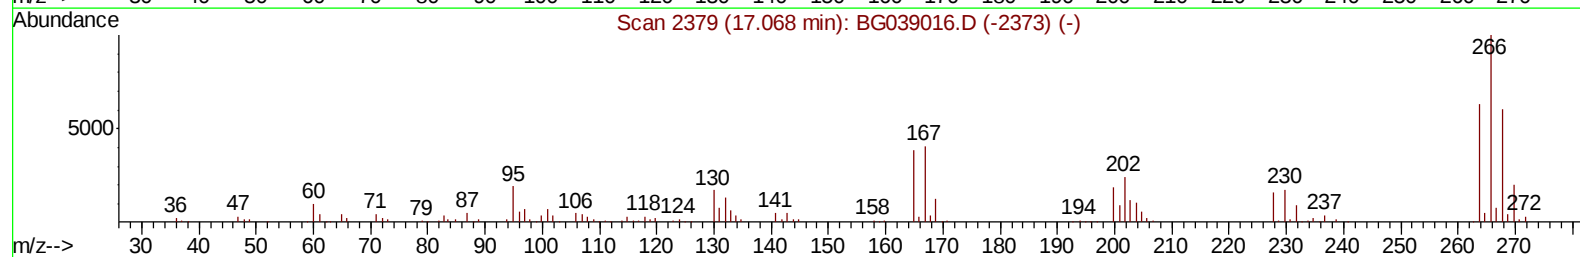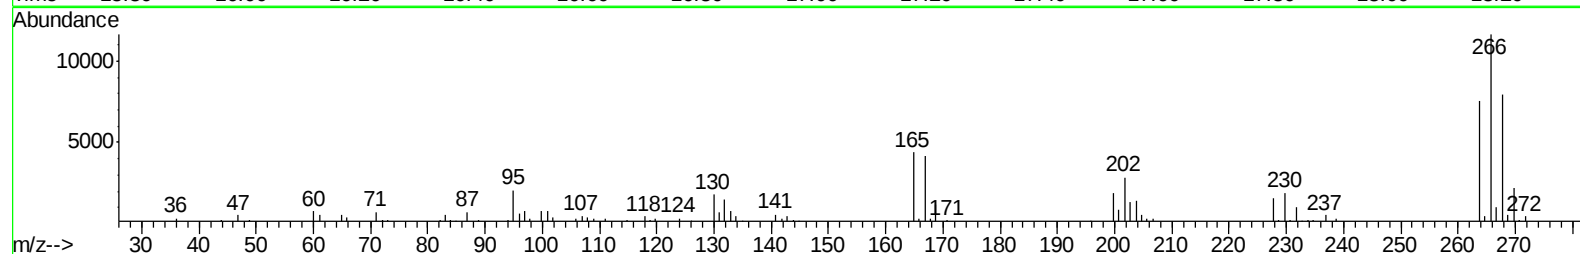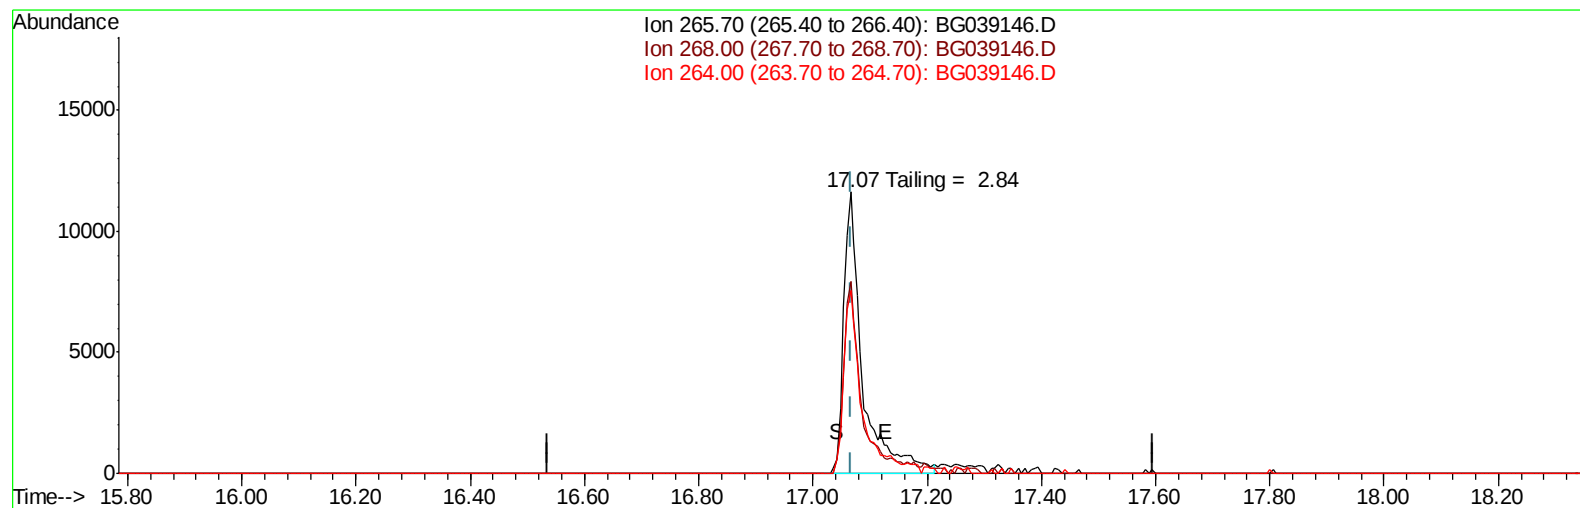

TIC: BG039146.D

(70) Pentachlorophenol (C)

17.066min (-0.001) 23872.12ng

response 26760

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	73.27
264.00	68.20	69.08
0.00	0.00	0.00