


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011519\
 Data File : BG039130.D
 Acq On : 15 Jan 2019 12:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

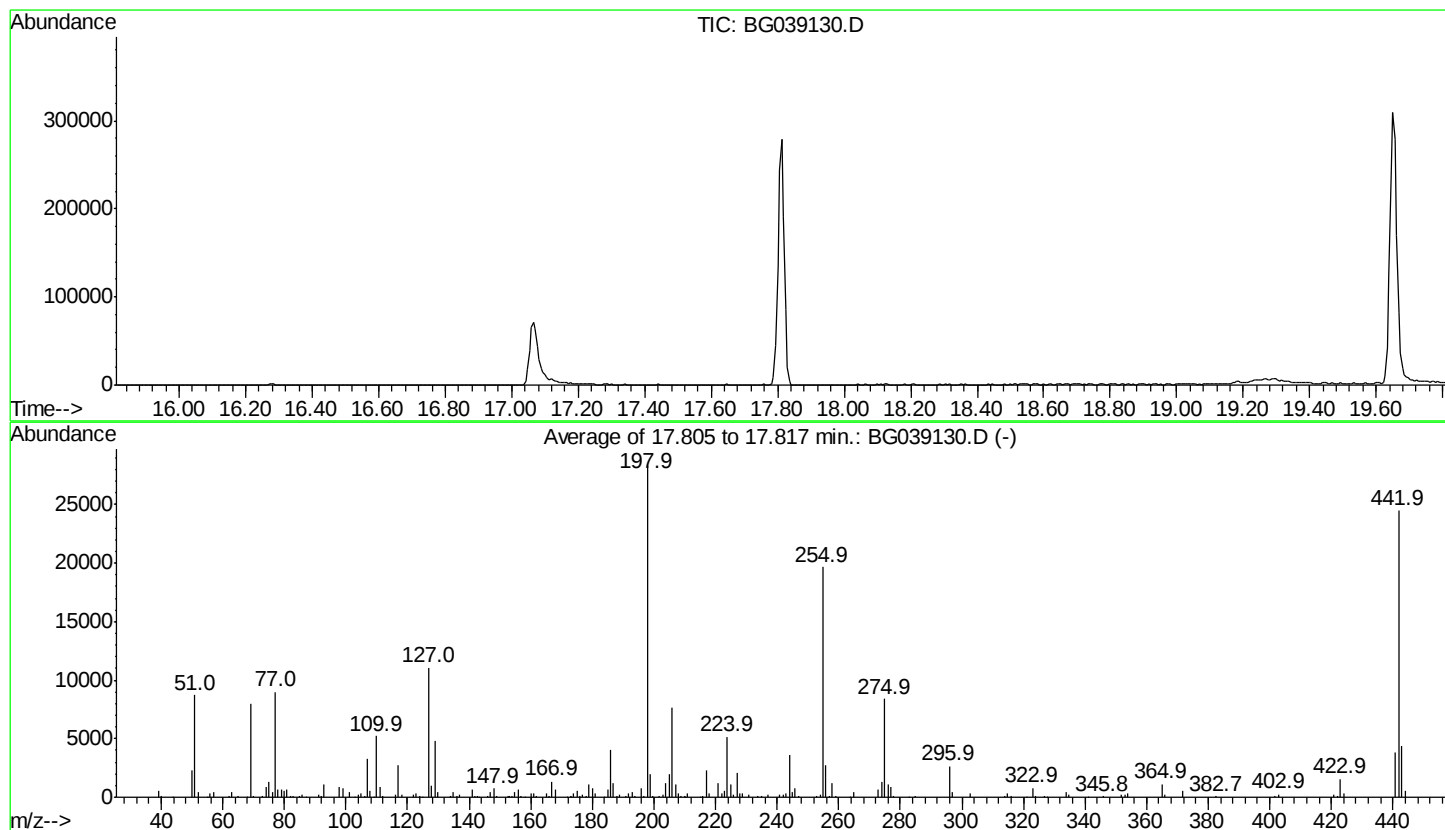

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	8697	PASS
68	69	0.00	2	0.7	58	PASS
69	198	0.00	100	28.4	8039	PASS
70	69	0.00	2	0.7	59	PASS
127	198	10	80	39.1	11089	PASS
197	198	0.00	2	0.4	117	PASS
198	198	100	100	100.0	28328	PASS
199	198	5	9	7.1	2015	PASS
275	198	10	60	29.7	8403	PASS
365	198	1	100	4.0	1142	PASS
441	198	0.01	100	13.4	3804	PASS
442	198	50	100	86.3	24453	PASS
443	442	15	24	17.7	4323	PASS