

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051994.D
 Acq On : 15 Jan 2022 13:20
 Operator : CG/JU
 Sample : N1132-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT6

Quant Time: Jan 17 03:59:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.243	152	28244	20.000	ng/u1	0.00
20) Naphthalene-d8	11.087	136	114857	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.887	164	81293	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.637	188	180478	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.954	240	158418	20.000	ng/u1	# 0.00
88) Perylene-d12	25.444	264	164769	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.573	96	3096	3.917	ng/uL	0.00
4) Pyridine-d5	4.002	84	41134	16.741	ng/u1	0.00
7) Phenol-d5	7.386	99	69125	25.006	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.550	67	43149	24.589	ng/u1	0.00
11) 2-Chlorophenol-d4	7.773	132	46805	25.573	ng/u1	0.00
15) 4-Methylphenol-d8	8.942	113	54858	25.529	ng/u1	0.00
21) Nitrobenzene-d5	9.412	128	24549	27.049	ng/u1	0.00
24) 2-Nitrophenol-d4	10.147	143	29201	29.092	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.693	165	51679	26.340	ng/u1	0.00
31) 4-Chloroaniline-d4	11.210	131	59843	21.902	ng/u1	0.00
46) Dimethylphthalate-d6	14.276	166	171495	25.522	ng/u1	0.00
49) Acenaphthylene-d8	14.582	160	217697	26.821	ng/u1	0.00
54) 4-Nitrophenol-d4	15.064	143	30113	26.804	ng/u1	0.00
60) Fluorene-d10	15.880	176	149022	25.437	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.986	200	30232	26.553	ng/u1	0.00
73) Anthracene-d10	17.736	188	231874	27.083	ng/u1	0.00
81) Pyrene-d10	20.016	212	258729	28.378	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.203	264	234913	27.082	ng/u1	0.00
Target Compounds						
8) Phenol	7.415	94	5723	2.028	ng/u1	92
86) Bis(2-ethylhexyl)phtha...	21.819	149	8340	1.580	ng/u1#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051994.D
Acq On : 15 Jan 2022 13:20
Operator : CG/JU
Sample : N1132-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT6

Quant Time: Jan 17 03:59:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration




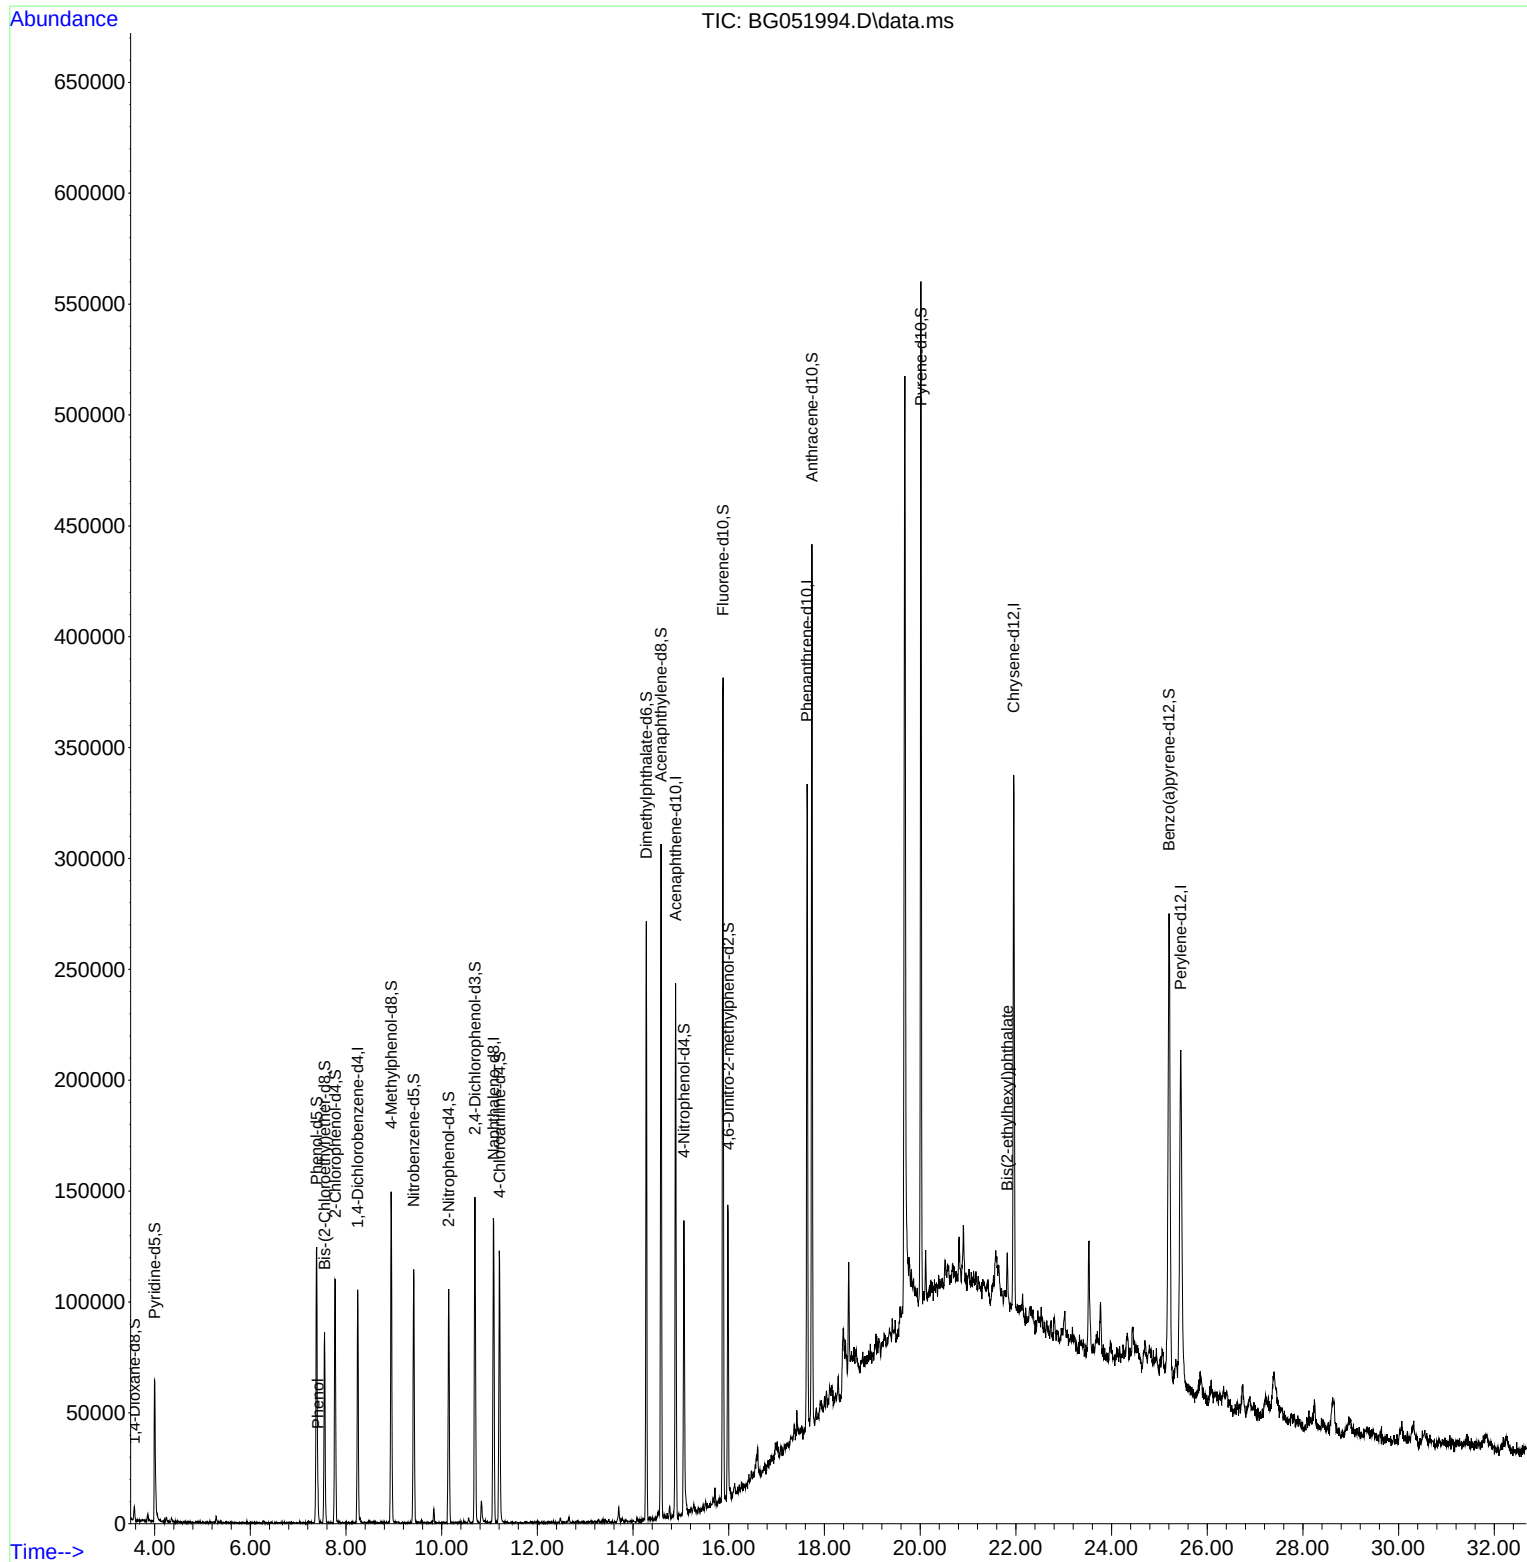


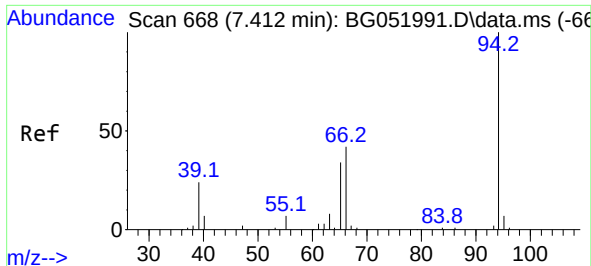

#8
Phenol
Concen: 2.028 ng/ul
RT: 7.415 min Scan# 6
Delta R.T. -0.004 min
Lab File: BG051994.D
Acq: 15 Jan 2022 13:20

Instrument :
BNA_G
ClientSampleId :
BGLT6

Tgt Ion: 94 Resp: 5723
Ion Ratio Lower Upper
94 100
65 35.5 25.1 37.7
66 44.2 31.6 47.4

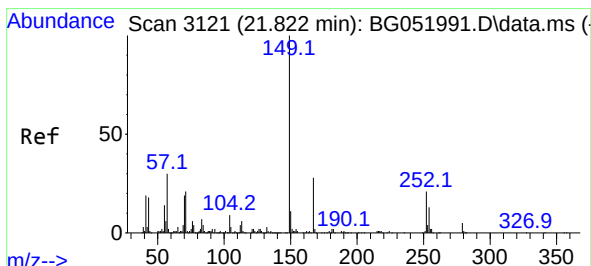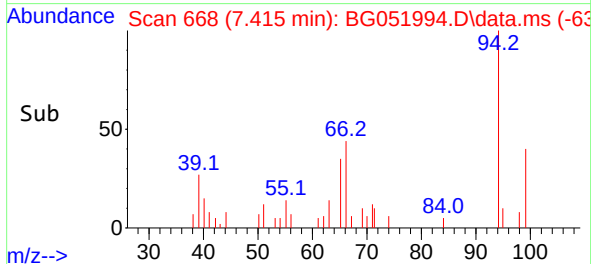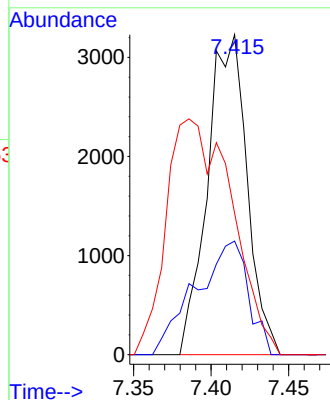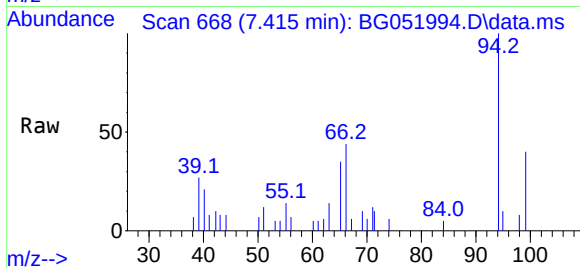

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.580 ng/ul
RT: 21.819 min Scan# 3120
Delta R.T. 0.002 min
Lab File: BG051994.D
Acq: 15 Jan 2022 13:20

Tgt Ion:149 Resp: 8340
Ion Ratio Lower Upper
149 100
167 25.6 21.1 31.7
279 6.7 2.7 4.1#

