

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051995.D
 Acq On : 15 Jan 2022 13:58
 Operator : CG/JU
 Sample : N1132-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT7

Quant Time: Jan 17 03:59:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.241	152	23770	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.084	136	104720	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.885	164	77131	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.634	188	184985	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.952	240	165353	20.000	ng/ul	# 0.00
88) Perylene-d12	25.447	264	167246	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.571	96	2907	4.370	ng/uL	0.00
4) Pyridine-d5	4.000	84	22136	10.705	ng/ul	0.00
7) Phenol-d5	7.383	99	54533	23.440	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	35645	24.136	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.771	132	38842	25.217	ng/ul	0.00
15) 4-Methylphenol-d8	8.946	113	44799	24.771	ng/ul	0.00
21) Nitrobenzene-d5	9.416	128	20977	25.351	ng/ul	0.00
24) 2-Nitrophenol-d4	10.144	143	23873	26.086	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.696	165	43499	24.317	ng/ul	0.00
31) 4-Chloroaniline-d4	11.207	131	58403	23.444	ng/ul	0.00
46) Dimethylphthalate-d6	14.274	166	155794	24.436	ng/ul	0.00
49) Acenaphthylene-d8	14.585	160	192029	24.935	ng/ul	0.00
54) 4-Nitrophenol-d4	15.061	143	23193	21.759	ng/ul	0.00
60) Fluorene-d10	15.878	176	137501	24.736	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.983	200	23968	20.539	ng/ul	0.00
73) Anthracene-d10	17.734	188	234191	26.688	ng/ul	0.00
81) Pyrene-d10	20.013	212	267104	28.068	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.206	264	227973	25.893	ng/ul	0.01
Target Compounds						
					Qvalue	
8) Phenol	7.418	94	4121	1.735	ng/ul	91
86) Bis(2-ethylhexyl)phtha...	21.817	149	6652	1.207	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051995.D
Acq On : 15 Jan 2022 13:58
Operator : CG/JU
Sample : N1132-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT7

Quant Time: Jan 17 03:59:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration




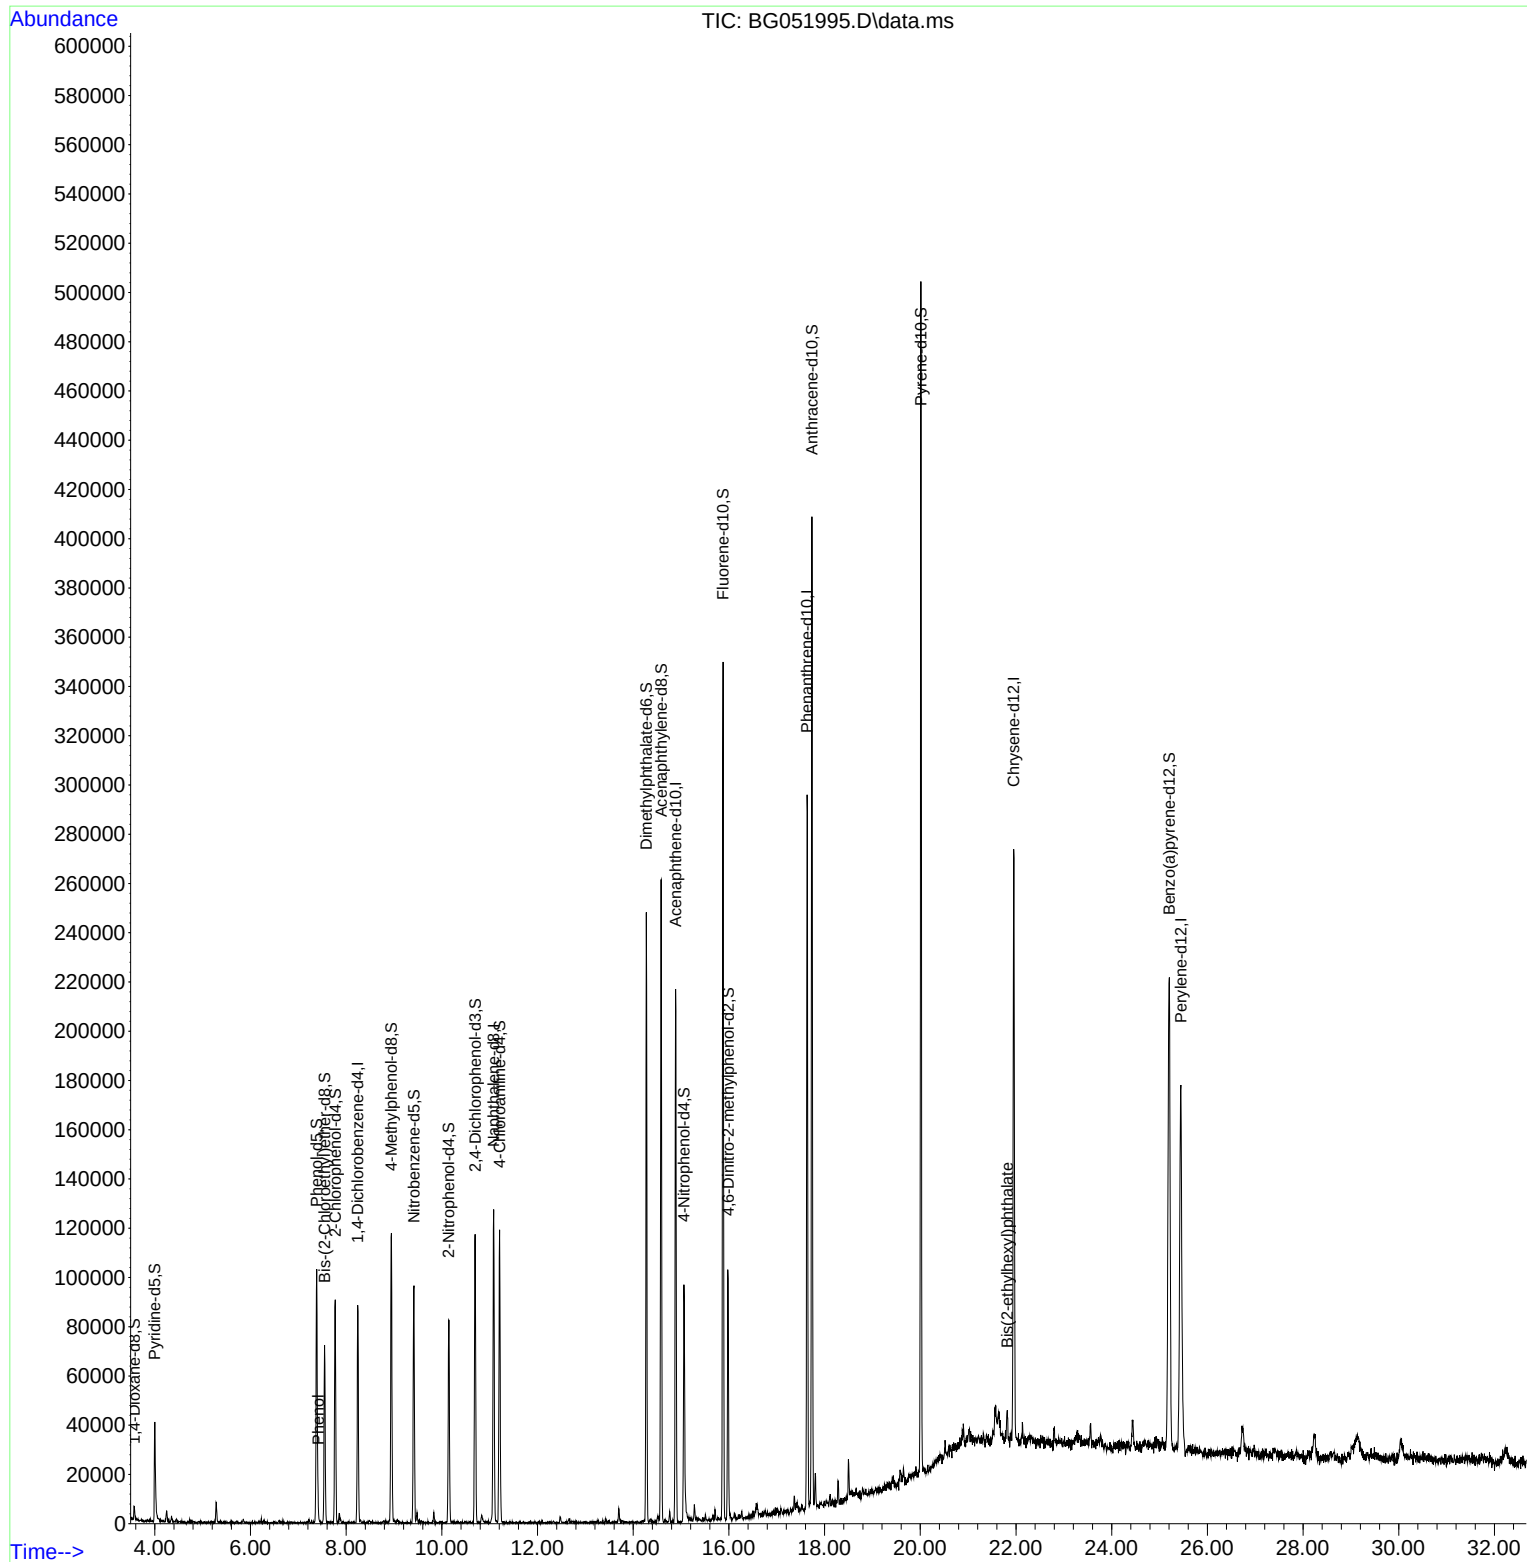


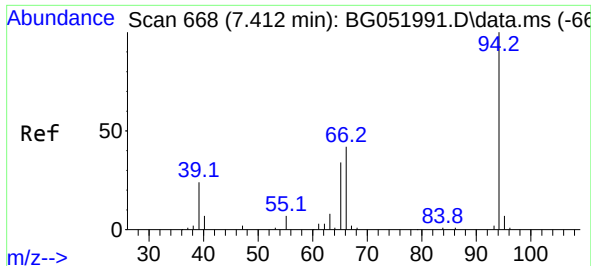

#8
Phenol
Concen: 1.735 ng/ul
RT: 7.418 min Scan# 669
Delta R.T. -0.000 min
Lab File: BG051995.D
Acq: 15 Jan 2022 13:58

Instrument :
BNA_G
ClientSampleId :
BGLT7

Tgt Ion: 94	Resp:	4121
Ion	Ratio	Lower Upper
94	100	
65	26.2	25.1 37.7
66	44.7	31.6 47.4

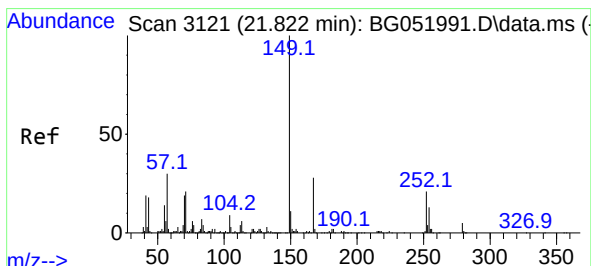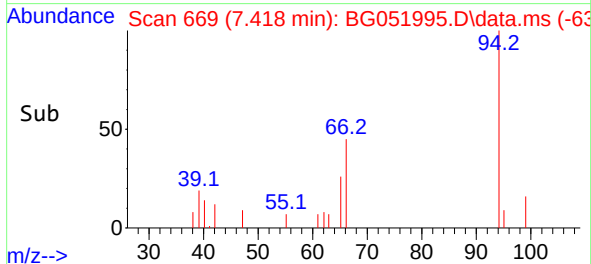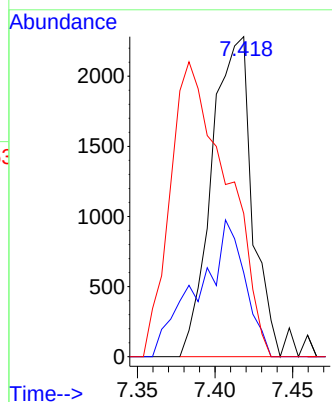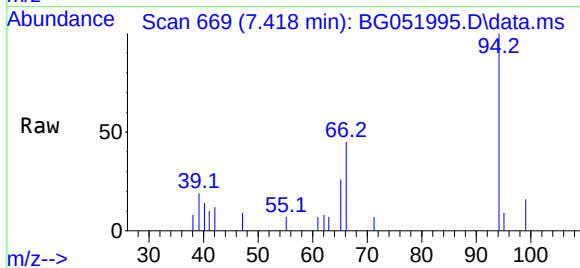

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.207 ng/ul
RT: 21.817 min Scan# 3120
Delta R.T. -0.000 min
Lab File: BG051995.D
Acq: 15 Jan 2022 13:58

Tgt Ion: 149	Resp:	6652
Ion	Ratio	Lower Upper
149	100	
167	22.2	21.1 31.7
279	4.4	2.7 4.1#

