

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051992.D
 Acq On : 15 Jan 2022 12:05
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	9	14	21	rBV	9834	14497	1.29%	0.142%
2	3.993	82	86	95	rBV	112882	193007	17.23%	1.889%
3	4.352	142	147	153	rBV2	8249	12958	1.16%	0.127%
4	4.898	239	240	246	rVB2	745	1175	0.10%	0.012%
5	7.383	656	663	671	rBV	156963	266265	23.78%	2.606%
6	7.553	684	692	700	rBV	104138	178704	15.96%	1.749%
7	7.771	721	729	738	rBV	145739	244411	21.82%	2.392%
8	8.246	802	810	816	rBV	89108	153647	13.72%	1.504%
9	8.945	922	929	936	rBV2	179761	308931	27.59%	3.024%
10	9.415	1001	1009	1016	rVB	145036	251731	22.48%	2.464%
11	10.150	1125	1134	1143	rBV	124495	224141	20.01%	2.194%
12	10.696	1220	1227	1234	rBV	176634	313319	27.98%	3.067%
13	11.084	1285	1293	1300	rBV	130711	228274	20.38%	2.234%
14	11.207	1307	1314	1322	rBV	179052	323083	28.85%	3.163%
15	12.652	1555	1560	1566	rBV3	3122	4594	0.41%	0.045%
16	12.734	1570	1574	1577	rBV2	615	1147	0.10%	0.011%
17	14.279	1830	1837	1845	rVB	374606	552454	49.33%	5.408%
18	14.585	1882	1889	1898	rVB	398949	600733	53.64%	5.880%
19	14.890	1934	1941	1948	rVB	224446	345835	30.88%	3.385%
20	15.067	1963	1971	1985	rBV	185902	322363	28.79%	3.155%
21	15.161	1985	1987	1991	rVV3	1809	2313	0.21%	0.023%
22	15.877	2103	2109	2117	rVB	497789	763535	68.18%	7.474%
23	15.983	2121	2127	2137	rVV	192490	283646	25.33%	2.776%
24	16.059	2138	2140	2146	rVB2	1377	2031	0.18%	0.020%
25	16.112	2146	2149	2153	rBV2	1507	2075	0.19%	0.020%
26	16.512	2216	2217	2222	rBV	942	1213	0.11%	0.012%
27	17.422	2368	2372	2375	rBV4	1374	1896	0.17%	0.019%
28	17.640	2402	2409	2416	rVB	310200	475174	42.43%	4.651%
29	17.739	2419	2426	2433	rBV	628822	946027	84.48%	9.260%
30	17.863	2443	2447	2449	rBV	852	1212	0.11%	0.012%
31	18.474	2548	2551	2553	rVB2	1123	1157	0.10%	0.011%
32	18.568	2565	2567	2573	rBV3	1231	1916	0.17%	0.019%
33	18.644	2577	2580	2584	rBV2	743	1183	0.11%	0.012%
34	18.855	2614	2616	2620	rVB	1009	1428	0.13%	0.014%
35	18.914	2620	2626	2627	rBV3	870	1236	0.11%	0.012%
36	18.949	2630	2632	2635	rVV4	1570	1767	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051992.D
 Acq On : 15 Jan 2022 12:05
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.008	2639	2642	2643	rVB3	1371	1132	0.10%	0.011%
38	19.220	2676	2678	2681	rVV3	1425	1919	0.17%	0.019%
39	19.255	2683	2684	2687	rVV	1372	1209	0.11%	0.012%
40	19.296	2687	2691	2694	rVB4	2534	3637	0.32%	0.036%
41	19.367	2699	2703	2706	rBV3	1128	1298	0.12%	0.013%
42	19.390	2706	2707	2710	rBV3	1398	1384	0.12%	0.014%
43	19.490	2722	2724	2727	rBV2	1724	2250	0.20%	0.022%
44	19.584	2736	2740	2744	rVB4	9724	14331	1.28%	0.140%
45	19.649	2747	2751	2757	rBV	9628	15532	1.39%	0.152%
46	19.725	2763	2764	2766	rBV2	2363	1841	0.16%	0.018%
47	19.754	2766	2769	2770	rVV3	2227	1968	0.18%	0.019%
48	19.784	2773	2774	2776	rBV2	1472	1159	0.10%	0.011%
49	19.901	2792	2794	2797	rBV4	2373	3286	0.29%	0.032%
50	20.019	2807	2814	2820	rBV	767709	1119872	100.00%	10.962%
51	20.066	2820	2822	2824	rVB2	1347	1199	0.11%	0.012%
52	20.148	2833	2836	2838	rBV4	2653	2433	0.22%	0.024%
53	20.171	2838	2840	2841	rVV3	1554	1369	0.12%	0.013%
54	20.189	2841	2843	2846	rVV4	2175	2379	0.21%	0.023%
55	20.224	2846	2849	2852	rVB4	2372	2820	0.25%	0.028%
56	20.259	2852	2855	2856	rBV3	2322	2709	0.24%	0.027%
57	20.342	2868	2869	2871	rBV	2402	2054	0.18%	0.020%
58	20.553	2903	2905	2906	rBV2	2452	1954	0.17%	0.019%
59	21.393	3046	3048	3050	rBV3	3400	2615	0.23%	0.026%
60	21.575	3077	3079	3080	rBV2	4213	2617	0.23%	0.026%
61	21.646	3089	3091	3095	rVB5	7281	9547	0.85%	0.093%
62	21.957	3138	3144	3151	rVB	281402	476778	42.57%	4.667%
63	22.045	3158	3159	3162	rBV3	3516	2154	0.19%	0.021%
64	22.145	3175	3176	3177	rBV	4435	2065	0.18%	0.020%
65	22.733	3273	3276	3279	rBV5	4215	6057	0.54%	0.059%
66	22.780	3282	3284	3285	rBV	4232	2966	0.26%	0.029%
67	23.026	3324	3326	3329	rBV3	3975	4838	0.43%	0.047%
68	23.226	3358	3360	3361	rBV2	3558	1889	0.17%	0.018%
69	23.661	3430	3434	3437	rBV6	3532	5838	0.52%	0.057%
70	24.847	3634	3636	3639	rBV4	4562	4533	0.40%	0.044%
71	25.206	3686	3697	3710	rVB2	325826	962500	85.95%	9.422%
72	25.447	3727	3738	3753	rVB2	150437	485328	43.34%	4.751%
73	25.746	3787	3789	3790	rBV2	4529	3017	0.27%	0.030%
74	26.169	3859	3861	3862	rBV2	3621	2860	0.26%	0.028%
75	26.821	3970	3972	3975	rVB4	4097	3042	0.27%	0.030%
76	27.232	4040	4042	4044	rBV3	3460	2432	0.22%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051992.D
Acq On : 15 Jan 2022 12:05
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	27.649	4111	4113	4114	rBV2	3748	1767	0.16%	0.017%
78	28.689	4288	4290	4292	rBV3	4331	3395	0.30%	0.033%
79	29.071	4353	4355	4358	rBV4	3900	4003	0.36%	0.039%
80	31.174	4711	4713	4715	rBV3	4235	3089	0.28%	0.030%
81	32.026	4856	4858	4863	rBV5	3233	4028	0.36%	0.039%
82	32.408	4922	4923	4924	rBV	4028	1817	0.16%	0.018%




Sum of corrected areas: 10215988

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051992.D
Acq On : 15 Jan 2022 12:05
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

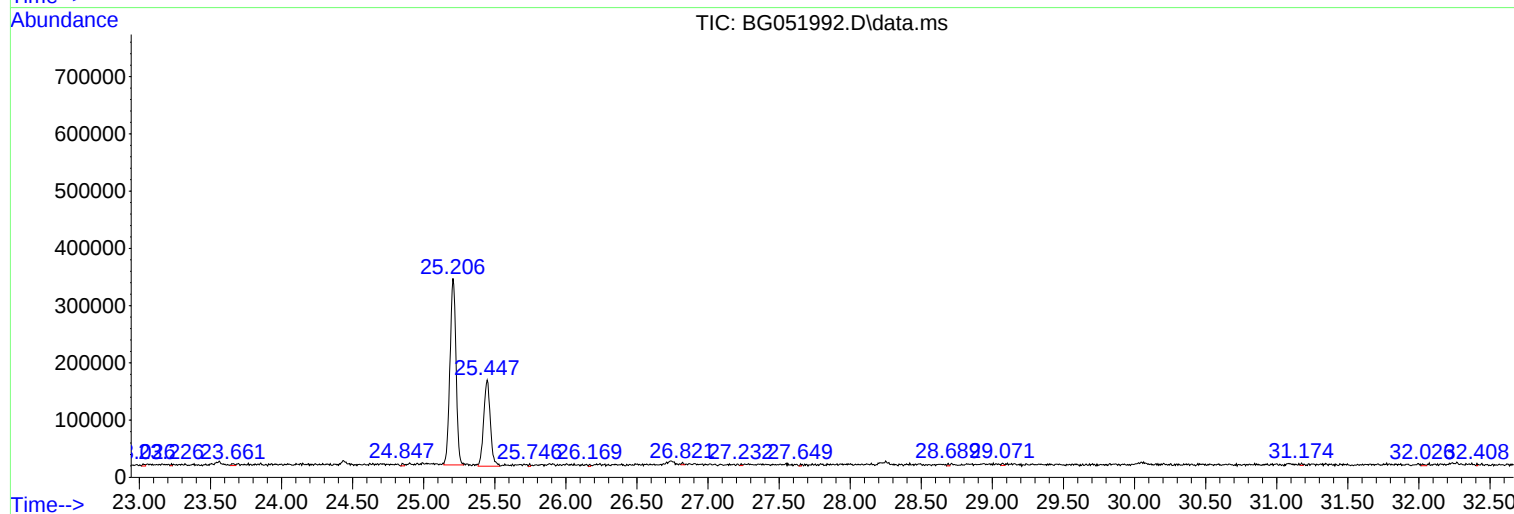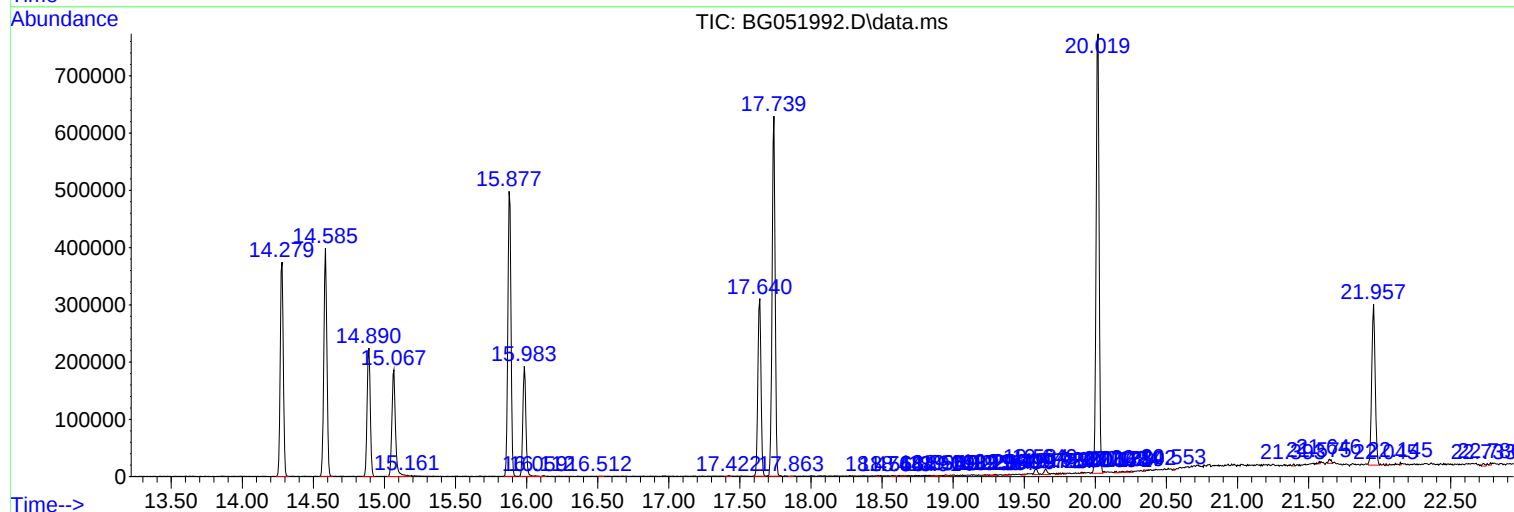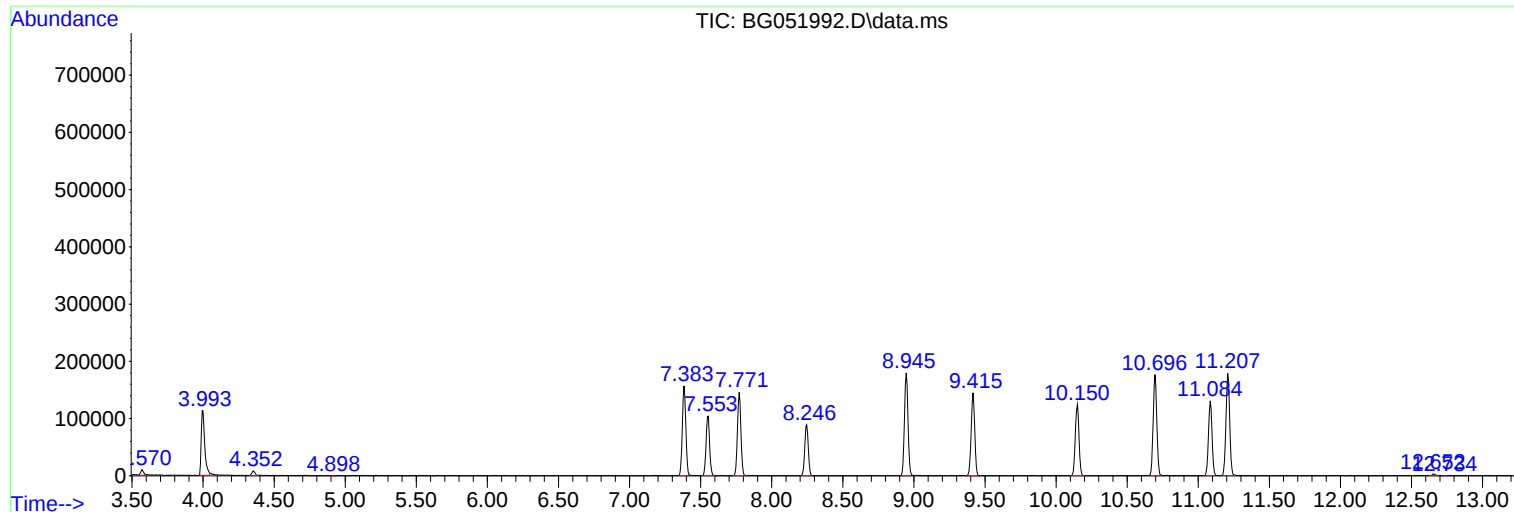

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051992.D
Acq On : 15 Jan 2022 12:05
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051992.D
Acq On : 15 Jan 2022 12:05
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc