

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051995.D
 Acq On : 15 Jan 2022 13:58
 Operator : CG/JU
 Sample : N1132-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.565	9	13	18	rBV2	5540	7837	1.15%	0.107%
2	3.718	37	39	42	rVB2	1141	971	0.14%	0.013%
3	3.906	67	71	74	rBV2	1241	1351	0.20%	0.018%
4	4.000	82	87	104	rBV	40641	73111	10.77%	0.998%
5	4.246	125	129	132	rBV3	4035	5686	0.84%	0.078%
6	4.352	142	147	150	rBV3	2299	3034	0.45%	0.041%
7	4.452	159	164	166	rBB2	1332	1862	0.27%	0.025%
8	4.687	200	204	208	rBV	973	1965	0.29%	0.027%
9	4.728	210	211	215	rVB2	1696	1423	0.21%	0.019%
10	5.280	301	305	313	rVB	8361	12768	1.88%	0.174%
11	5.715	375	379	382	rBV2	982	1246	0.18%	0.017%
12	5.850	397	402	405	rBV2	1389	1879	0.28%	0.026%
13	6.226	463	466	469	rVB2	1989	1855	0.27%	0.025%
14	6.279	471	475	476	rBV2	1046	1141	0.17%	0.016%
15	6.602	524	530	532	rVB	1148	1398	0.21%	0.019%
16	7.125	616	619	622	rBV	722	966	0.14%	0.013%
17	7.225	632	636	640	rVB	1637	2052	0.30%	0.028%
18	7.277	641	645	647	rBV	1182	1206	0.18%	0.016%
19	7.383	655	663	677	rVB	103212	190991	28.13%	2.607%
20	7.548	682	691	698	rBV	72581	120875	17.80%	1.650%
21	7.771	722	729	736	rBV	90769	159373	23.47%	2.175%
22	7.853	738	743	746	rBV3	4018	6255	0.92%	0.085%
23	8.241	803	809	816	rBV	88347	151490	22.31%	2.068%
24	8.300	816	819	823	rVB2	1195	1592	0.23%	0.022%
25	8.488	847	851	855	rVB2	1091	1937	0.29%	0.026%
26	8.946	923	929	936	rVB	117033	206257	30.37%	2.815%
27	9.069	947	950	956	rVB2	1668	3155	0.46%	0.043%
28	9.122	956	959	961	rBV	857	1024	0.15%	0.014%
29	9.416	1002	1009	1015	rBV	96336	173013	25.48%	2.362%
30	9.480	1016	1020	1025	rVB5	4440	6407	0.94%	0.087%
31	9.527	1025	1028	1032	rBV2	1591	2119	0.31%	0.029%
32	9.568	1032	1035	1039	rBV2	1093	1728	0.25%	0.024%
33	9.833	1075	1080	1086	rVB4	4617	7489	1.10%	0.102%
34	9.886	1086	1089	1092	rBV	813	1001	0.15%	0.014%
35	10.144	1127	1133	1142	rVB	82411	151513	22.31%	2.068%
36	10.485	1186	1191	1195	rBV2	766	1292	0.19%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051995.D
 Acq On : 15 Jan 2022 13:58
 Operator : CG/JU
 Sample : N1132-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	10.696	1220	1227	1234	rBV	117420	210808	31.04%	2.877%
38	10.831	1246	1250	1259	rBV5	3256	7376	1.09%	0.101%
39	11.084	1280	1293	1300	rBV	127415	233305	34.36%	3.185%
40	11.207	1306	1314	1323	rBV	118912	211064	31.08%	2.881%
41	11.860	1422	1425	1428	rVB	893	960	0.14%	0.013%
42	12.030	1450	1454	1455	rBV2	803	974	0.14%	0.013%
43	12.094	1461	1465	1468	rBV2	1599	2163	0.32%	0.030%
44	12.312	1499	1502	1504	rBV2	700	1026	0.15%	0.014%
45	12.470	1525	1529	1536	rBV3	2643	4436	0.65%	0.061%
46	12.664	1559	1562	1564	rVB	1729	1651	0.24%	0.023%
47	12.723	1569	1572	1576	rVB2	860	1254	0.18%	0.017%
48	13.322	1668	1674	1676	rBV2	714	998	0.15%	0.014%
49	13.416	1687	1690	1692	rBV2	2039	1957	0.29%	0.027%
50	13.493	1698	1703	1706	rVB4	809	1229	0.18%	0.017%
51	13.698	1733	1738	1743	rBV3	5570	8003	1.18%	0.109%
52	13.945	1776	1780	1783	rBV2	692	1340	0.20%	0.018%
53	14.192	1820	1822	1826	rBV3	1001	1512	0.22%	0.021%
54	14.274	1830	1836	1844	rVB	247842	352826	51.96%	4.816%
55	14.362	1847	1851	1853	rVB2	1364	1844	0.27%	0.025%
56	14.468	1867	1869	1872	rBV2	1025	1072	0.16%	0.015%
57	14.515	1872	1877	1878	rBV2	2922	3985	0.59%	0.054%
58	14.585	1882	1889	1897	rVB	261106	414335	61.02%	5.656%
59	14.656	1897	1901	1903	rBV	1114	1058	0.16%	0.014%
60	14.761	1915	1919	1923	rVB3	4593	6393	0.94%	0.087%
61	14.885	1933	1940	1947	rBV	216786	348880	51.38%	4.762%
62	15.061	1963	1970	1983	rBV2	96321	177659	26.16%	2.425%
63	15.226	1996	1998	2001	rVB	1211	1100	0.16%	0.015%
64	15.278	2001	2007	2011	rBV4	6909	10454	1.54%	0.143%
65	15.455	2034	2037	2038	rVB3	1669	996	0.15%	0.014%
66	15.508	2044	2046	2050	rBV2	2418	2501	0.37%	0.034%
67	15.648	2067	2070	2071	rBV2	1163	1256	0.18%	0.017%
68	15.672	2073	2074	2076	rVV	2228	1627	0.24%	0.022%
69	15.707	2078	2080	2086	rVV4	4509	5493	0.81%	0.075%
70	15.784	2090	2093	2097	rVV4	1136	1230	0.18%	0.017%
71	15.878	2103	2109	2116	rBV	348250	516479	76.06%	7.050%
72	15.977	2121	2126	2134	rVV	100621	155380	22.88%	2.121%
73	16.113	2147	2149	2153	rVB2	2403	2896	0.43%	0.040%
74	16.271	2173	2176	2182	rVB3	3576	5392	0.79%	0.074%
75	16.324	2182	2185	2188	rBV3	982	1629	0.24%	0.022%
76	16.406	2197	2199	2202	rBV3	1522	1195	0.18%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051995.D
 Acq On : 15 Jan 2022 13:58
 Operator : CG/JU
 Sample : N1132-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	16.471	2208	2210	2212	rVB2	1507	1185	0.17%	0.016%
78	16.506	2212	2216	2219	rBV4	2976	3148	0.46%	0.043%
79	16.571	2219	2227	2230	rBV6	5562	11503	1.69%	0.157%
80	16.700	2247	2249	2250	rVB2	2292	1298	0.19%	0.018%
81	16.718	2250	2252	2254	rBV3	1592	1140	0.17%	0.016%
82	16.894	2280	2282	2284	rBV3	1409	1197	0.18%	0.016%
83	17.005	2299	2301	2303	rBV3	2249	1484	0.22%	0.020%
84	17.064	2307	2311	2312	rBV4	1528	1912	0.28%	0.026%
85	17.364	2359	2362	2367	rBV6	5983	7805	1.15%	0.107%
86	17.399	2367	2368	2369	rBV	2579	1190	0.18%	0.016%
87	17.634	2402	2408	2415	rBV	289829	449115	66.14%	6.130%
88	17.734	2419	2425	2432	rVV	402355	601002	88.50%	8.204%
89	17.804	2433	2437	2443	rVB8	13658	20110	2.96%	0.274%
90	18.280	2515	2518	2523	rVB5	9608	13378	1.97%	0.183%
91	18.498	2552	2555	2560	rVB3	14561	17590	2.59%	0.240%
92	20.013	2807	2813	2820	rBV	483542	679065	100.00%	9.269%
93	21.952	3137	3143	3151	rVB	238857	436297	64.25%	5.955%
94	25.206	3687	3697	3707	rVB3	190465	584043	86.01%	7.972%
95	25.447	3730	3738	3753	rVB2	150974	478672	70.49%	6.534%




Sum of corrected areas: 7326132

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051995.D
Acq On : 15 Jan 2022 13:58
Operator : CG/JU
Sample : N1132-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

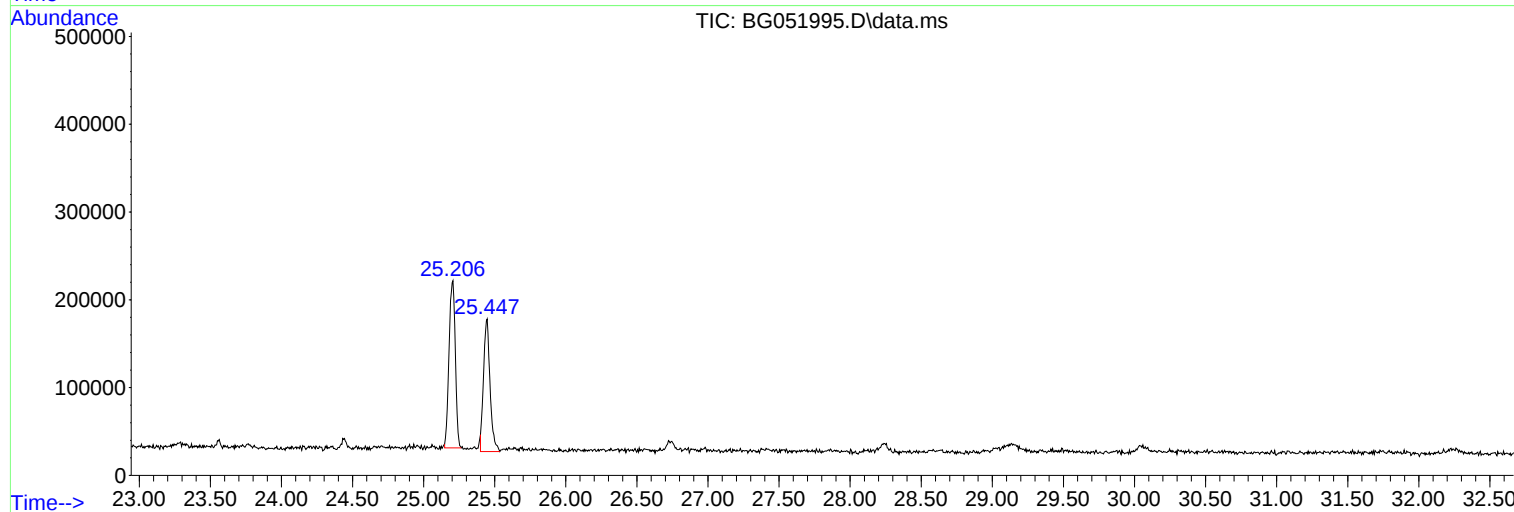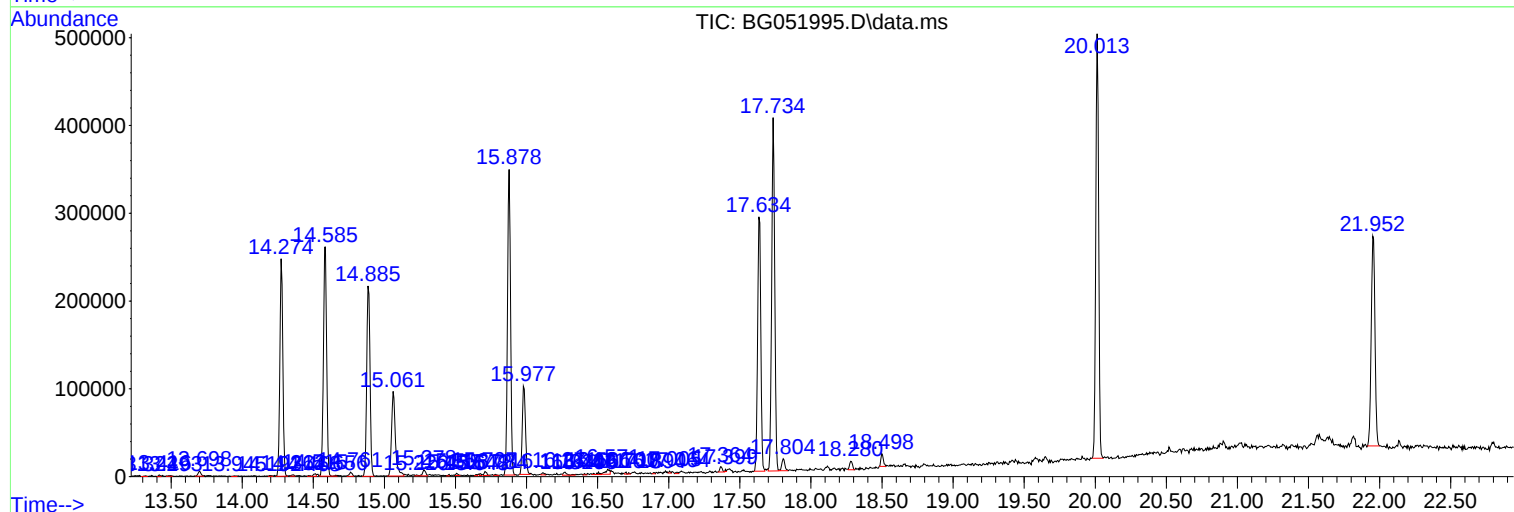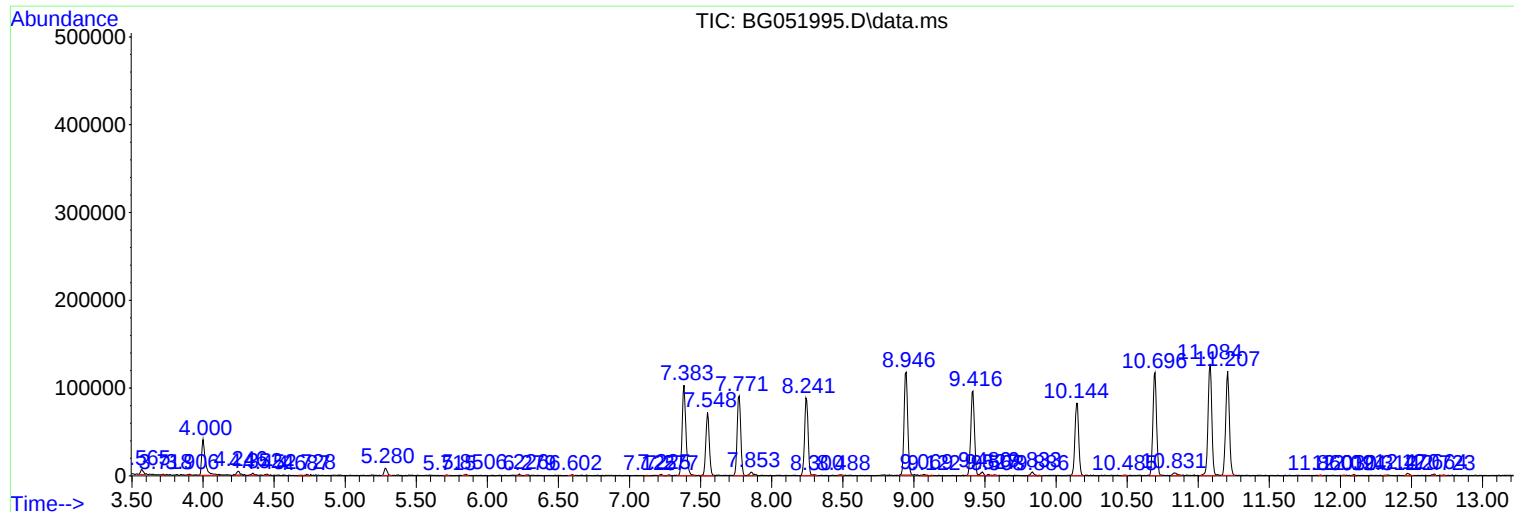

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051995.D
Acq On : 15 Jan 2022 13:58
Operator : CG/JU
Sample : N1132-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051995.D
Acq On : 15 Jan 2022 13:58
Operator : CG/JU
Sample : N1132-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc