

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051997.D
 Acq On : 15 Jan 2022 15:13
 Operator : CG/JU
 Sample : N1132-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	20	rVB3	5441	9250	1.23%	0.116%
2	3.999	83	87	101	rBV	54229	93197	12.40%	1.165%
3	4.205	119	122	125	rBV2	1370	1674	0.22%	0.021%
4	4.252	128	130	134	rVB2	1823	1639	0.22%	0.020%
5	4.346	145	146	149	rBV	2223	1698	0.23%	0.021%
6	4.534	176	178	182	rVB	983	1311	0.17%	0.016%
7	5.286	302	306	313	rBV2	2140	4042	0.54%	0.051%
8	6.984	591	595	597	rBV2	888	1112	0.15%	0.014%
9	7.383	654	663	672	rBV	119848	210217	27.98%	2.628%
10	7.547	685	691	700	rBV	78748	132648	17.66%	1.658%
11	7.771	722	729	736	rVB	102468	177023	23.56%	2.213%
12	8.247	802	810	815	rBV	103953	174998	23.29%	2.188%
13	8.293	815	818	826	rVB2	1730	2920	0.39%	0.037%
14	8.946	922	929	938	rVB	131956	229126	30.50%	2.865%
15	9.415	1000	1009	1016	rBV	103239	190464	25.35%	2.381%
16	9.568	1033	1035	1039	rVB	843	1070	0.14%	0.013%
17	9.833	1077	1080	1086	rVB2	5319	7434	0.99%	0.093%
18	10.144	1126	1133	1143	rVB2	88672	161572	21.51%	2.020%
19	10.690	1219	1226	1234	rBV	128389	236087	31.42%	2.952%
20	10.831	1243	1250	1257	rBV3	12028	23173	3.08%	0.290%
21	11.084	1285	1293	1301	rVB	143858	265091	35.28%	3.314%
22	11.207	1307	1314	1321	rBV	117002	211176	28.11%	2.640%
23	12.476	1525	1530	1535	rBV3	1722	2520	0.34%	0.032%
24	12.658	1557	1561	1564	rBV2	1889	2350	0.31%	0.029%
25	13.481	1697	1701	1706	rBV2	1718	3211	0.43%	0.040%
26	13.704	1734	1739	1744	rBV3	3901	6738	0.90%	0.084%
27	13.768	1744	1750	1755	rBV3	1084	1872	0.25%	0.023%
28	14.092	1800	1805	1808	rBV3	1731	2398	0.32%	0.030%
29	14.274	1830	1836	1844	rBV	241300	362672	48.27%	4.534%
30	14.503	1872	1875	1878	rBV4	2728	3428	0.46%	0.043%
31	14.585	1882	1889	1896	rVB	280144	450570	59.97%	5.633%
32	14.761	1915	1919	1924	rVB4	2517	3337	0.44%	0.042%
33	14.890	1933	1941	1947	rBV	252576	391957	52.17%	4.900%
34	15.061	1963	1970	1981	rBV	104071	190141	25.31%	2.377%
35	15.284	2005	2008	2011	rVB2	1606	1493	0.20%	0.019%
36	15.672	2069	2074	2077	rBV5	2774	4880	0.65%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
 Data File : BG051997.D
 Acq On : 15 Jan 2022 15:13
 Operator : CG/JU
 Sample : N1132-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.713	2077	2081	2086	rVB2	2862	3748	0.50%	0.047%
38	15.877	2102	2109	2116	rVB	363904	563416	74.99%	7.044%
39	15.983	2121	2127	2133	rBV	101871	153074	20.37%	1.914%
40	16.118	2146	2150	2154	rVB3	1681	2602	0.35%	0.033%
41	16.265	2169	2175	2181	rBV3	4007	6111	0.81%	0.076%
42	16.312	2181	2183	2185	rBV	1273	1126	0.15%	0.014%
43	16.506	2213	2216	2219	rBV3	1763	2655	0.35%	0.033%
44	16.547	2219	2223	2225	rBV3	2312	3401	0.45%	0.043%
45	16.618	2234	2235	2238	rVB	1950	1365	0.18%	0.017%
46	16.653	2238	2241	2247	rBV5	1715	2542	0.34%	0.032%
47	16.753	2255	2258	2262	rVB3	2748	3172	0.42%	0.040%
48	16.858	2275	2276	2279	rVB2	1606	1026	0.14%	0.013%
49	16.929	2282	2288	2289	rBV3	1601	2475	0.33%	0.031%
50	16.982	2294	2297	2300	rBV4	1734	2347	0.31%	0.029%
51	17.146	2322	2325	2327	rBV2	1218	1640	0.22%	0.021%
52	17.223	2336	2338	2340	rBV2	1380	1092	0.15%	0.014%
53	17.364	2359	2362	2367	rVB	4551	4594	0.61%	0.057%
54	17.422	2367	2372	2375	rBV2	2265	3632	0.48%	0.045%
55	17.522	2387	2389	2393	rVB5	3297	4100	0.55%	0.051%
56	17.563	2393	2396	2398	rBV2	1092	1105	0.15%	0.014%
57	17.640	2402	2409	2415	rVV	333428	514815	68.52%	6.436%
58	17.734	2419	2425	2434	rVV2	422249	640660	85.27%	8.010%
59	17.804	2434	2437	2443	rVB5	7234	8749	1.16%	0.109%
60	18.110	2487	2489	2491	rVB2	2048	1383	0.18%	0.017%
61	18.221	2505	2508	2509	rBV2	1449	1435	0.19%	0.018%
62	18.245	2509	2512	2514	rVV3	1447	1429	0.19%	0.018%
63	18.280	2514	2518	2525	rVB3	10778	15089	2.01%	0.189%
64	18.503	2553	2556	2559	rBV3	3512	4810	0.64%	0.060%
65	18.556	2563	2565	2567	rBV3	1528	1419	0.19%	0.018%
66	18.650	2579	2581	2585	rBV4	1373	1127	0.15%	0.014%
67	18.797	2602	2606	2609	rBV5	3825	4273	0.57%	0.053%
68	18.826	2609	2611	2613	rBV3	1566	1484	0.20%	0.019%
69	18.956	2632	2633	2635	rBV2	1810	1434	0.19%	0.018%
70	19.179	2670	2671	2673	rBV2	2140	1448	0.19%	0.018%
71	19.355	2698	2701	2704	rBV5	2511	4053	0.54%	0.051%
72	19.502	2724	2726	2728	rVB3	2467	1302	0.17%	0.016%
73	19.578	2737	2739	2743	rVB3	4077	4210	0.56%	0.053%
74	19.643	2748	2750	2757	rVB4	5408	9533	1.27%	0.119%
75	20.013	2807	2813	2819	rBV	526888	751304	100.00%	9.393%
76	20.230	2848	2850	2852	rBV3	2687	1878	0.25%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051997.D
Acq On : 15 Jan 2022 15:13
Operator : CG/JU
Sample : N1132-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	21.957	3137	3144	3152	rVB	310415	525125	69.90%	6.565%
78	25.200	3687	3696	3709	rVB2	216979	641511	85.39%	8.020%
79	25.441	3728	3737	3751	rVB3	164553	530371	70.59%	6.631%




Sum of corrected areas: 7998554

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051997.D
Acq On : 15 Jan 2022 15:13
Operator : CG/JU
Sample : N1132-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

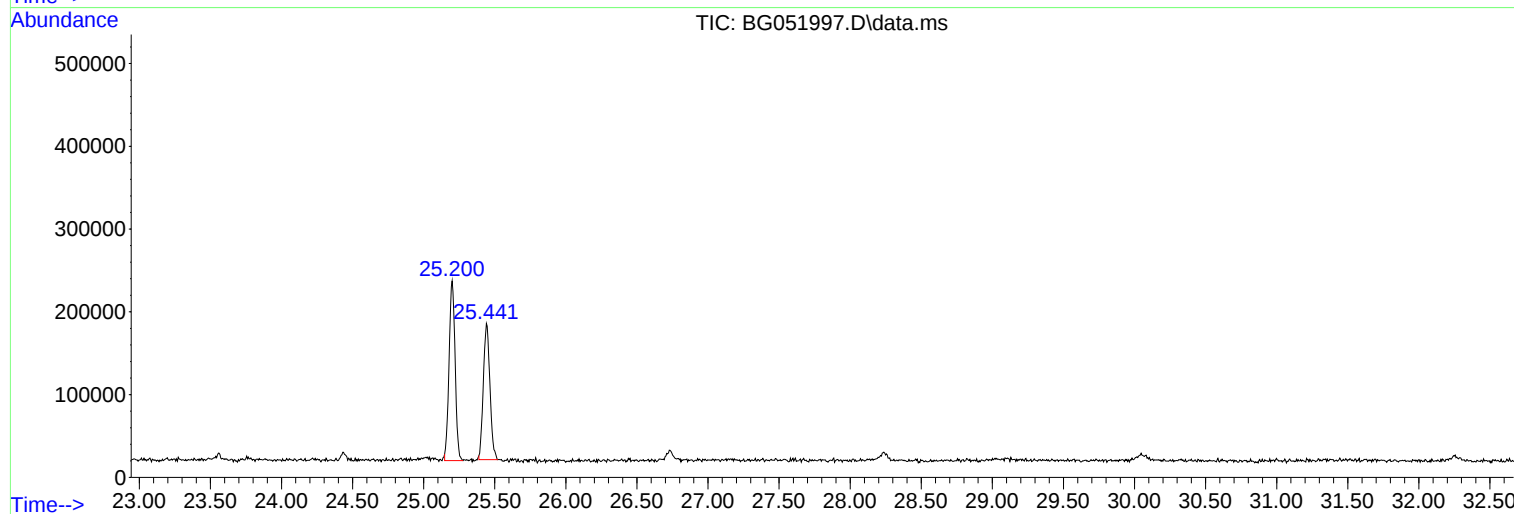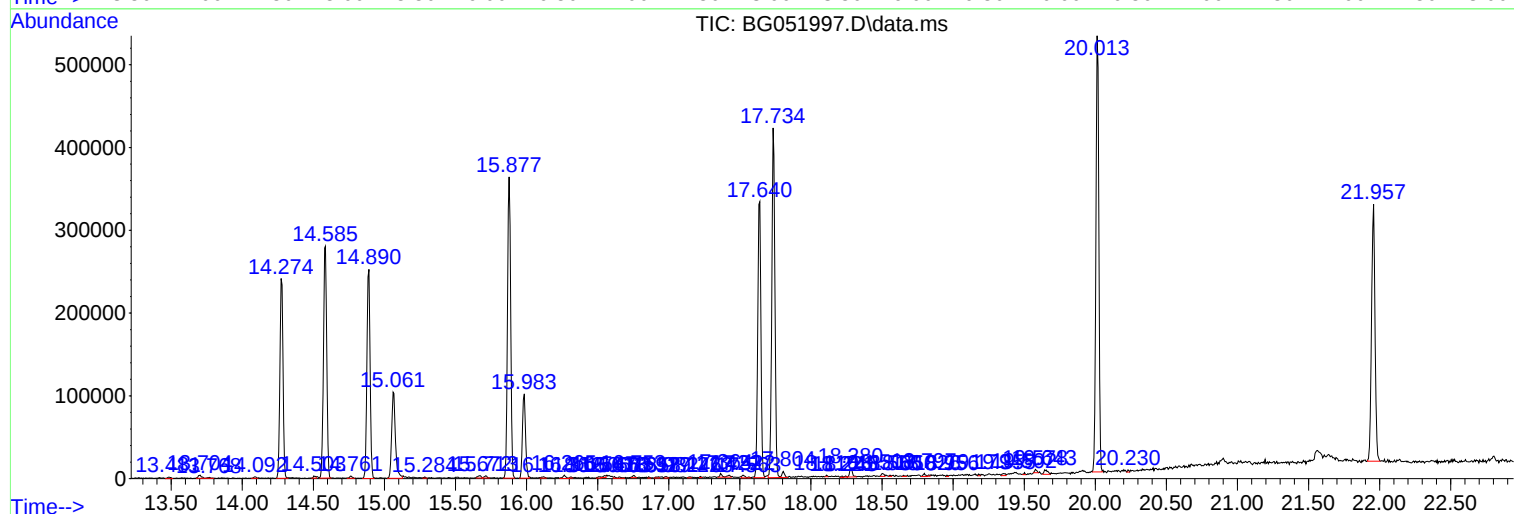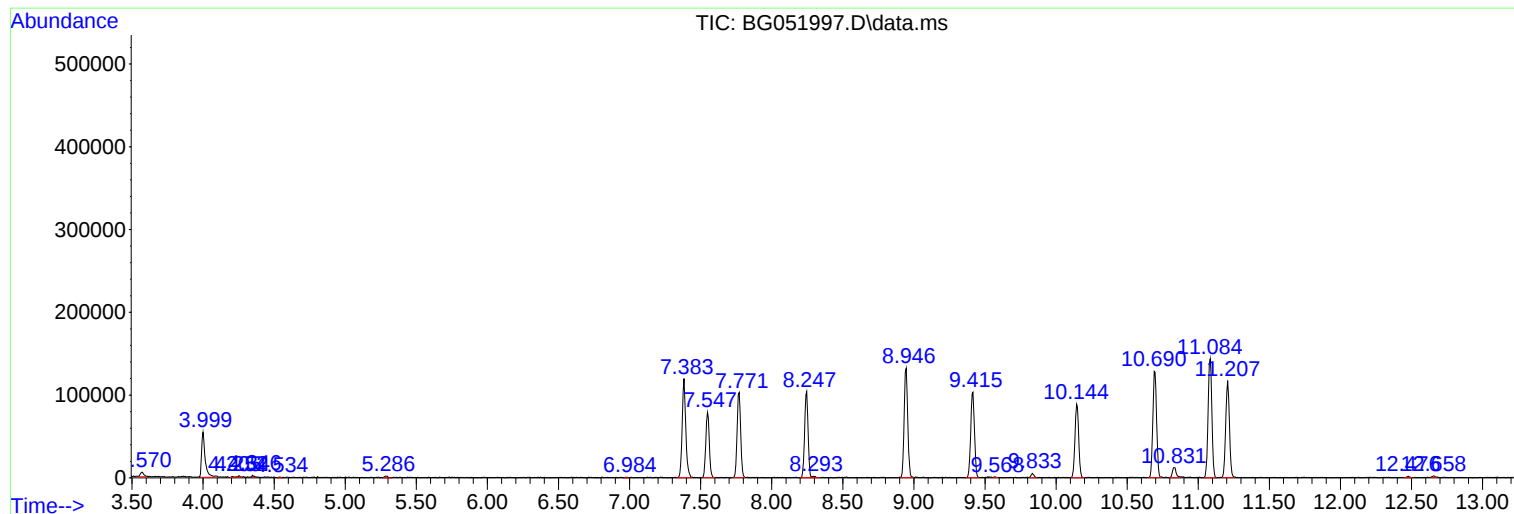

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051997.D
Acq On : 15 Jan 2022 15:13
Operator : CG/JU
Sample : N1132-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011522\
Data File : BG051997.D
Acq On : 15 Jan 2022 15:13
Operator : CG/JU
Sample : N1132-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc