

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011619\
 Data File : BG039174.D
 Acq On : 17 Jan 2019 2:14
 Operator : JU/SJ
 Sample : K1010-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-01-011519-B

Quant Time: Jan 17 05:39:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 09 14:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	19561	20.00	ng	-0.02
21) Naphthalene-d8	10.83	136	85219	20.00	ng	-0.01
39) Acenaphthene-d10	14.66	164	82630	20.00	ng	-0.01
64) Phenanthrene-d10	17.41	188	161278	20.00	ng	-0.01
76) Chrysene-d12	21.68	240	184278	20.00	ng	-0.02
87) Perylene-d12	24.94	264	181084	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	157966	153.19	ng	-0.01
7) Phenol-d6	7.18	99	221794	149.46	ng	-0.01
23) Nitrobenzene-d5	9.19	82	166822	107.12	ng	-0.02
42) 2,4,6-Tribromophenol	16.15	330	158615	114.51	ng	-0.02
45) 2-Fluorobiphenyl	13.28	172	422217	69.93	ng	-0.01
79) Terphenyl-d14	20.01	244	954765	95.84	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011619\
Data File : BG039174.D
Acq On : 17 Jan 2019 2:14
Operator : JU/SJ
Sample : K1010-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-01-011519-B

Quant Time: Jan 17 05:39:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

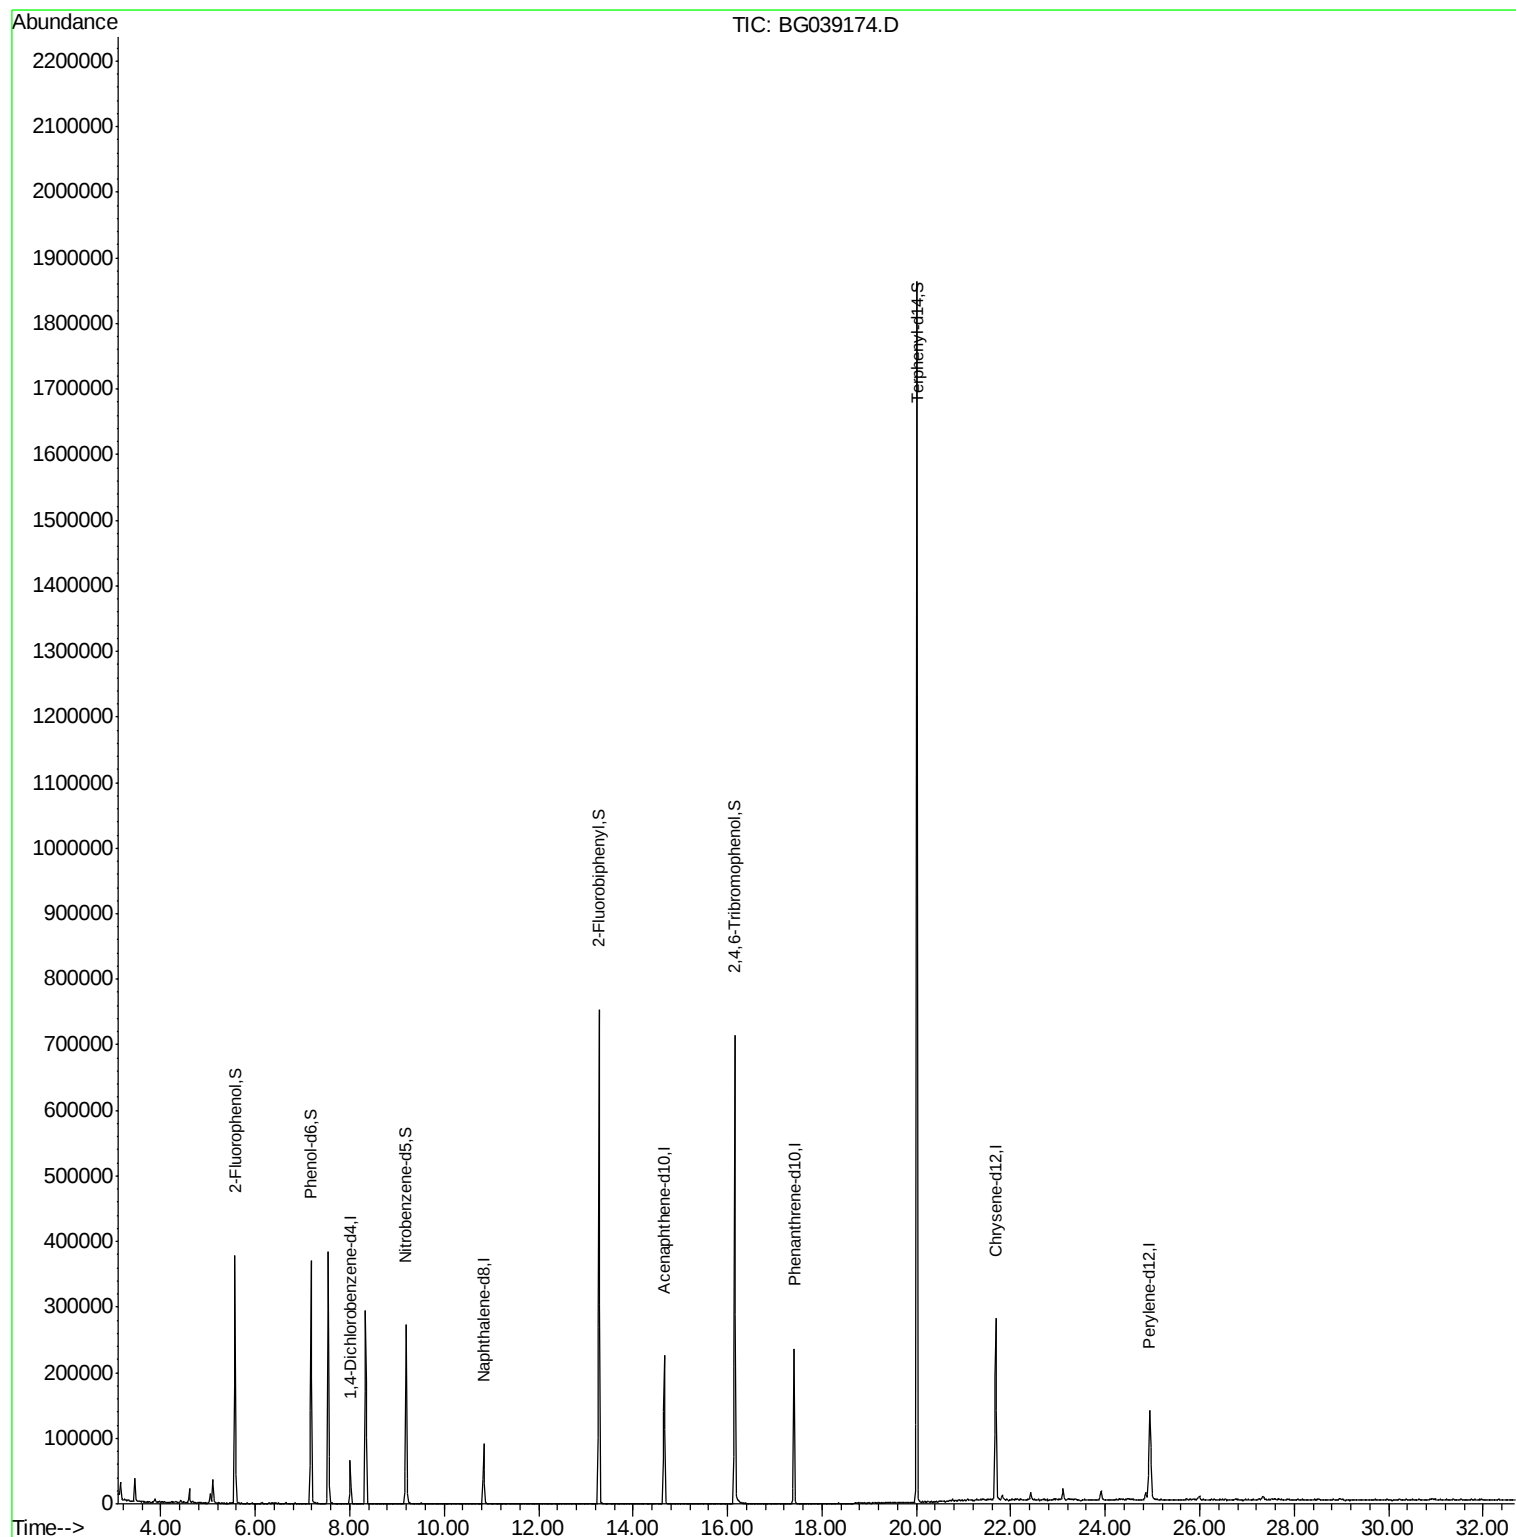




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 838
Delta R.T. -0.02 min
Lab File: BG039174.D
Acq: 17 Jan 2019 2:14

Instrument :
BNA_G
ClientSampleId :
OK-01-011519-B

Tot Ion:152 Resp: 19561
Ion Ratio Lower Upper
152 100
150 160.6 124.7 187.1
115 54.0 46.5 69.7

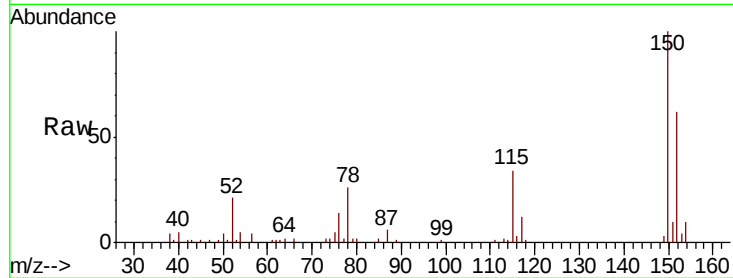


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

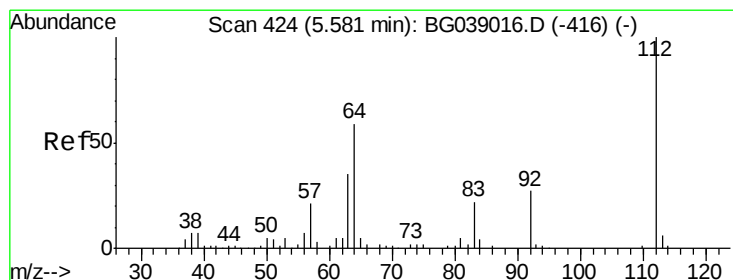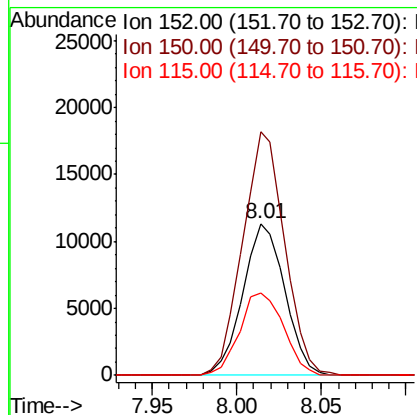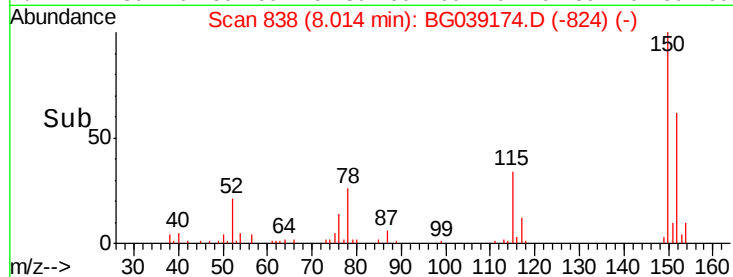



#5


2-Fluorophenol
Concen: 153.192 ng
RT: 5.57 min Scan# 422
Delta R.T. -0.01 min
Lab File: BG039174.D
Acq: 17 Jan 2019 2:14

Tgt Ion:112 Resp: 157966
Ion Ratio Lower Upper
112 100
64 63.5 47.0 70.6
63 32.9 28.0 42.0

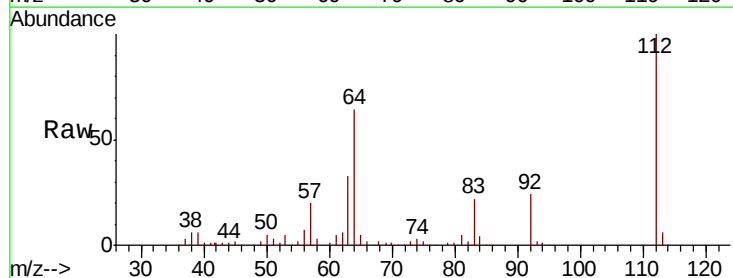

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

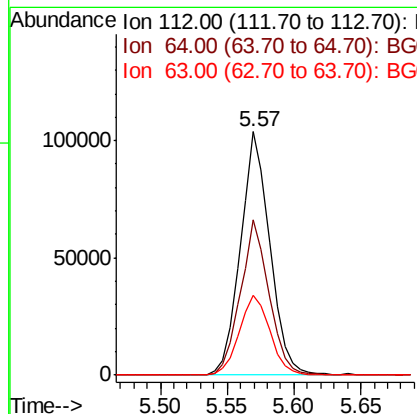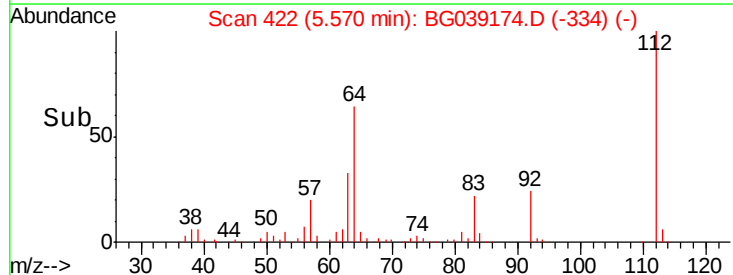

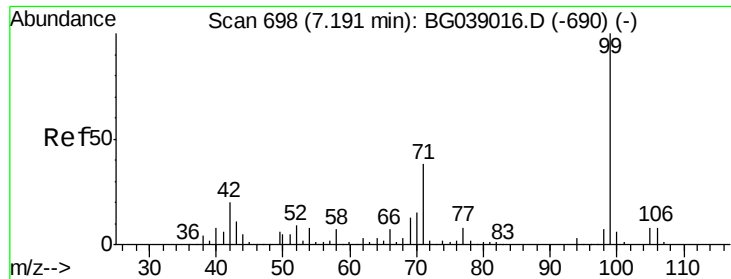

#7

Phenol-d6

Concen: 149.459 ng

RT: 7.18 min Scan# 696

Delta R.T. -0.01 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14

Instrument :

BNA_G

ClientSampleId :

OK-01-011519-B


Tot Ion: 99 Resp: 221794

Ion Ratio Lower Upper



99 100

42 19.9 15.8 23.6

71 36.4 30.2 45.4

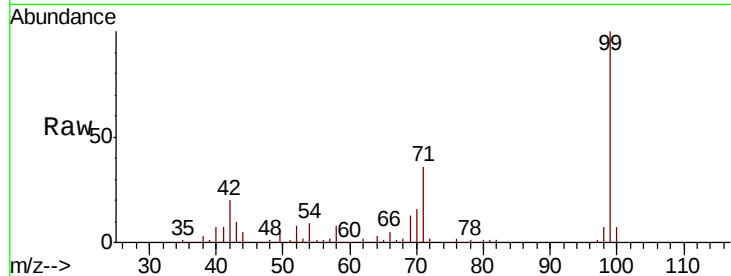

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

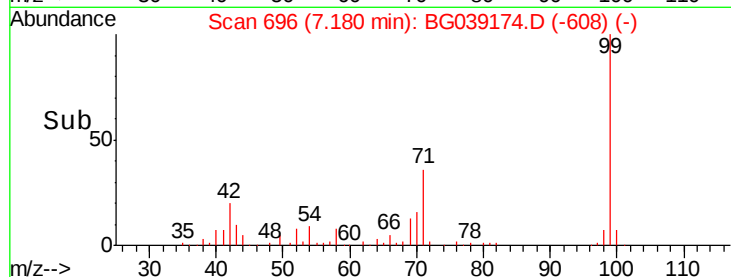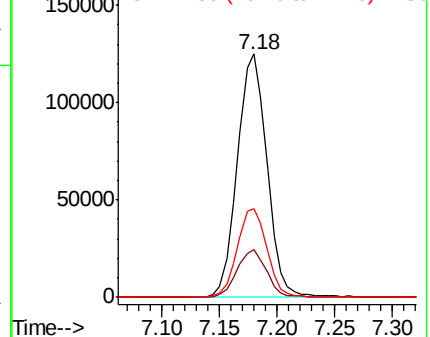

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1318

Delta R.T. -0.01 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14

Tgt Ion: 136 Resp: 85219


Ion Ratio Lower Upper

136 100



137 12.3 9.4 14.2


54 9.0 7.2 10.8

68 3.6 3.5 5.3

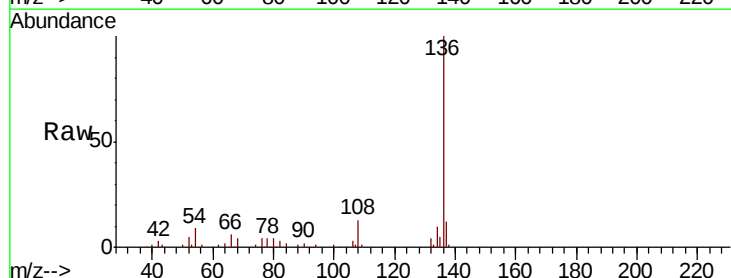

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



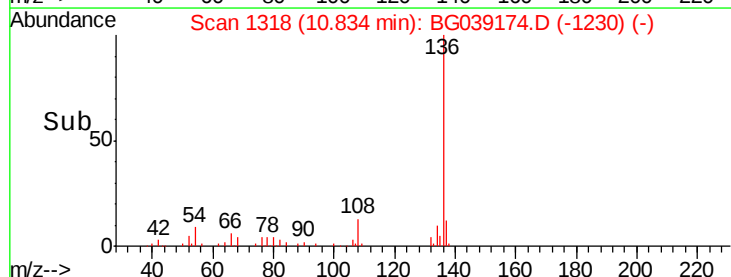
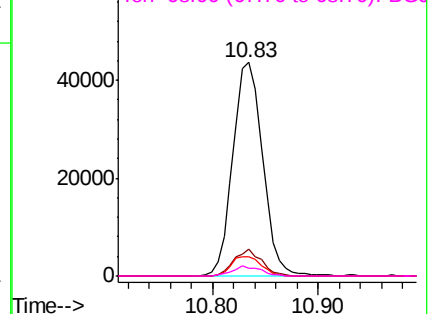


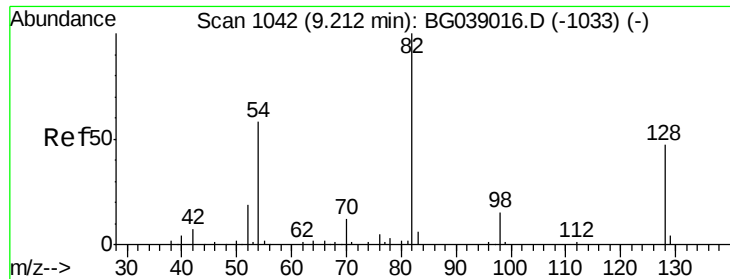

#23
 Nitrobenzene-d5
 Concen: 107.117 ng
 RT: 9.19 min Scan# 1039
 Delta R.T. -0.02 min
 Lab File: BG039174.D
 Acq: 17 Jan 2019 2:14




Instrument :
 BNA_G
 ClientSampleId :
 OK-01-011519-B


Tot Ion: 82 Resp: 166822
 Ion Ratio Lower Upper
 82 100
 128 46.5 37.3 55.9
 54 56.6 46.4 69.6

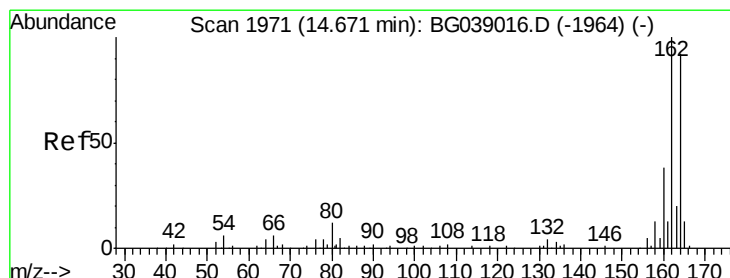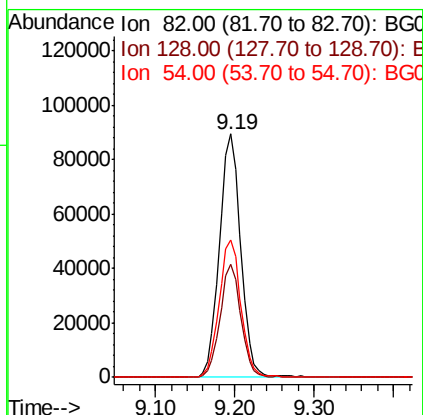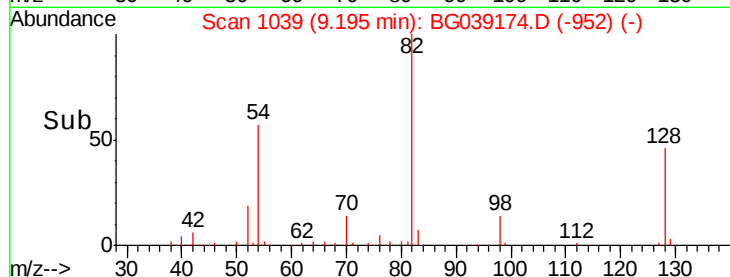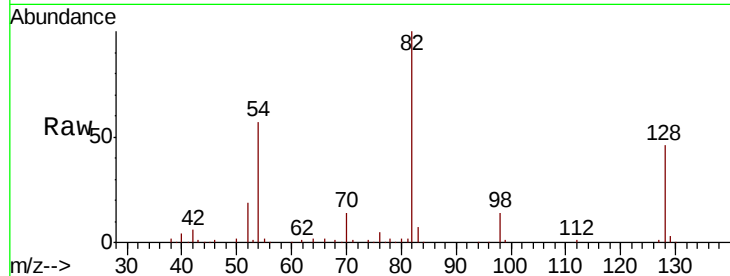

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1969
 Delta R.T. -0.01 min
 Lab File: BG039174.D
 Acq: 17 Jan 2019 2:14

Tgt Ion: 164 Resp: 82630
 Ion Ratio Lower Upper
 164 100
 162 102.4 87.2 130.8
 160 43.8 33.3 49.9

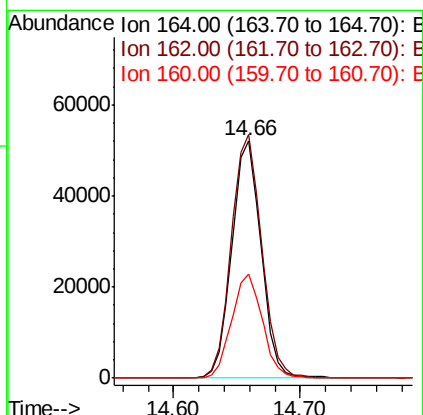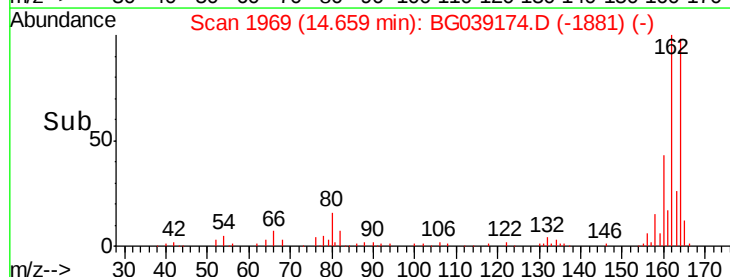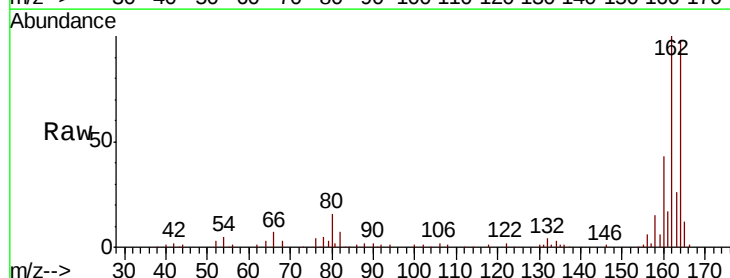


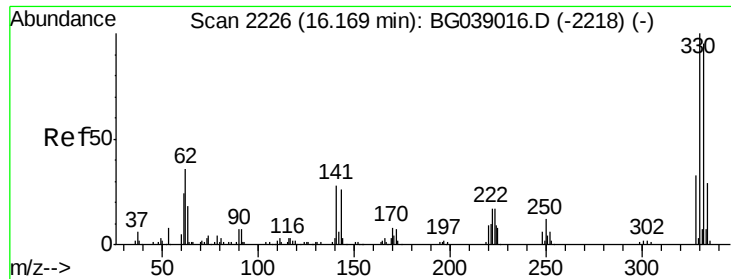

#42
 2,4,6-Tribromophenol
 Concen: 114.515 ng
 RT: 16.15 min Scan# 2223
 Delta R.T. -0.02 min
 Lab File: BG039174.D
 Acq: 17 Jan 2019 2:14

Instrument :
 BNA_G
 ClientSampleId :
 OK-01-011519-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.0	75.7	113.5
141	31.6	24.9	37.3



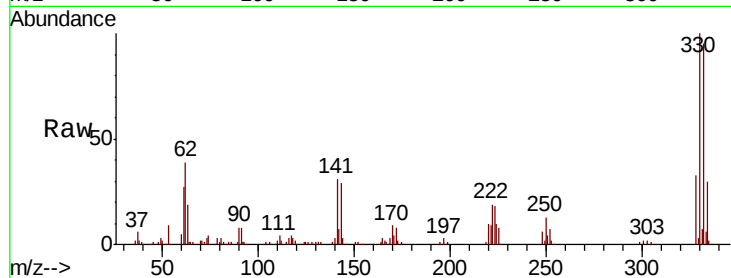


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

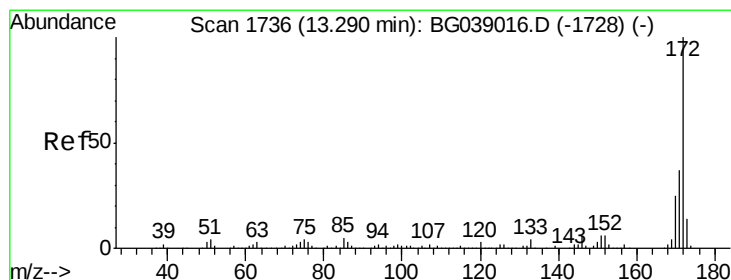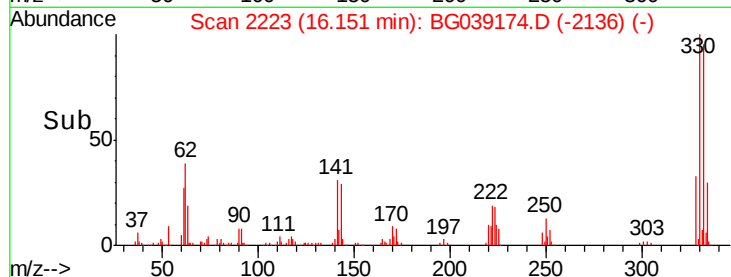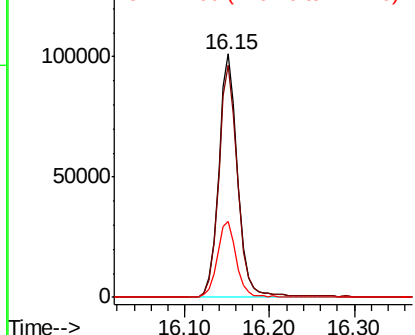

#45
 2-Fluorobiphenyl
 Concen: 69.930 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.01 min
 Lab File: BG039174.D
 Acq: 17 Jan 2019 2:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.4	44.0
170	24.4	20.1	30.1


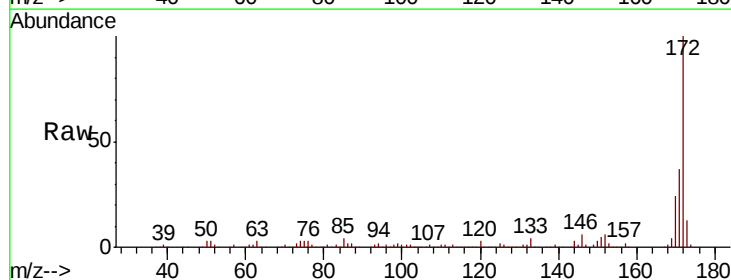


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

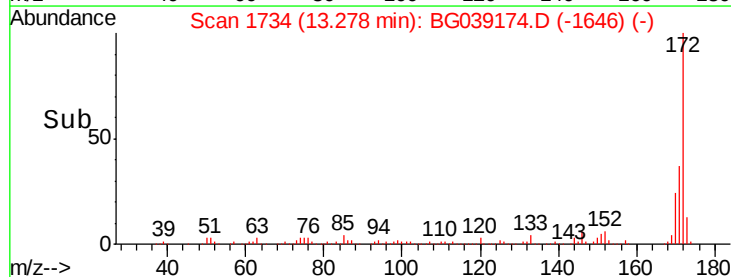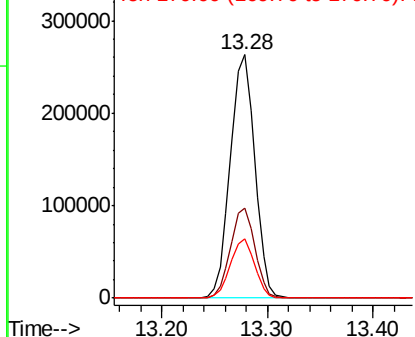



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2437

Delta R.T. -0.01 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14

Instrument :

BNA_G

ClientSampleId :

OK-01-011519-B


Tot Ion:188 Resp: 161278

Ion Ratio Lower Upper

188 100

94 6.5 5.0 7.4




80 5.7 4.7 7.1

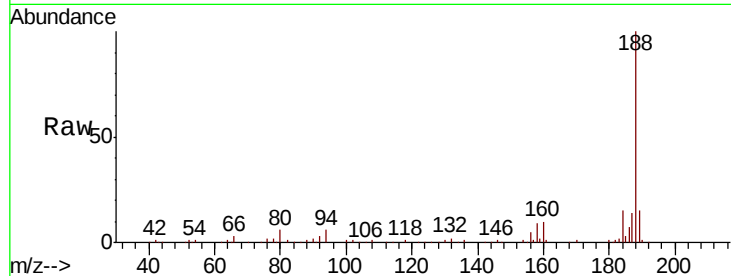

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

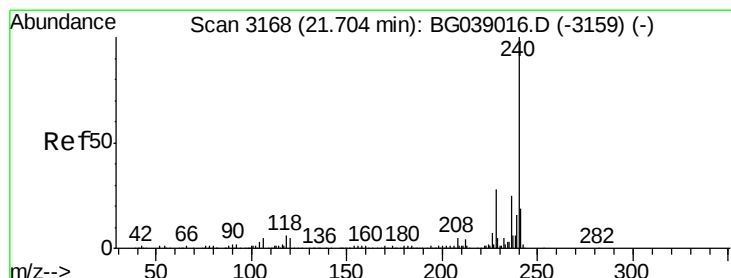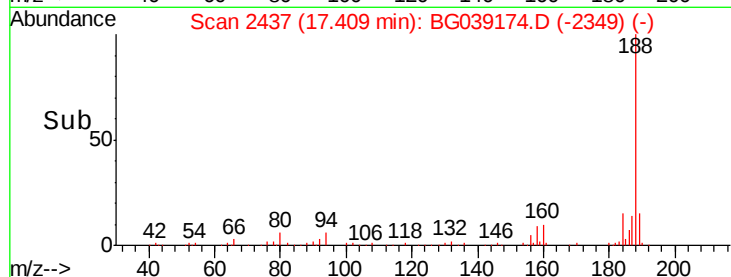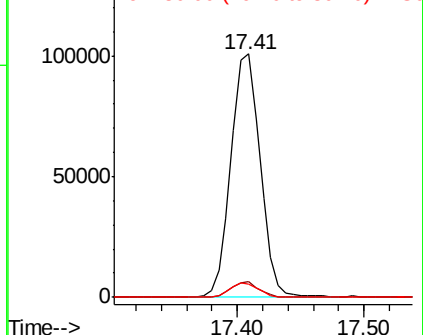

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3164

Delta R.T. -0.02 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14


Tgt Ion:240 Resp: 184278

Ion Ratio Lower Upper

240 100

120 5.4 4.3 6.5



236 25.3 20.1 30.1

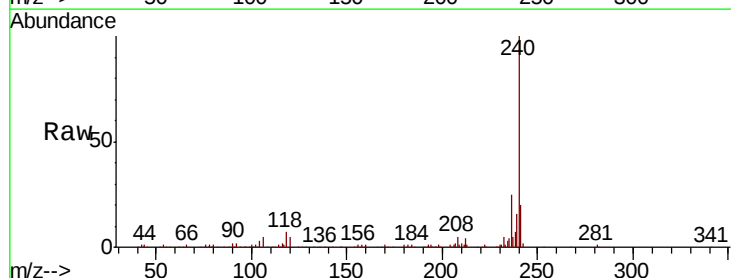


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

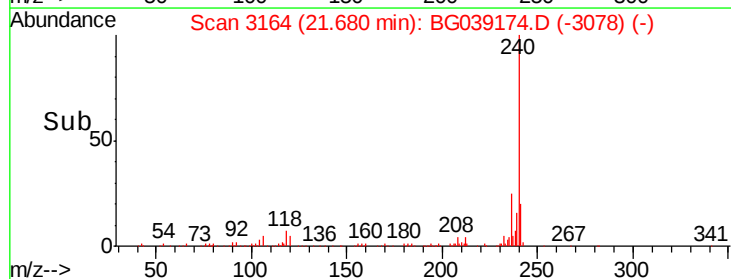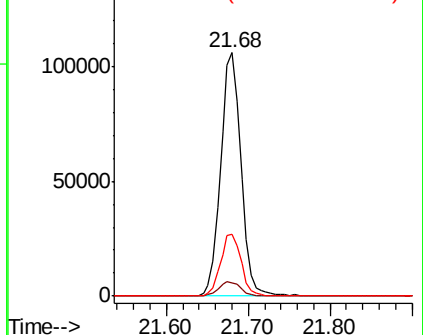

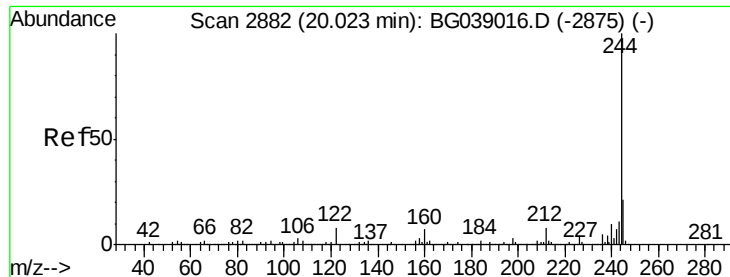

#79

Terphenyl-d14

Concen: 95.845 ng

RT: 20.01 min Scan# 2880

Delta R.T. -0.01 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14

Instrument :

BNA_G

ClientSampleId :

OK-01-011519-B


Tot Ion:244 Resp: 954765

Ion Ratio Lower Upper

244 100

212 7.6 6.1 9.1




122 6.9 6.1 9.1

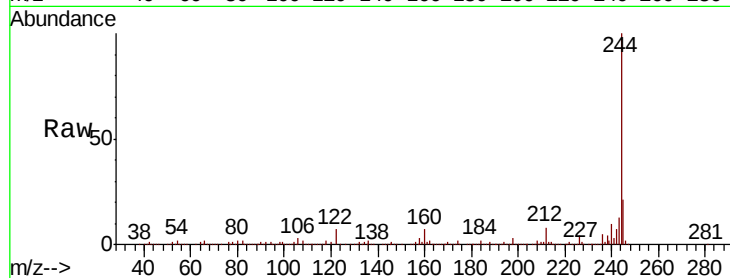

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

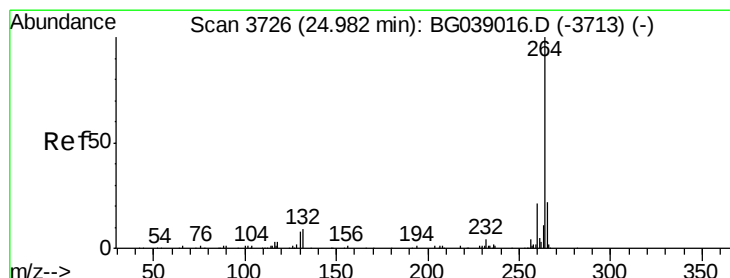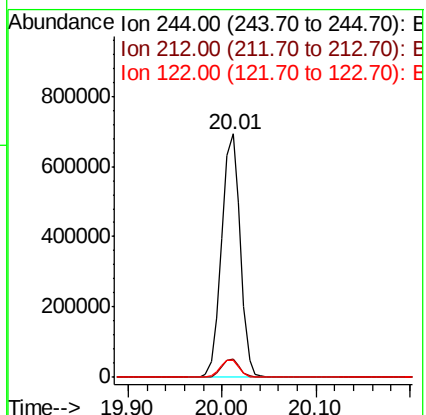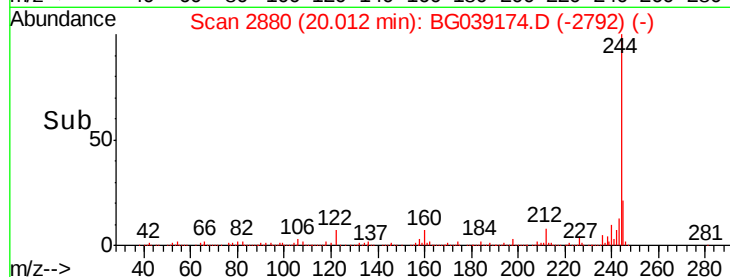

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.94 min Scan# 3719

Delta R.T. -0.04 min

Lab File: BG039174.D

Acq: 17 Jan 2019 2:14


Tgt Ion:264 Resp: 181084

Ion Ratio Lower Upper

264 100

260 21.2 17.0 25.6

265 20.7 17.2 25.8

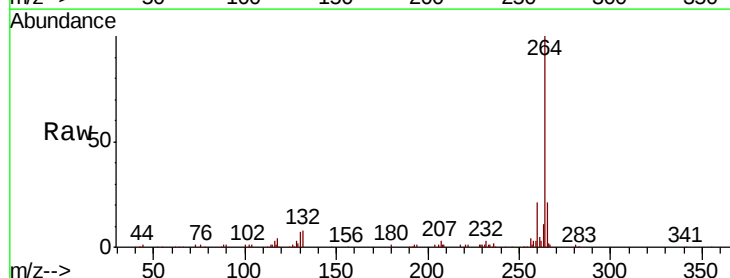

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

