

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011619\
 Data File : BG039175.D
 Acq On : 17 Jan 2019 2:53
 Operator : JU/SJ
 Sample : K1147-24
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-8

Quant Time: Jan 17 05:40:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 09 14:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	17609	20.00	ng	-0.02
21) Naphthalene-d8	10.83	136	79309	20.00	ng	-0.01
39) Acenaphthene-d10	14.66	164	58535	20.00	ng	-0.01
64) Phenanthrene-d10	17.40	188	159477	20.00	ng	-0.02
76) Chrysene-d12	21.68	240	175894	20.00	ng	-0.02
87) Perylene-d12	24.94	264	193777	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	139578	150.36	ng	-0.01
7) Phenol-d6	7.18	99	180194	134.89	ng	-0.01
23) Nitrobenzene-d5	9.20	82	143082	98.72	ng	-0.02
42) 2,4,6-Tribromophenol	16.15	330	144639	147.41	ng	-0.02
45) 2-Fluorobiphenyl	13.28	172	435619	101.85	ng	-0.01
79) Terphenyl-d14	20.01	244	847718	89.16	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011619\
Data File : BG039175.D
Acq On : 17 Jan 2019 2:53
Operator : JU/SJ
Sample : K1147-24
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-8

Quant Time: Jan 17 05:40:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

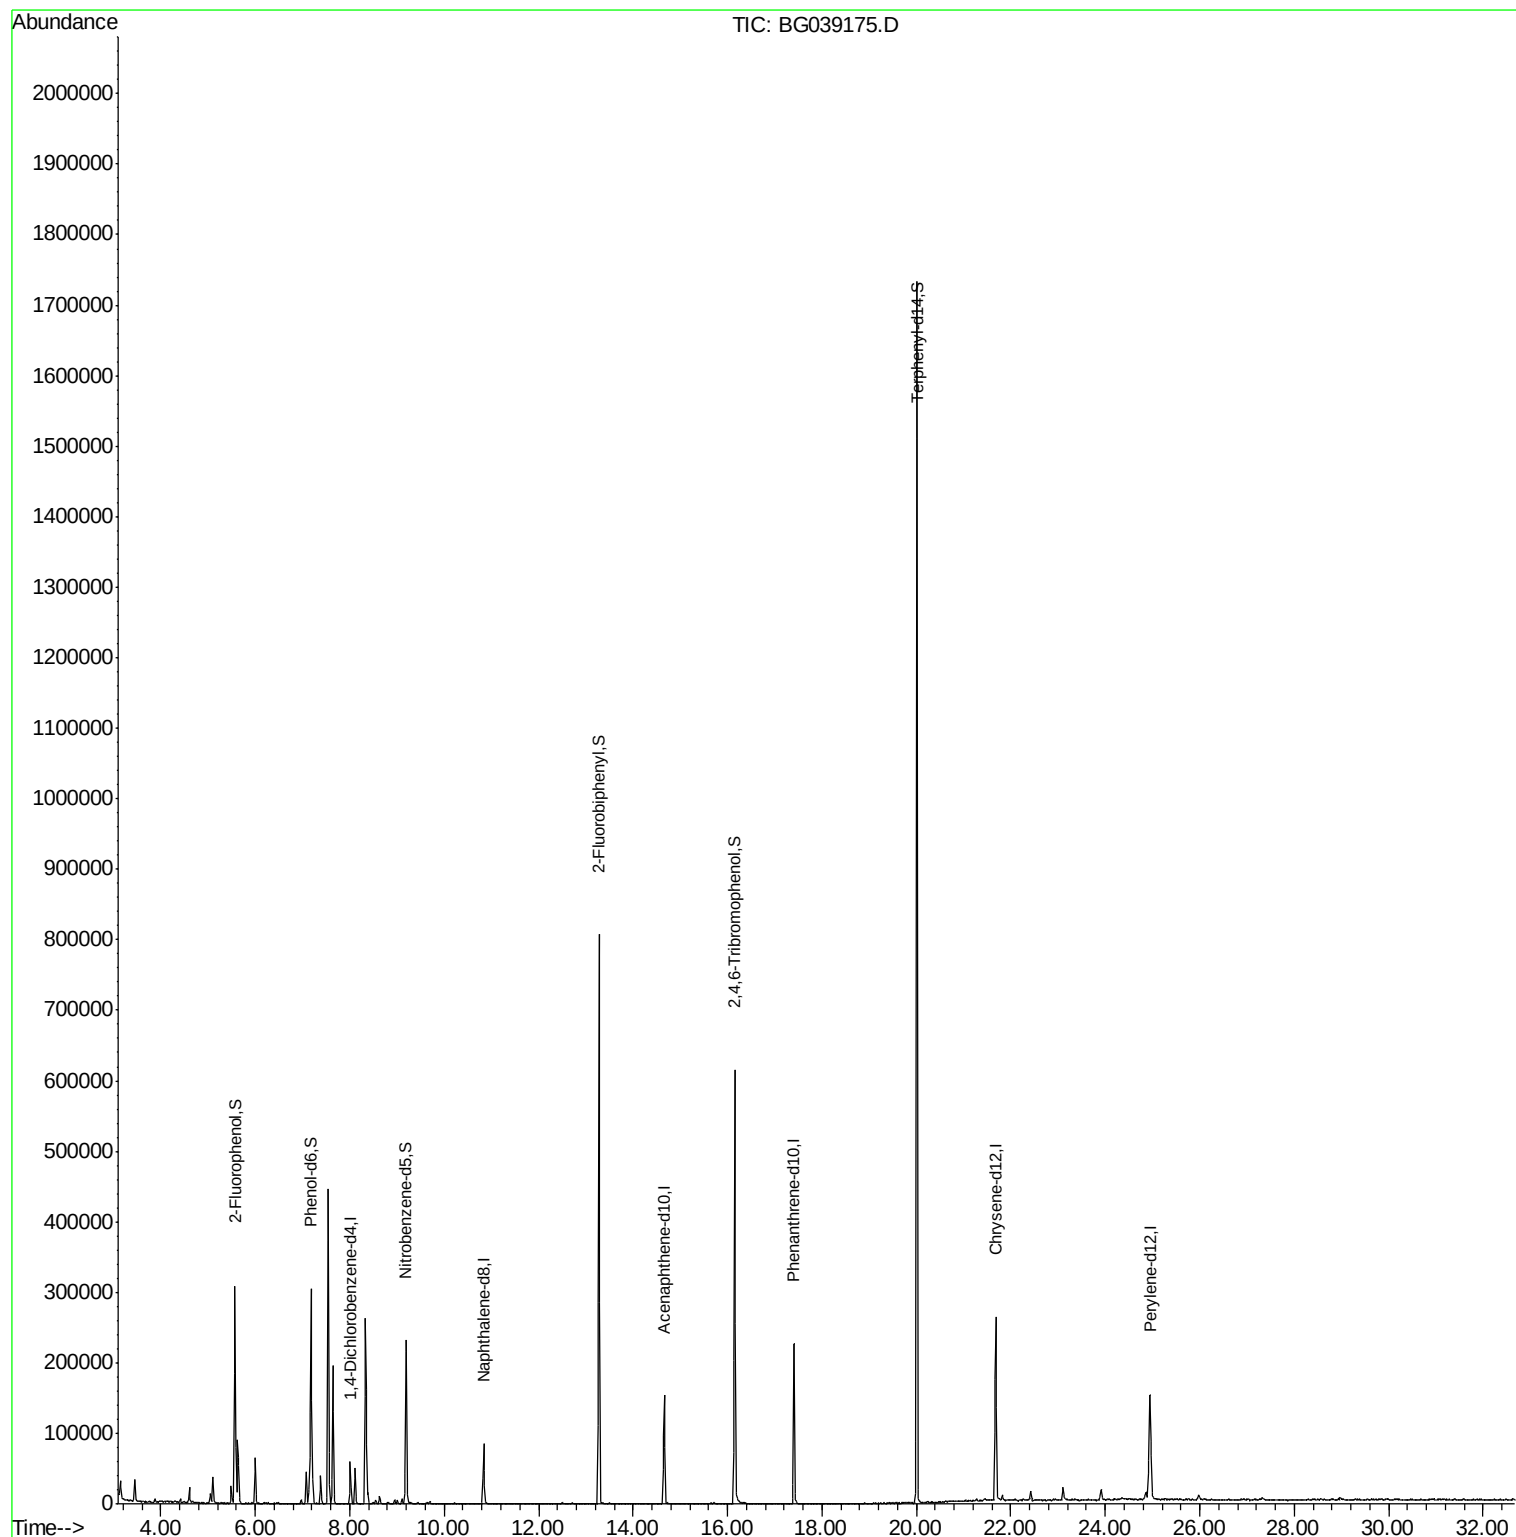

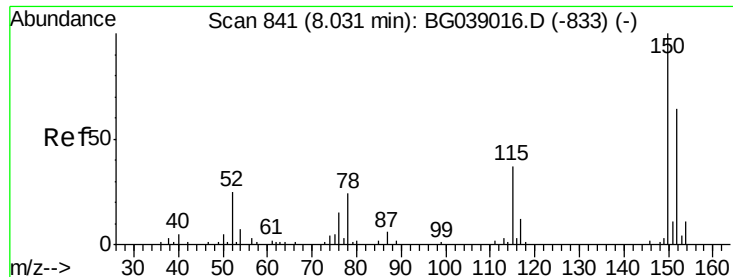


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 838
Delta R.T. -0.02 min
Lab File: BG039175.D
Acq: 17 Jan 2019 2:53

Instrument :
BNA_G
ClientSampleId :
TP-8

Tot Ion	Ratio	Lower	Upper
152	100		
150	149.5	124.7	187.1
115	60.1	46.5	69.7



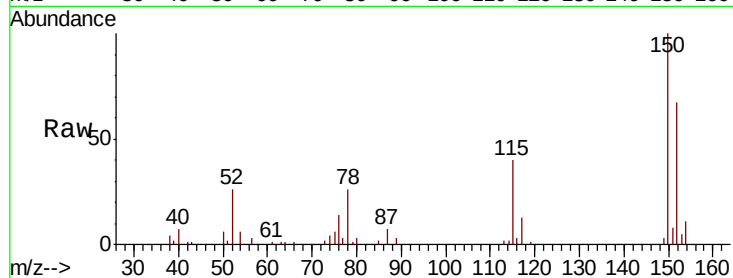


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

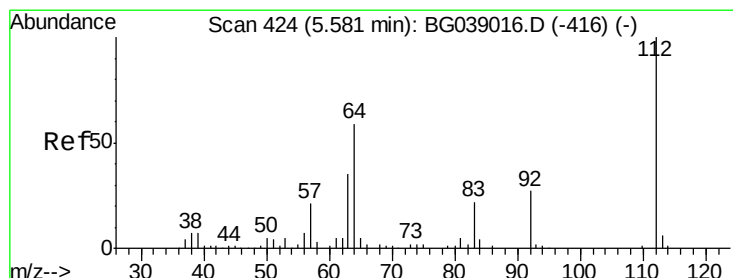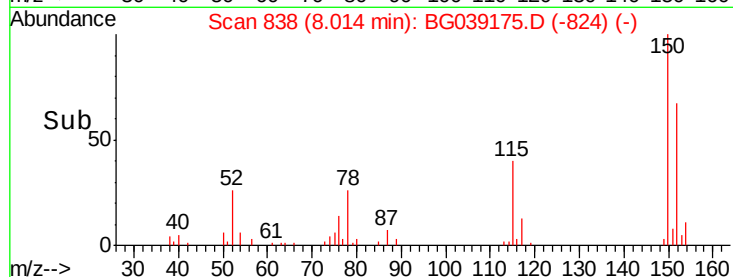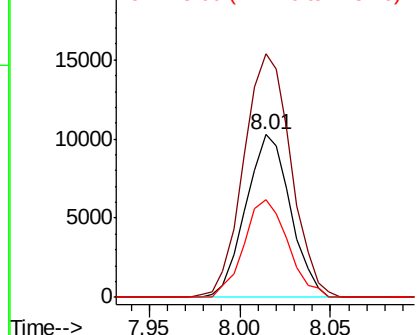

#5

2-Fluorophenol
Concen: 150.365 ng
RT: 5.57 min Scan# 422
Delta R.T. -0.01 min
Lab File: BG039175.D
Acq: 17 Jan 2019 2:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.6	47.0	70.6
63	36.0	28.0	42.0


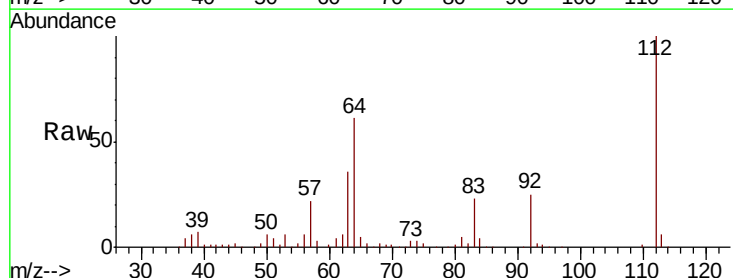



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

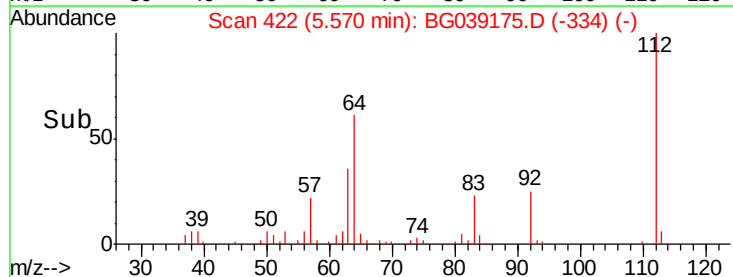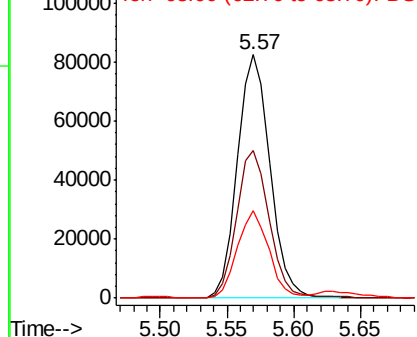

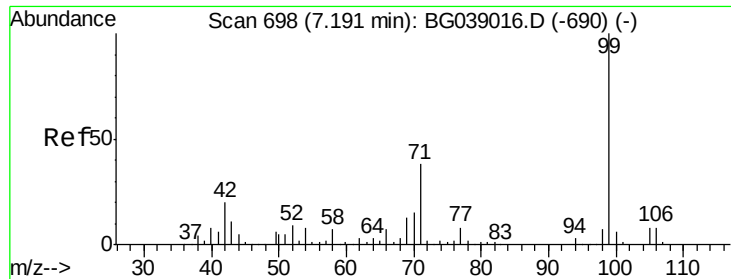

#7

Phenol-d6

Concen: 134.887 ng

RT: 7.18 min Scan# 696

Delta R.T. -0.01 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53

Instrument :

BNA_G

ClientSampled :

TP-8


Tot Ion: 99 Resp: 180194

Ion Ratio Lower Upper




99 100

42 20.9 15.8 23.6

71 38.3 30.2 45.4

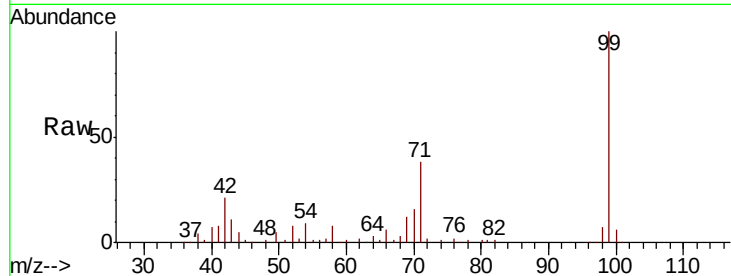

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

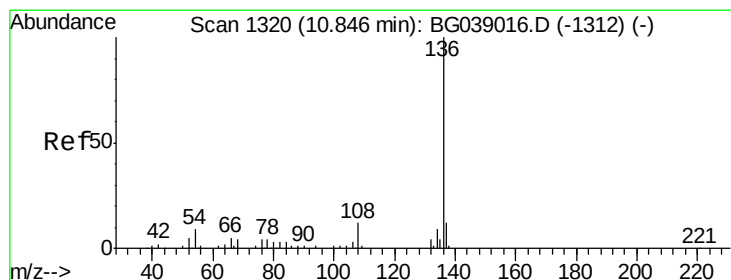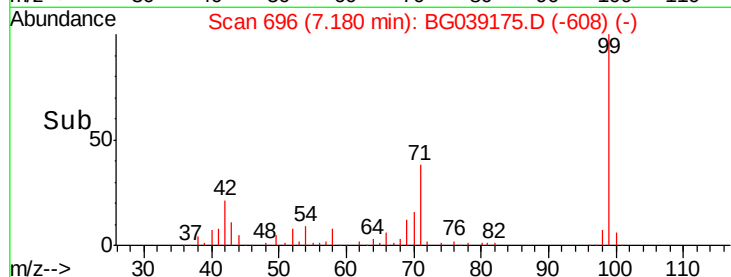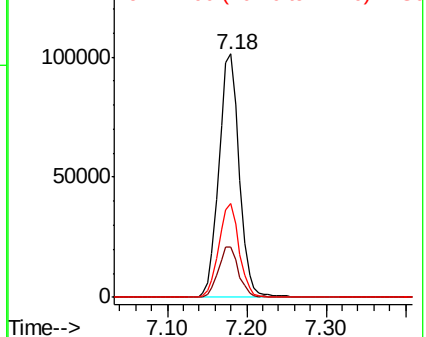

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1318

Delta R.T. -0.01 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53

Tgt Ion: 136 Resp: 79309


Ion Ratio Lower Upper

136 100



137 10.9 9.4 14.2


54 9.0 7.2 10.8

68 3.8 3.5 5.3

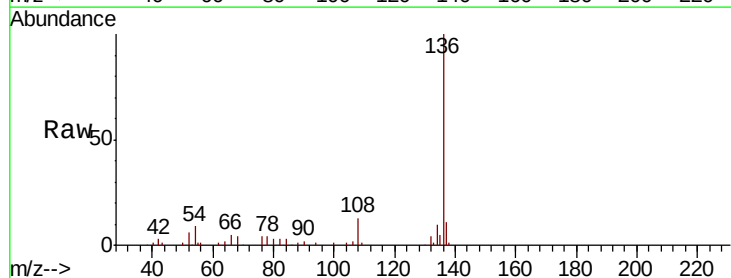

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

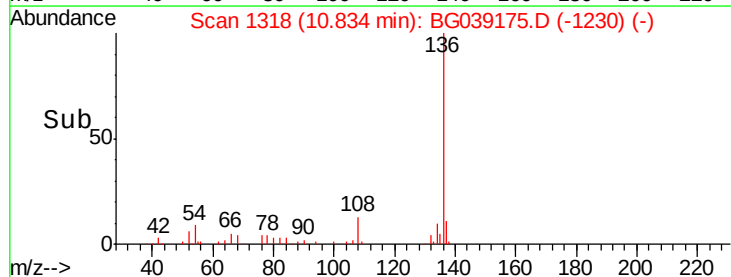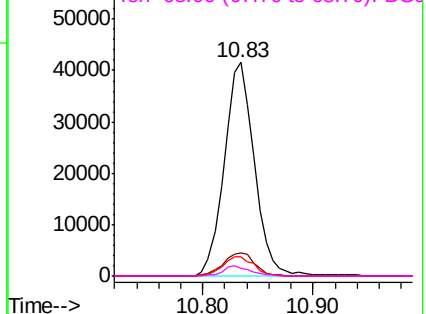


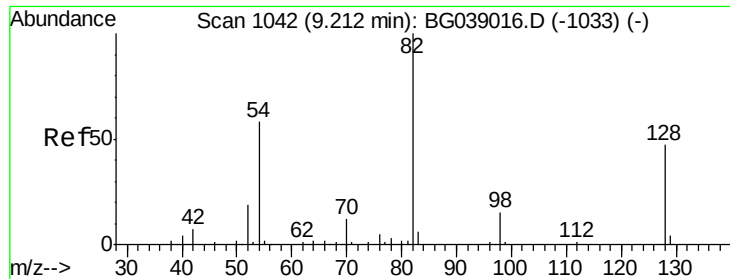

#23
 Nitrobenzene-d5
 Concen: 98.720 ng
 RT: 9.20 min Scan# 1039
 Delta R.T. -0.02 min
 Lab File: BG039175.D
 Acq: 17 Jan 2019 2:53

Instrument :
 BNA_G
 ClientSampled :
 TP-8

Tot Ion	82.00	Resp	143082
Ion Ratio	Lower	Upper	
82	100		
128	44.6	37.3	55.9
54	58.1	46.4	69.6



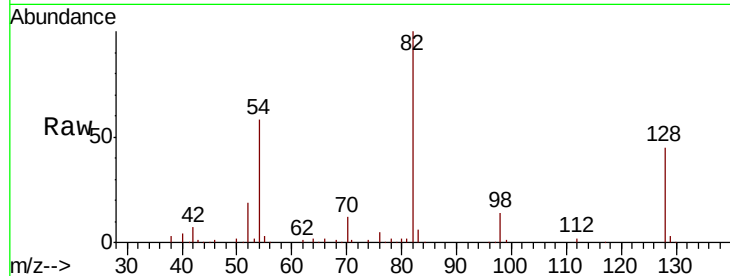


Abundance

Ion 82.00 (81.70 to 82.70): BG039175.D (-952) (-)


Ion 128.00 (127.70 to 128.70): BG039175.D (-952) (-)

Ion 54.00 (53.70 to 54.70): BG039175.D (-952) (-)

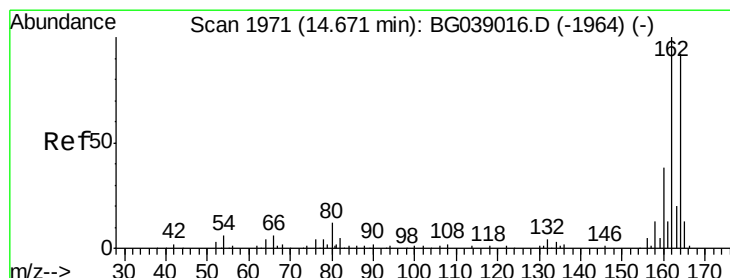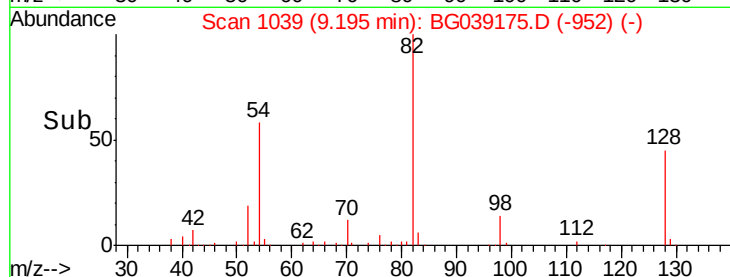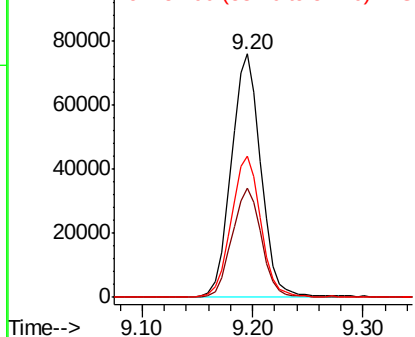

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1969
 Delta R.T. -0.01 min
 Lab File: BG039175.D
 Acq: 17 Jan 2019 2:53

Tgt Ion	164.00	Resp	58535
Ion Ratio	Lower	Upper	
164	100		
162	103.2	87.2	130.8
160	48.3	33.3	49.9


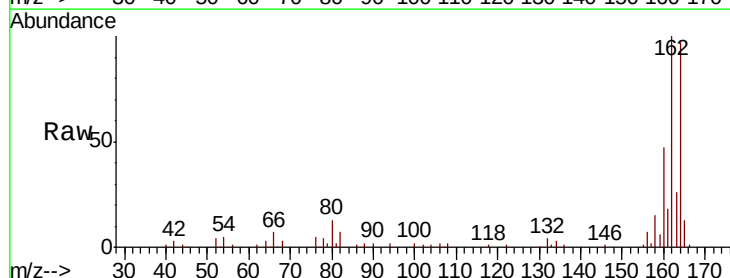



Abundance

Ion 164.00 (163.70 to 164.70): BG039175.D (-1881) (-)

Ion 162.00 (161.70 to 162.70): BG039175.D (-1881) (-)

Ion 160.00 (159.70 to 160.70): BG039175.D (-1881) (-)

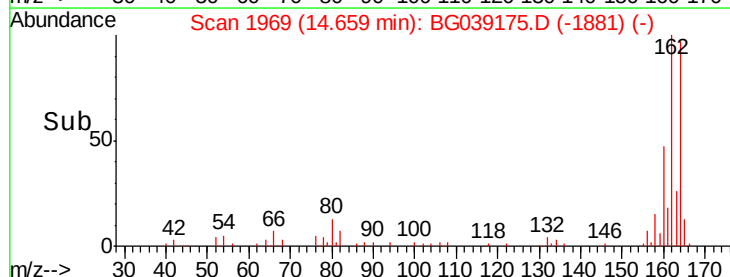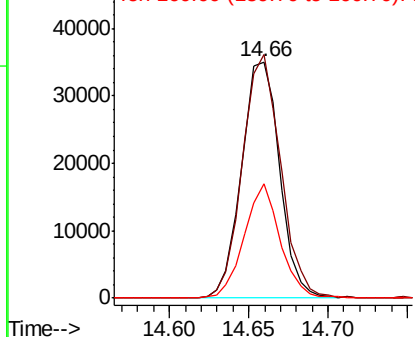

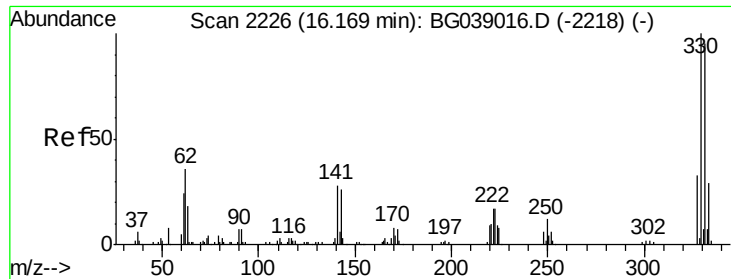

#42

2,4,6-Tribromophenol

Concen: 147.409 ng

RT: 16.15 min Scan# 2223

Delta R.T. -0.02 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53

Instrument :

BNA_G

ClientSampleId :

TP-8


Tot Ion:330 Resp: 144639

Ion Ratio Lower Upper

330 100

332 94.8 75.7 113.5




141 31.7 24.9 37.3

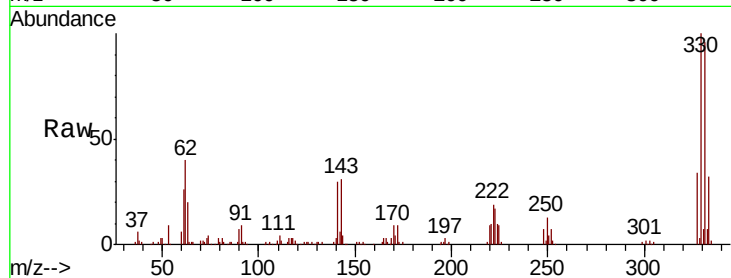

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

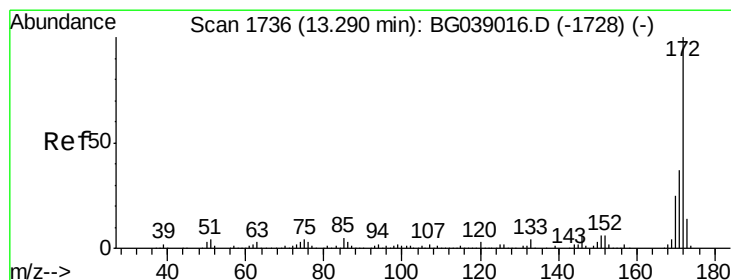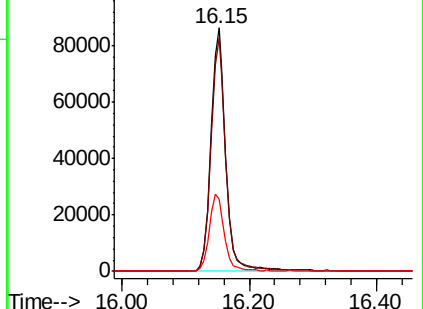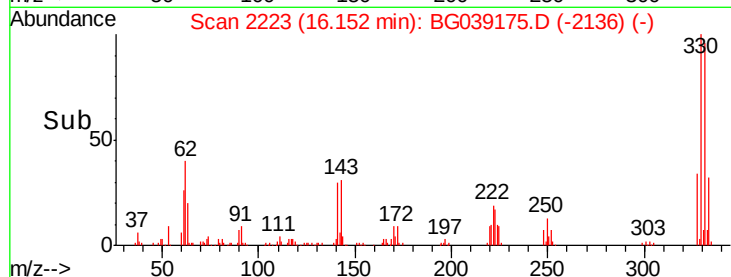

#45

2-Fluorobiphenyl

Concen: 101.849 ng

RT: 13.28 min Scan# 1734

Delta R.T. -0.01 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53


Tgt Ion:172 Resp: 435619

Ion Ratio Lower Upper

172 100

171 36.8 29.4 44.0



170 24.2 20.1 30.1

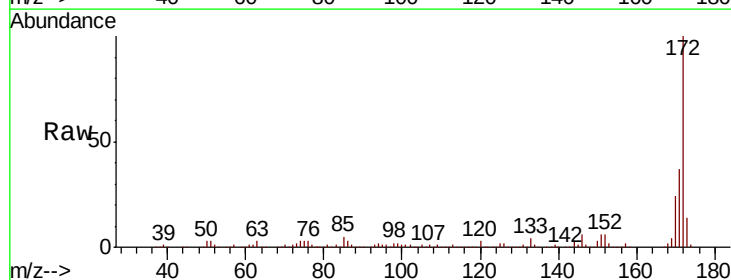


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

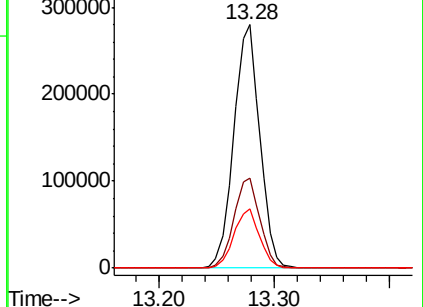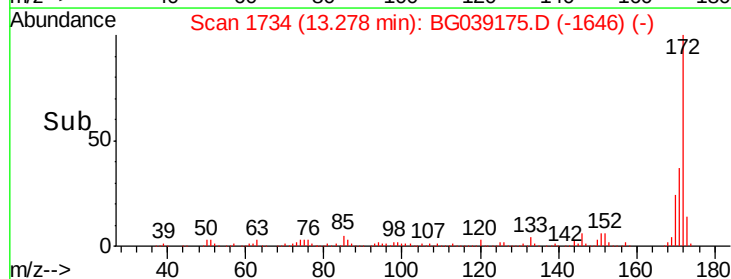

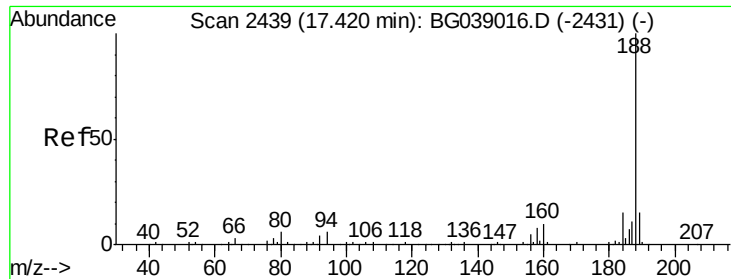

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2436

Delta R.T. -0.02 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53

Instrument :

BNA_G

ClientSampleId :

TP-8


Tot Ion:188 Resp: 159477

Ion Ratio Lower Upper

188 100

94 6.2 5.0 7.4




80 5.5 4.7 7.1

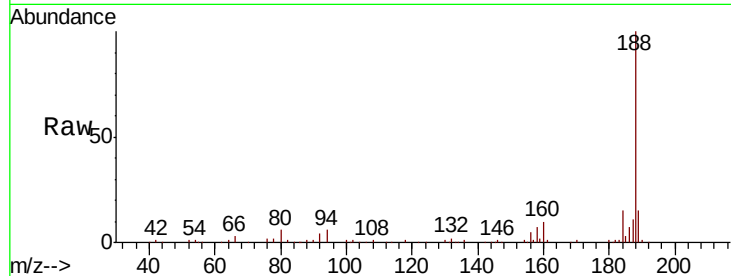

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

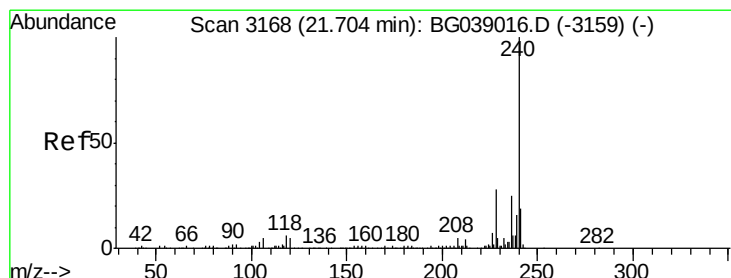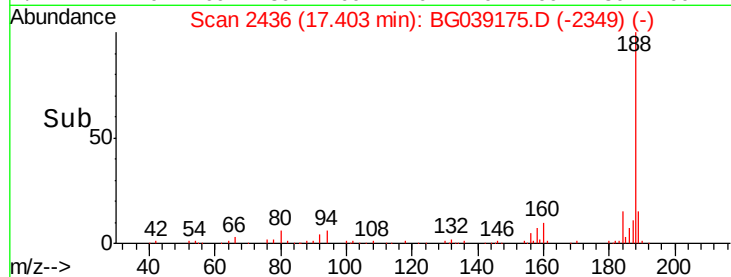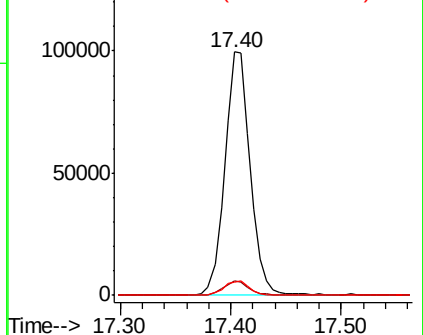

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3164

Delta R.T. -0.02 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53


Tgt Ion:240 Resp: 175894

Ion Ratio Lower Upper

240 100

120 6.8 4.3 6.5#



236 26.3 20.1 30.1

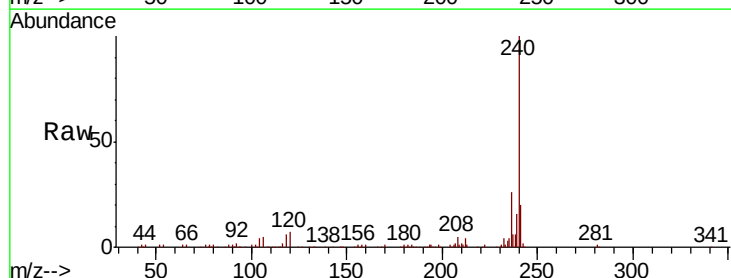


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

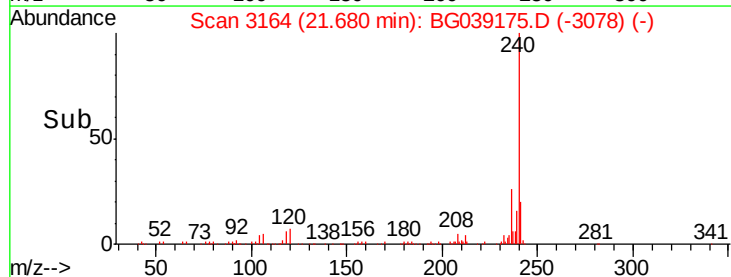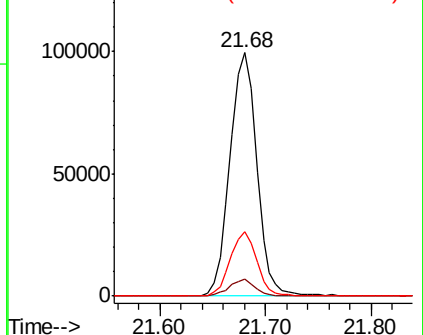

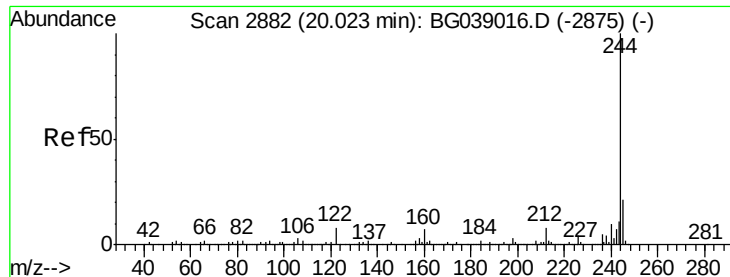

#79

Terphenyl-d14

Concen: 89.155 ng

RT: 20.01 min Scan# 2880

Delta R.T. -0.01 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53

Instrument :

BNA_G

ClientSampleId :

TP-8


Tot Ion:244 Resp: 847718

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1




122 6.8 6.1 9.1

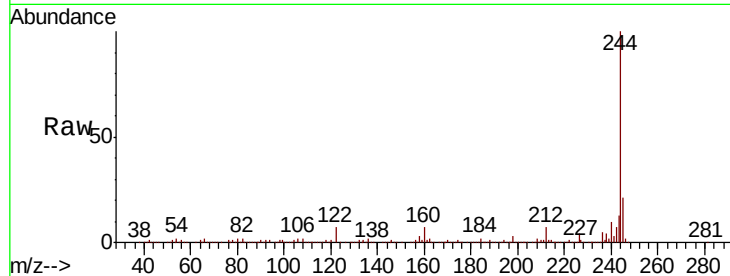

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

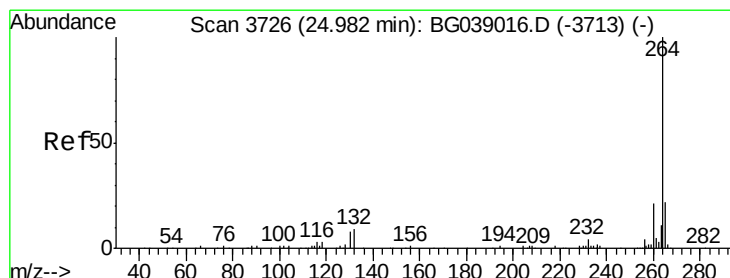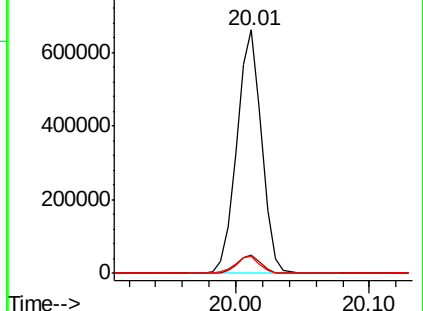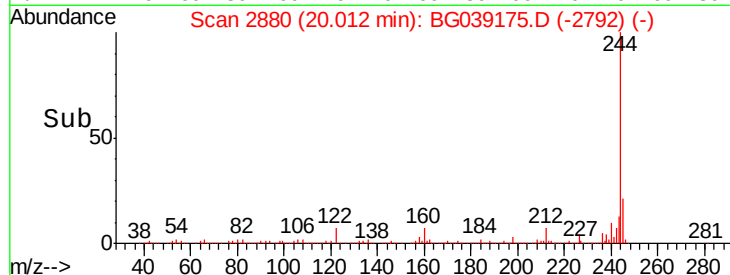

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.94 min Scan# 3719

Delta R.T. -0.04 min

Lab File: BG039175.D

Acq: 17 Jan 2019 2:53


Tgt Ion:264 Resp: 193777

Ion Ratio Lower Upper

264 100

260 23.0 17.0 25.6

265 20.5 17.2 25.8

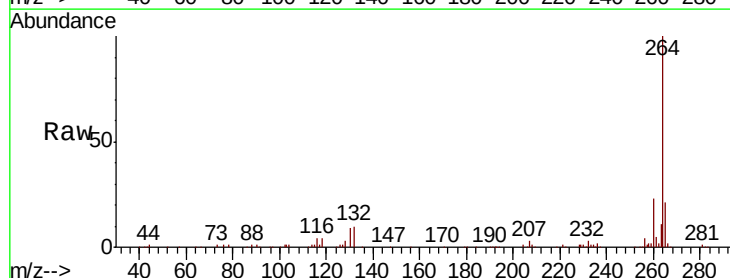

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

