


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011619\
 Data File : BG039152.D
 Acq On : 16 Jan 2019 10:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

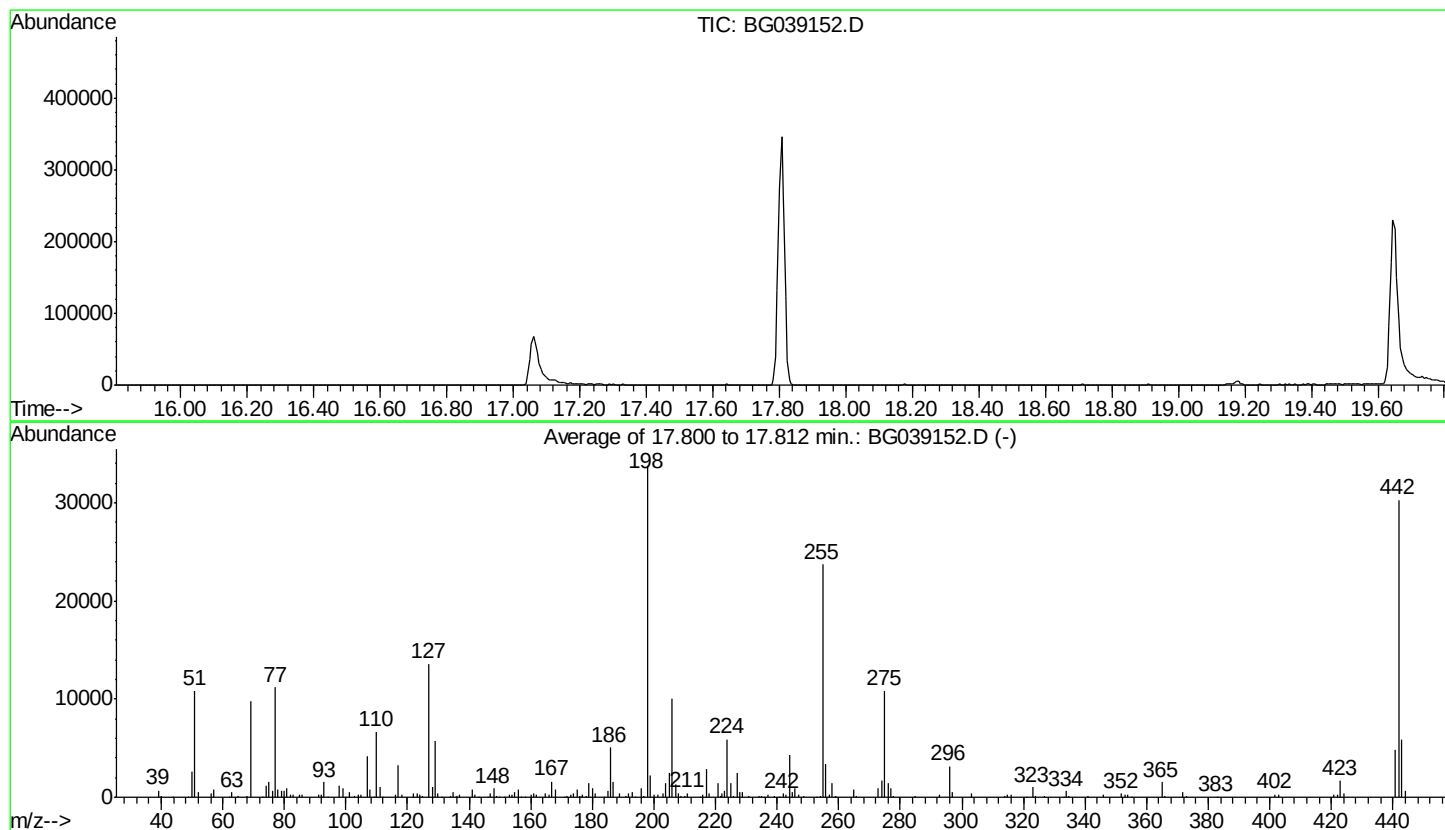

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	10880	PASS
68	69	0.00	2	1.5	147	PASS
69	198	0.00	100	29.0	9807	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.2	13589	PASS
197	198	0.00	2	0.3	113	PASS
198	198	100	100	100.0	33776	PASS
199	198	5	9	6.8	2285	PASS
275	198	10	60	32.2	10870	PASS
365	198	1	100	4.5	1508	PASS
441	198	0.01	100	14.1	4773	PASS
442	198	50	100	89.6	30256	PASS
443	442	15	24	19.4	5862	PASS