


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011619\
 Data File : BG039170.D
 Acq On : 16 Jan 2019 23:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

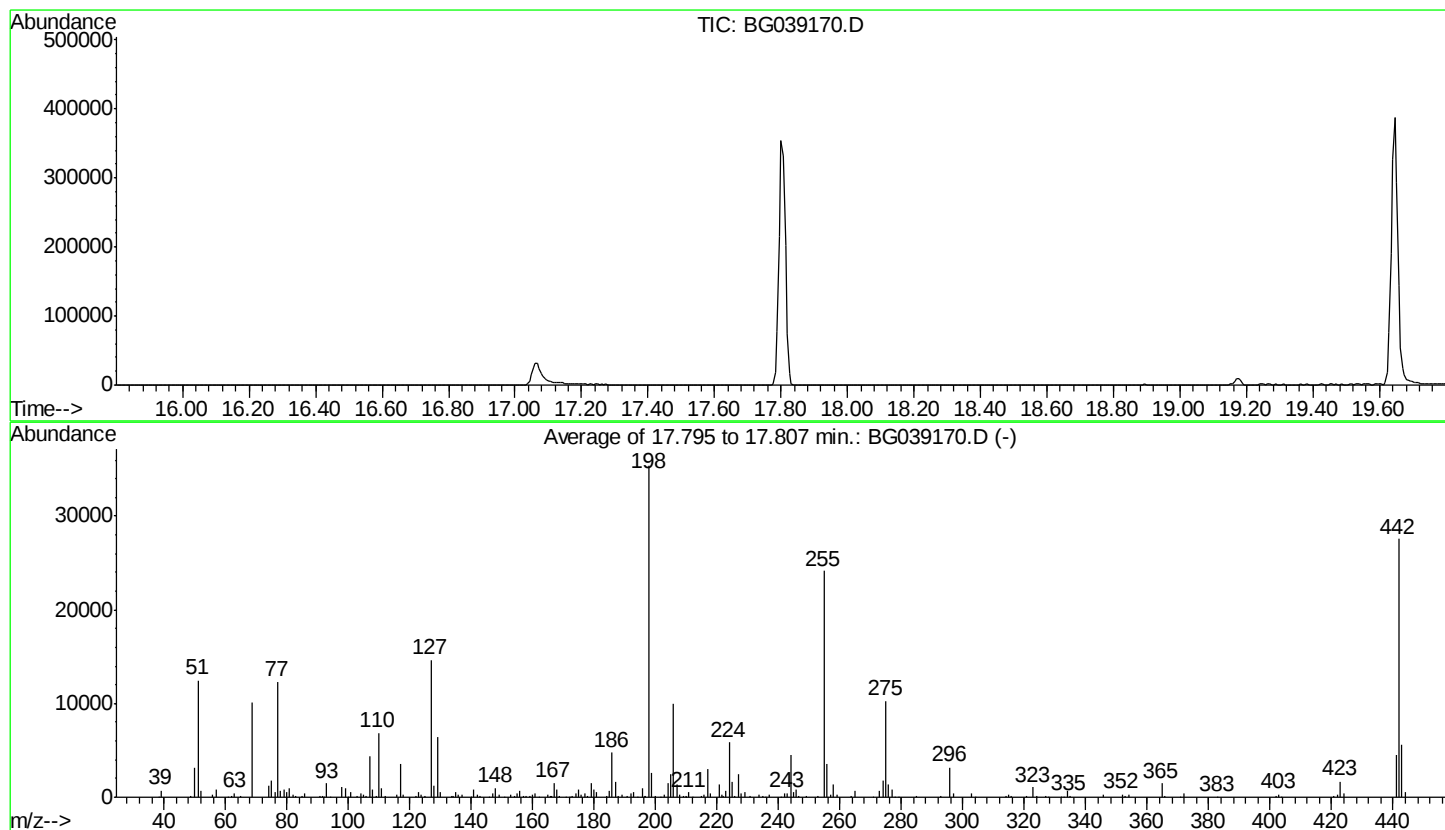

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	12485	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.5	10091	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.4	14652	PASS
197	198	0.00	2	0.4	138	PASS
198	198	100	100	100.0	35394	PASS
199	198	5	9	7.3	2597	PASS
275	198	10	60	29.1	10292	PASS
365	198	1	100	4.2	1496	PASS
441	198	0.01	100	12.7	4492	PASS
442	198	50	100	77.9	27585	PASS
443	442	15	24	20.4	5621	PASS