
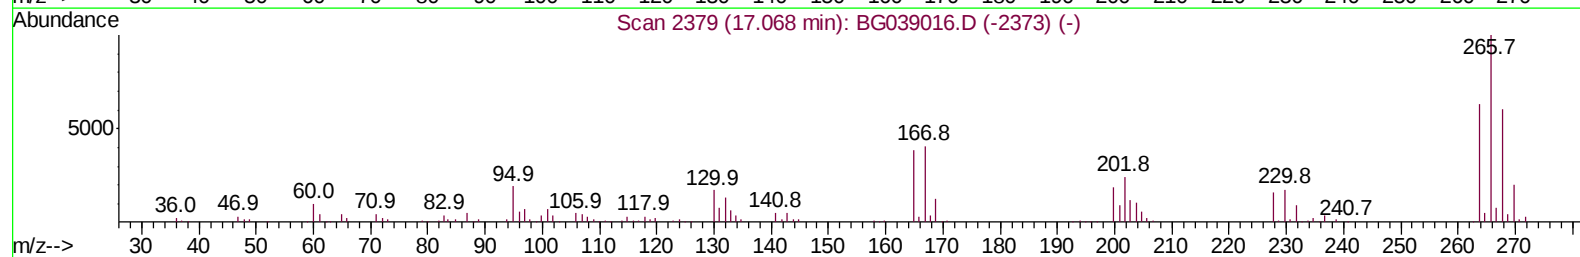
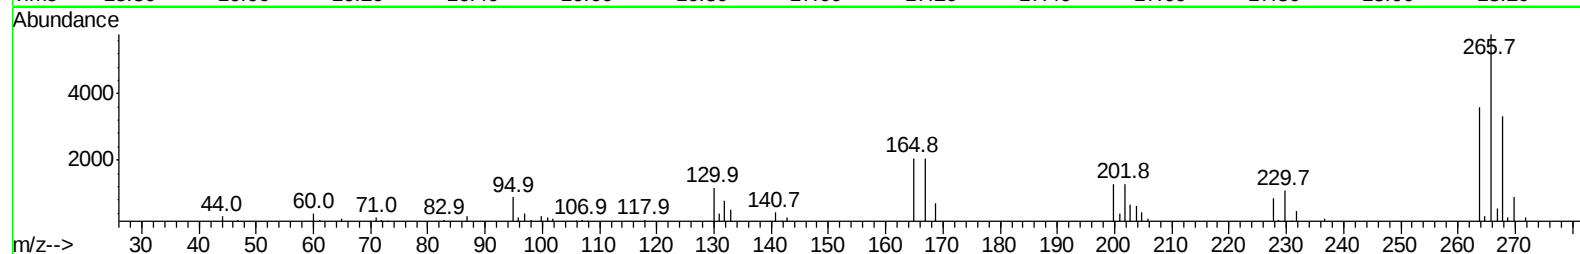


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011719\
Data File : BG039183.D
Acq On : 17 Jan 2019 11:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 05:54:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

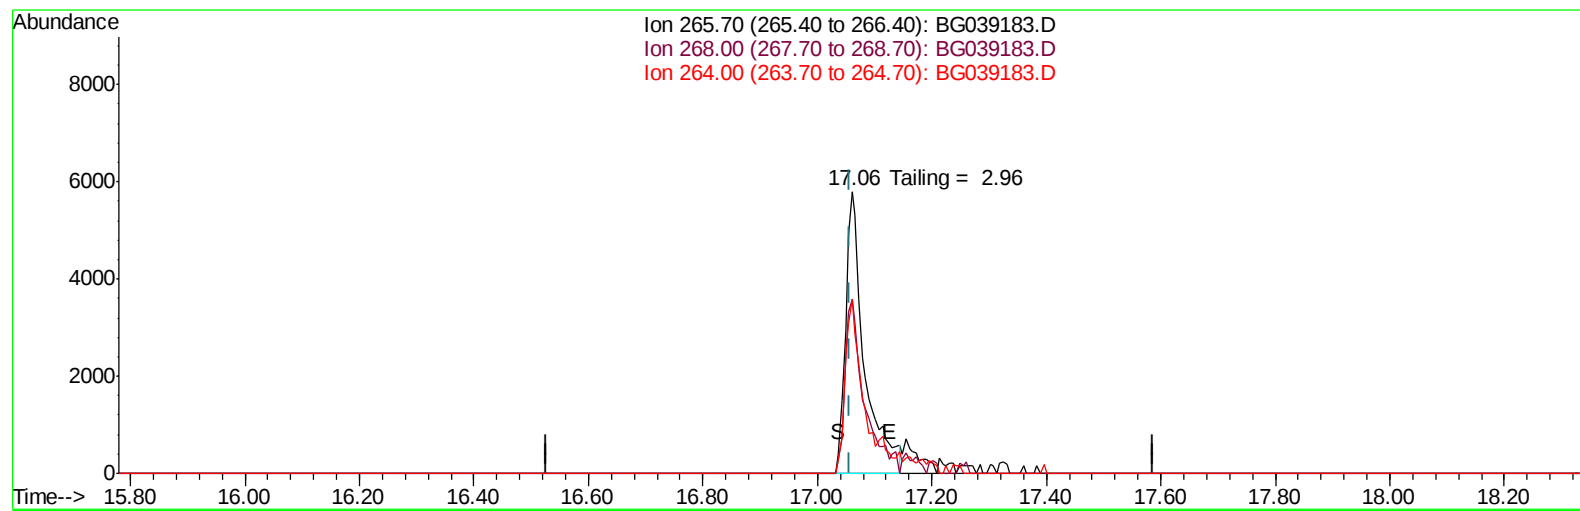

TIC: BG039183.D

(70) Pentachlorophenol (C)




17.060min (+0.003) 24253.05ng

response 13367

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.98
264.00	68.20	66.82
0.00	0.00	0.00

```
Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011719\  
Data File : BG039183.D  
Acq On    : 17 Jan 2019  11:32  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jan 18 05:54:10 2019
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

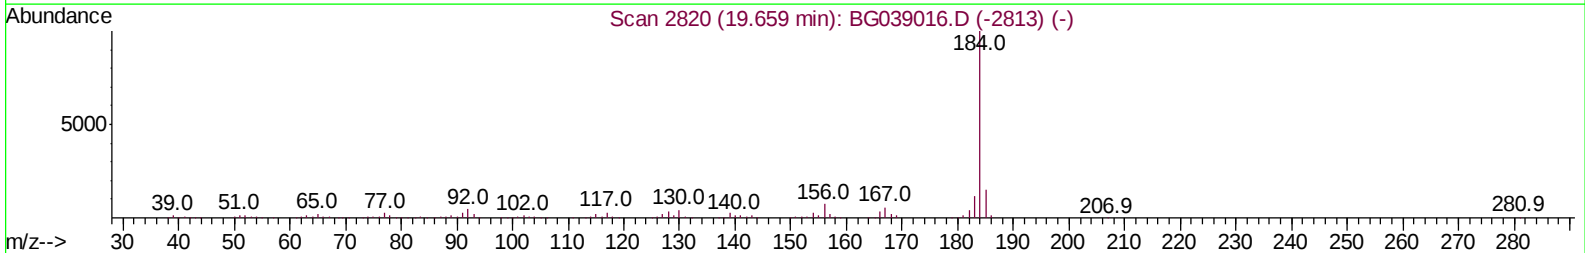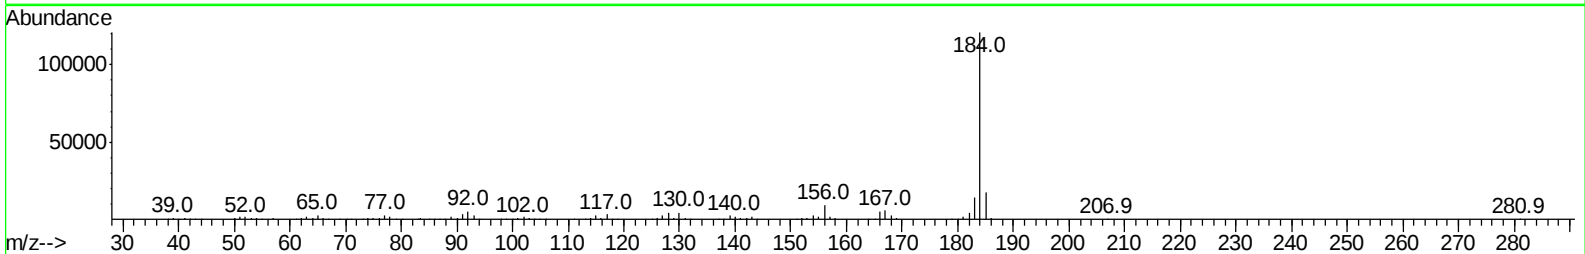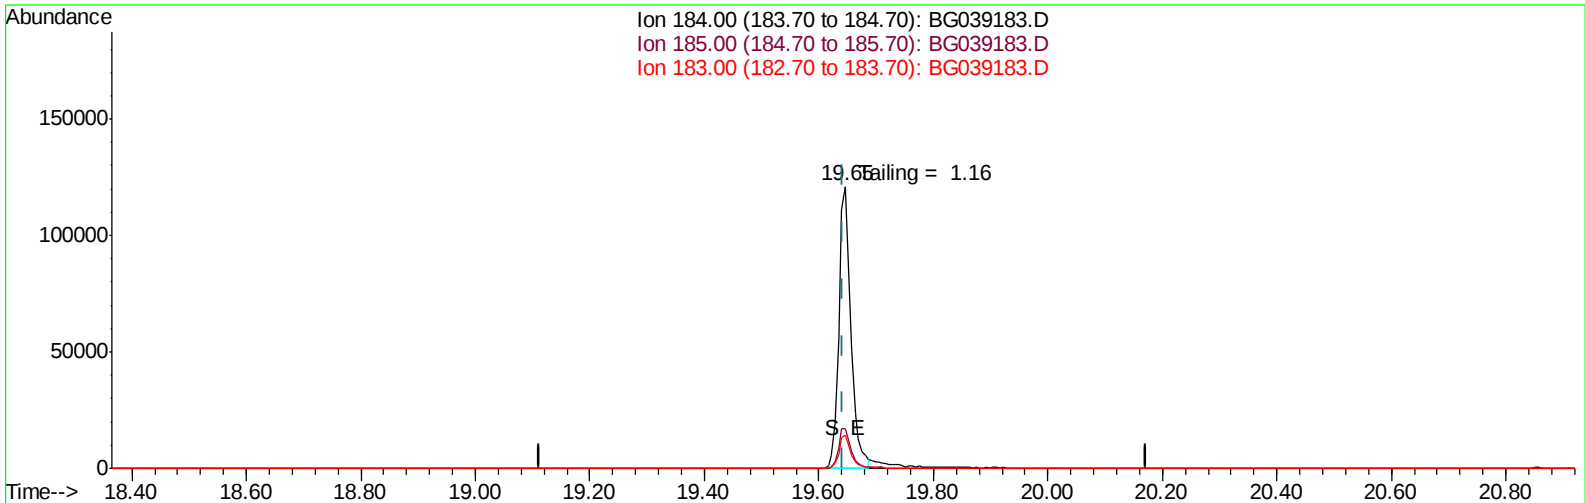

TIC: BG039183.D

(77) Benzidine

19.646min (+0.003) 98757.47ng

response 187278

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.25
183.00	11.90	12.00
0.00	0.00	0.00