
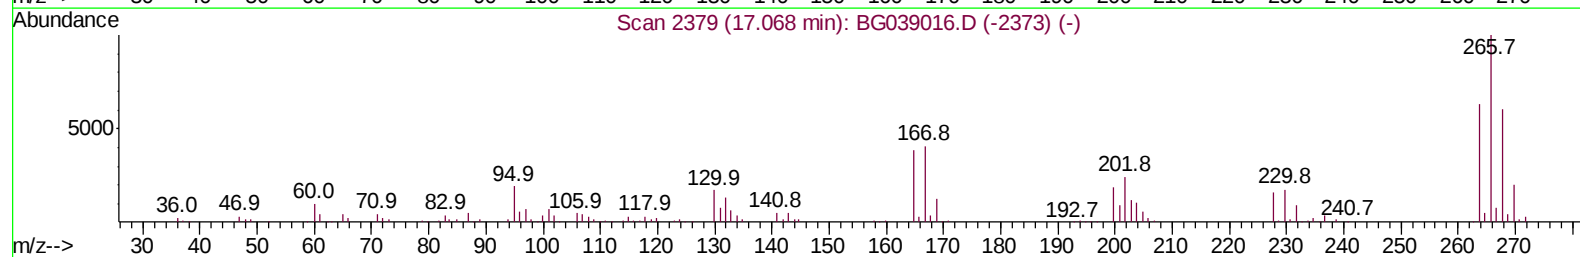
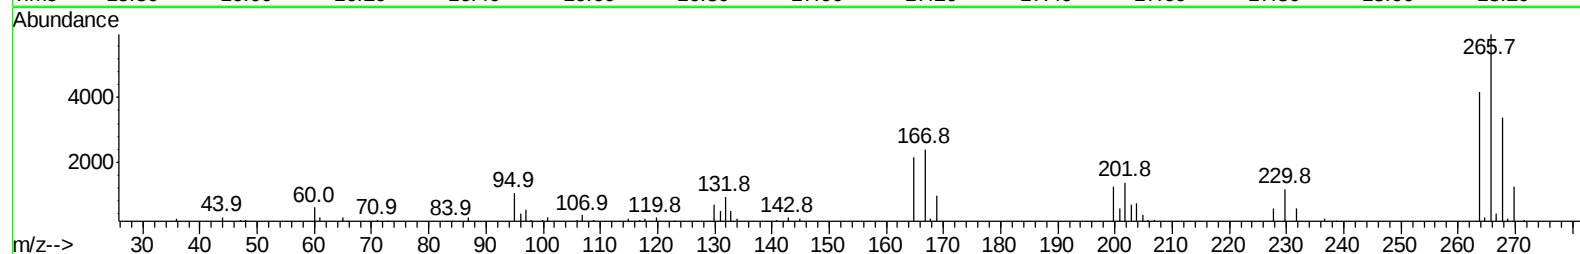


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011719\
Data File : BG039197.D
Acq On : 17 Jan 2019 23:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 05:58:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

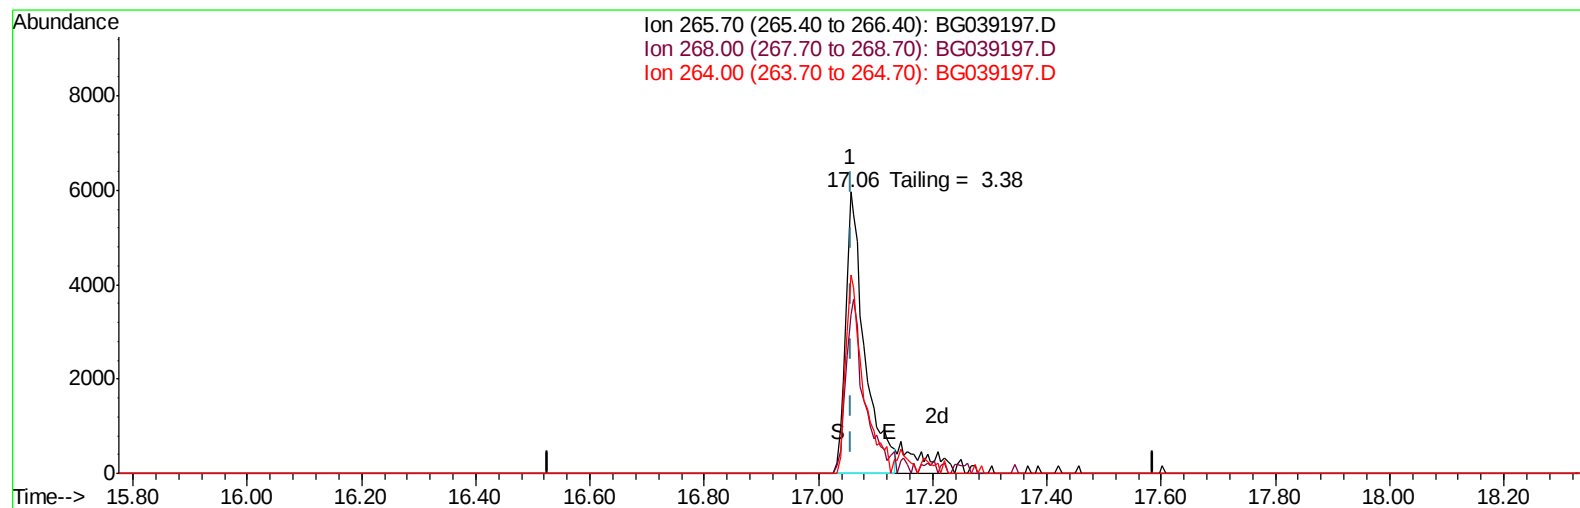

TIC: BG039197.D

(70) Pentachlorophenol (C)




17.056min (-0.002) 0.00ng

response 13934

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.43
264.00	68.20	74.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011719\
Data File : BG039197.D
Acq On : 17 Jan 2019 23:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 05:58:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

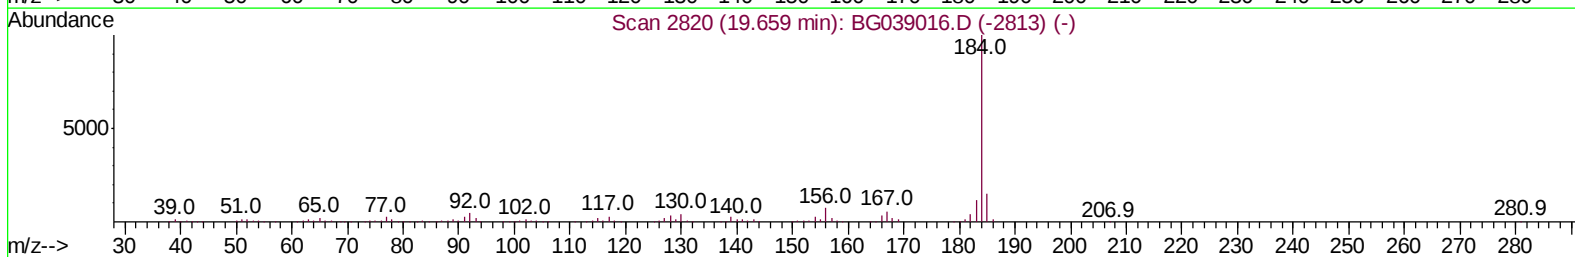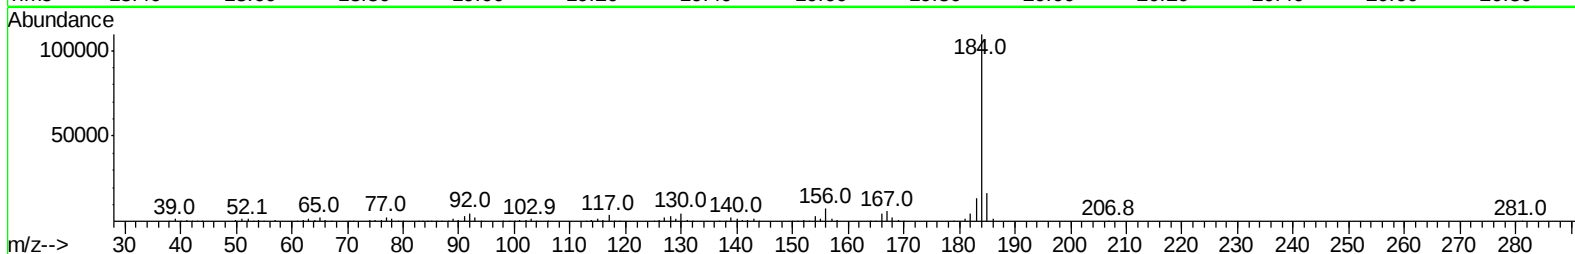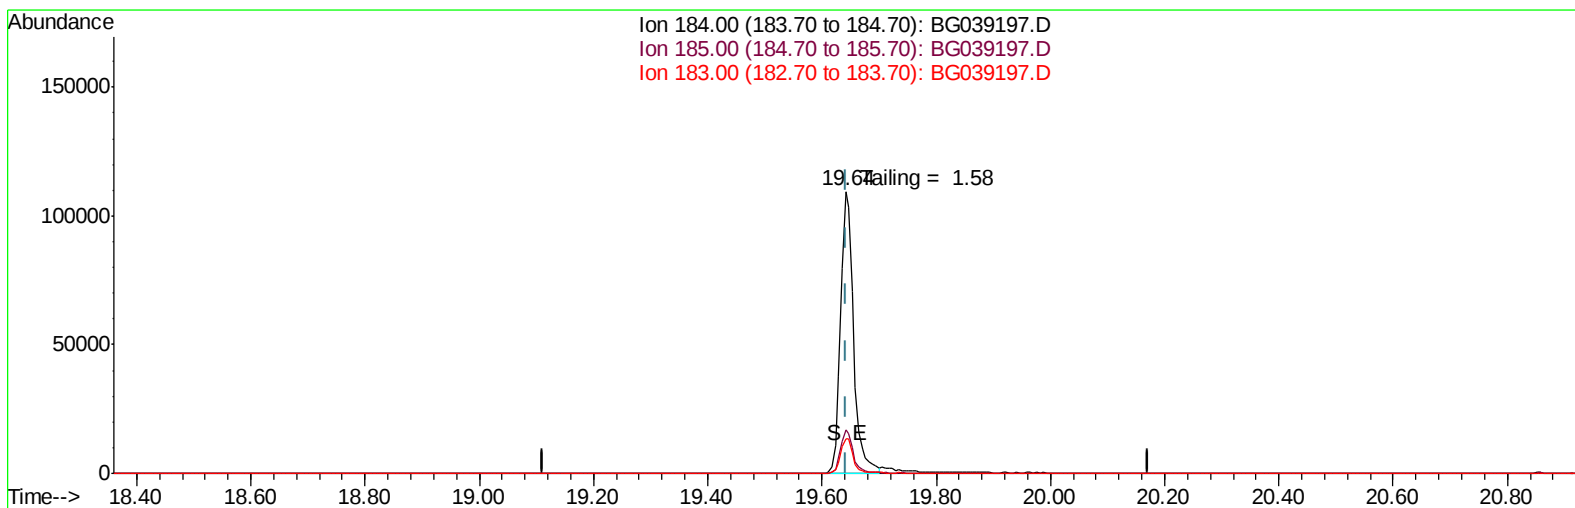

TIC: BG039197.D

(77) Benzidine

19.641min (-0.002) 0.00ng

response 179765

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.49
183.00	11.90	12.41
0.00	0.00	0.00