


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011719\
 Data File : BG039197.D
 Acq On : 17 Jan 2019 23:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 04:20:14 2019

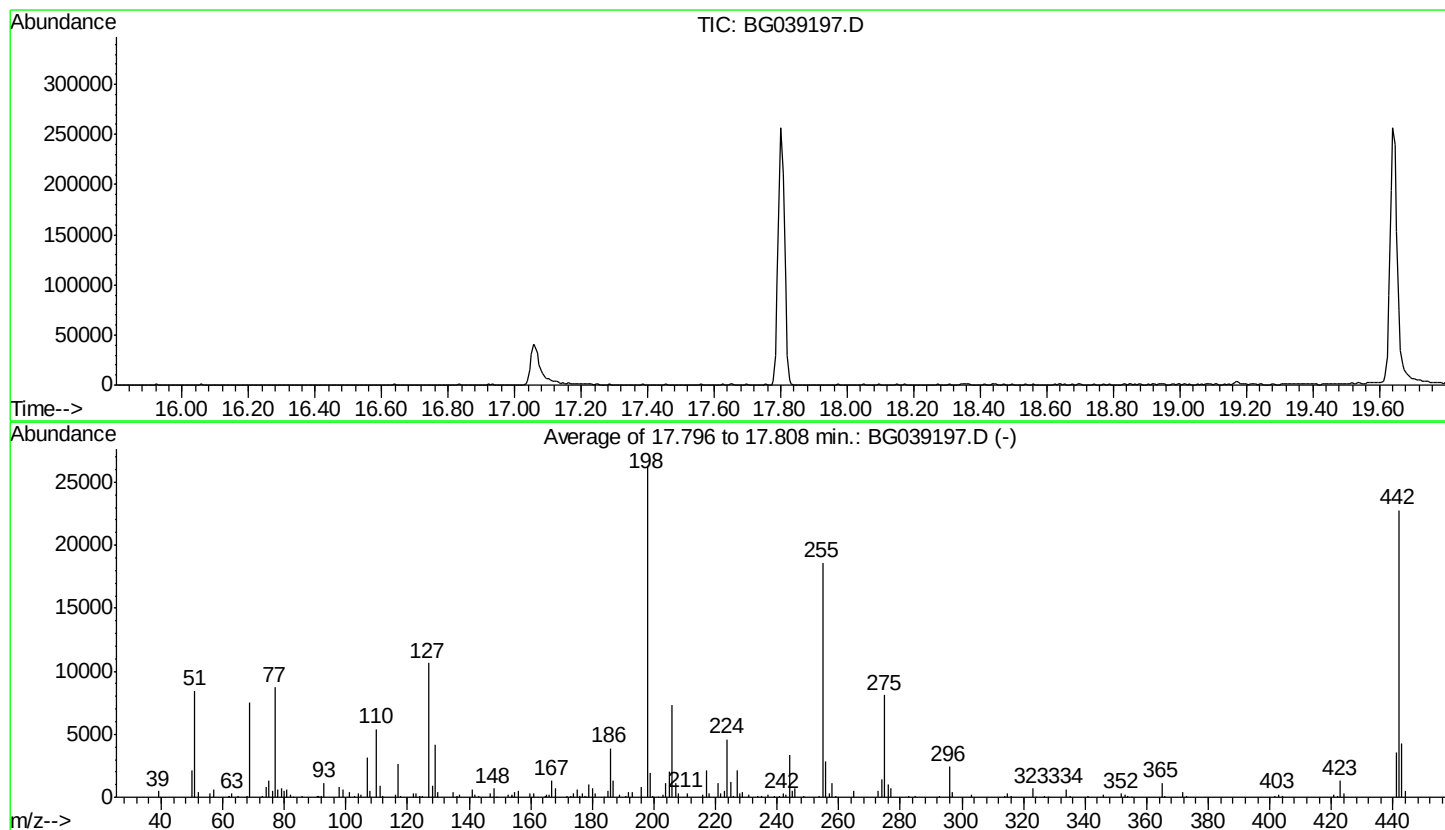

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	8433	PASS
68	69	0.00	2	0.8	60	PASS
69	198	0.00	100	28.7	7542	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	10665	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26317	PASS
199	198	5	9	7.3	1920	PASS
275	198	10	60	30.8	8118	PASS
365	198	1	100	4.3	1135	PASS
441	198	0.01	100	13.5	3545	PASS
442	198	50	100	86.6	22800	PASS
443	442	15	24	18.8	4291	PASS