
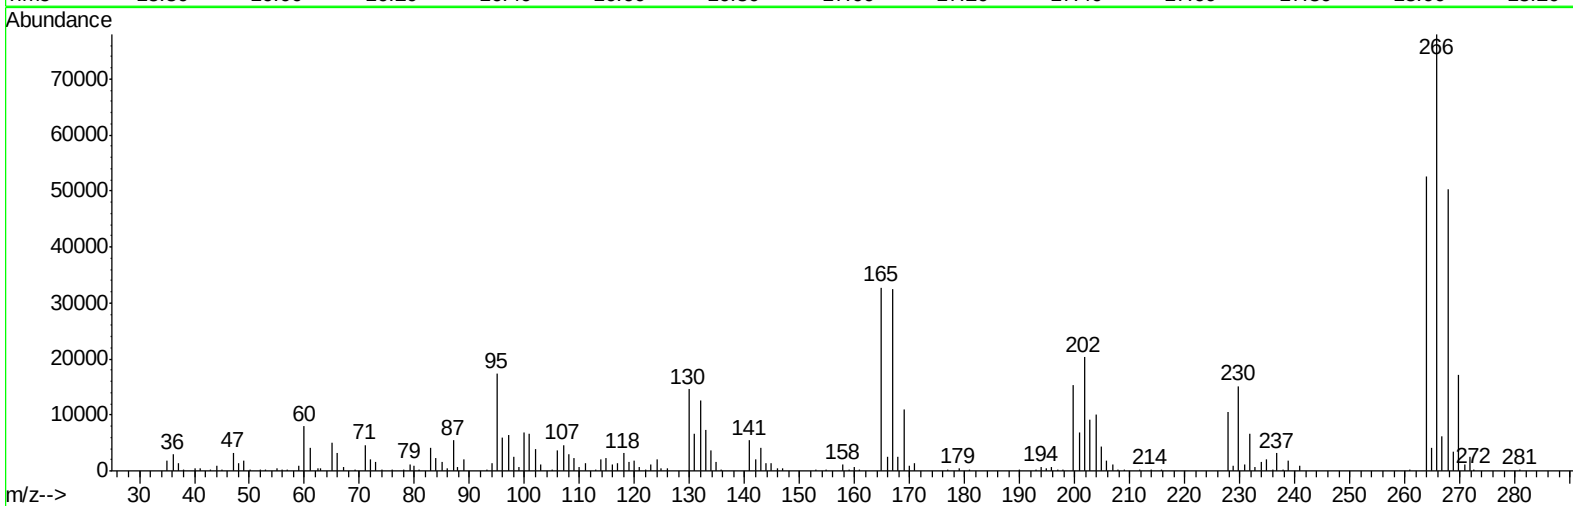


Data File : BG044074.D
Acq On : 17 Jan 2020 13:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 04:27:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

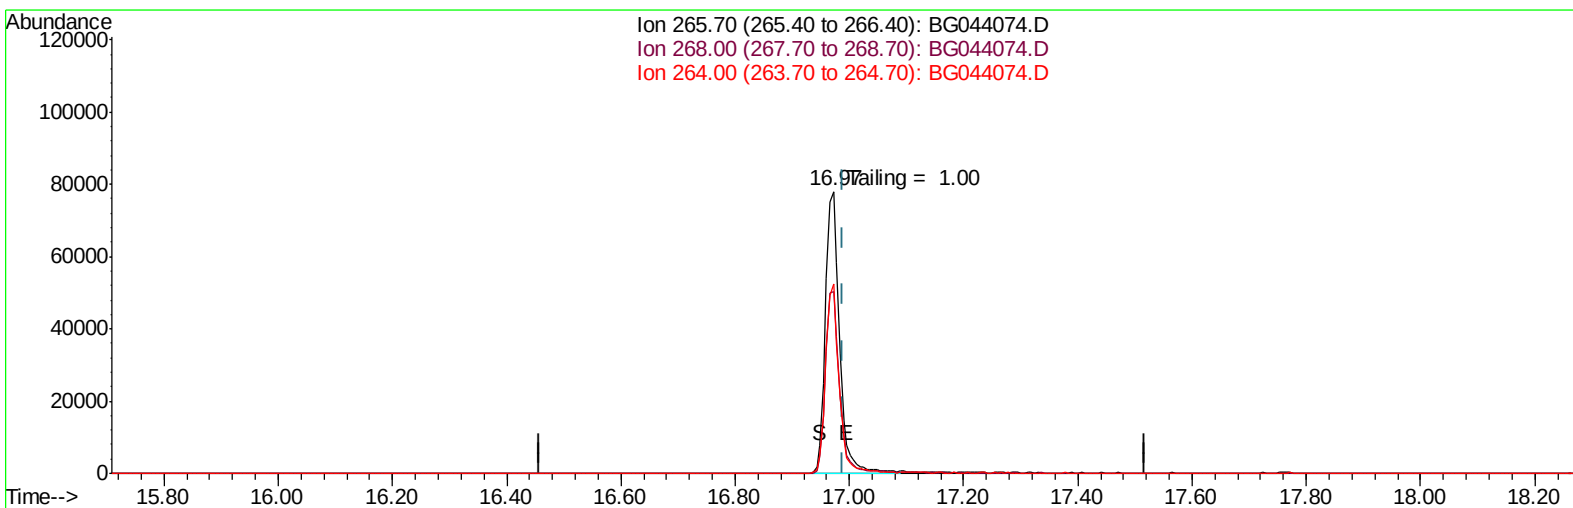

TIC: BG044074.D

(70) Pentachlorophenol (C)



16.972min (-0.017) 32062.19ng

response 134942

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	64.47
264.00	63.50	67.42
0.00	0.00	0.00

Data File : BG044074.D
Acq On : 17 Jan 2020 13:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 04:27:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

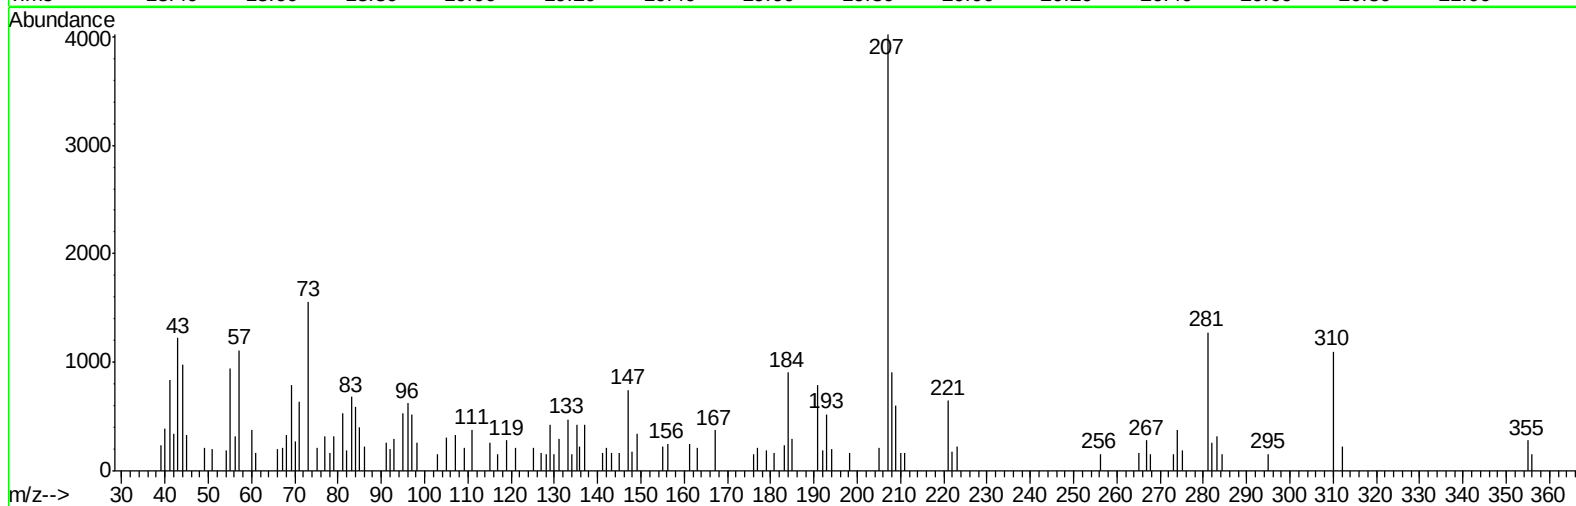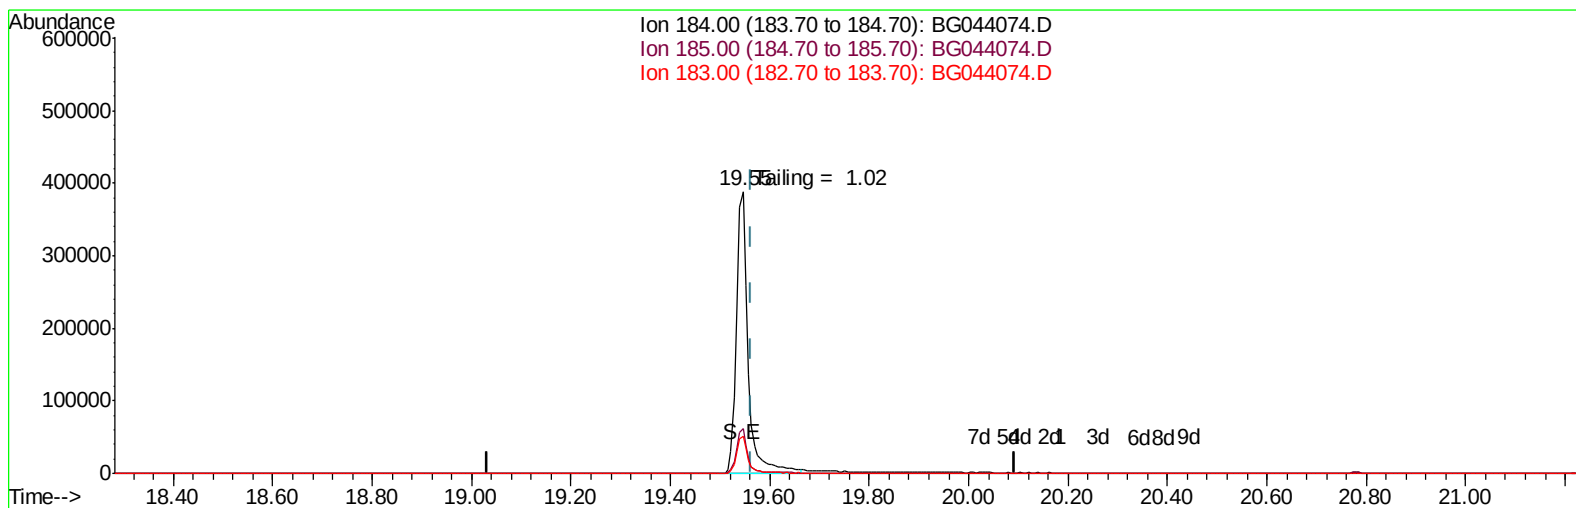

TIC: BG044074.D

(77) Benzidine

20.186min (+0.623) 433.36ng

response 610

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	32.63#
183.00	13.20	25.66#
0.00	0.00	0.00