

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052039.D
 Acq On : 18 Jan 2022 1:03
 Operator : CG/JU
 Sample : N1169-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLX8

Quant Time: Jan 18 01:52:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.241	152	23743	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.084	136	107197	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.891	164	83528	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.640	188	203270	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.963	240	199254	20.000	ng/ul	# 0.00
88) Perylene-d12	25.453	264	202452	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.571	96	2438	3.669	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.383	99	55624	23.937	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	35489	24.058	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.771	132	39365	25.586	ng/ul	0.00
15) 4-Methylphenol-d8	8.946	113	44174	24.454	ng/ul	0.00
21) Nitrobenzene-d5	9.416	128	22602	26.683	ng/ul	0.00
24) 2-Nitrophenol-d4	10.150	143	22600	24.125	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.696	165	44926	24.535	ng/ul	0.00
31) 4-Chloroaniline-d4	11.207	131	47723	18.714	ng/ul	0.00
46) Dimethylphthalate-d6	14.280	166	157770	22.851	ng/ul	0.00
49) Acenaphthylene-d8	14.585	160	212744	25.509	ng/ul	0.00
54) 4-Nitrophenol-d4	15.067	143	18037	15.626	ng/ul	0.00
60) Fluorene-d10	15.878	176	156523	26.002	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.989	200	14951	11.659	ng/ul	0.00
73) Anthracene-d10	17.740	188	259959	26.959	ng/ul	0.00
81) Pyrene-d10	20.019	212	302107	26.345	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.212	264	282898	26.543	ng/ul	0.02
Target Compounds						
					Qvalue	
8) Phenol	7.413	94	3548	1.496	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052039.D
Acq On : 18 Jan 2022 1:03
Operator : CG/JU
Sample : N1169-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLX8


Quant Time: Jan 18 01:52:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

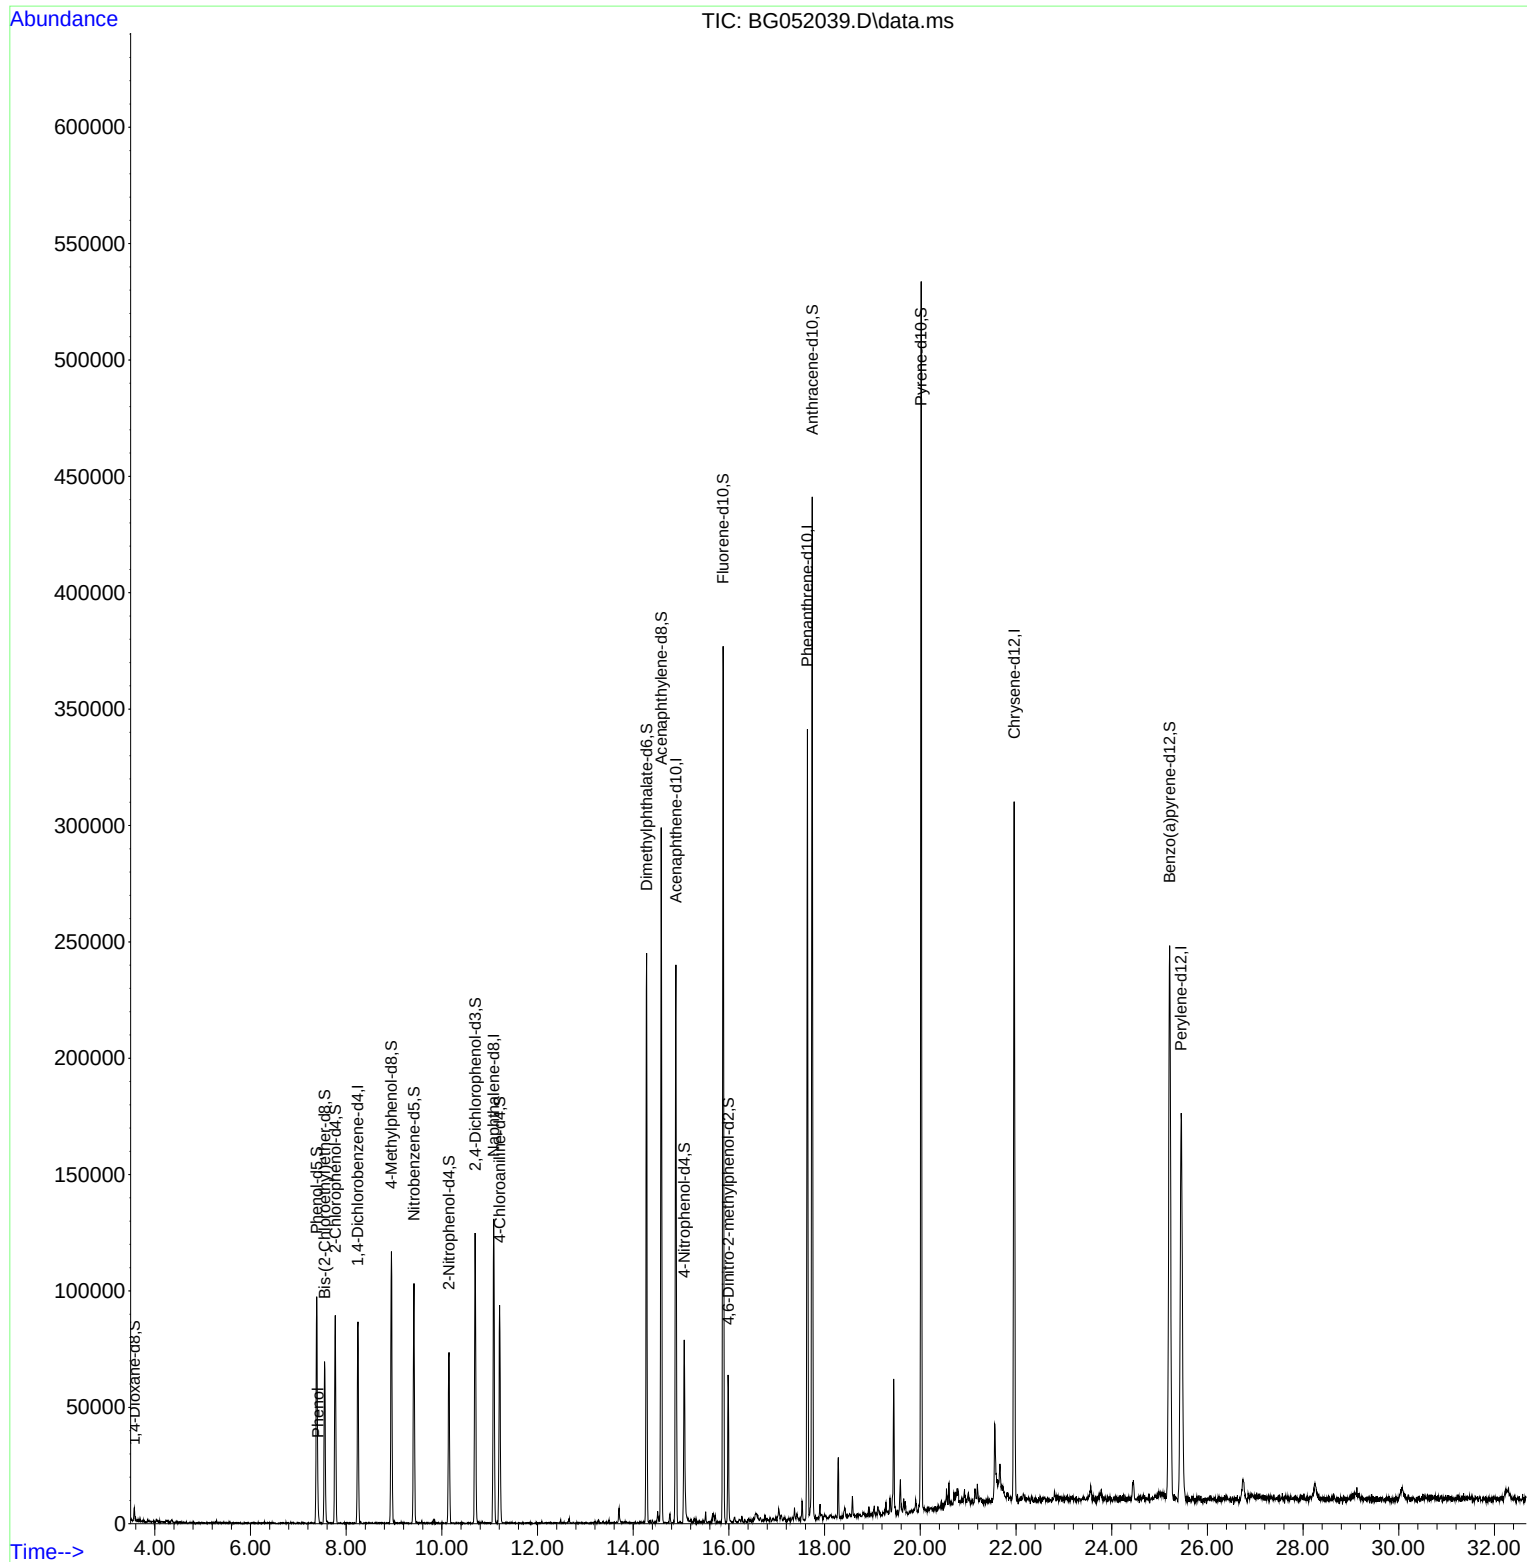

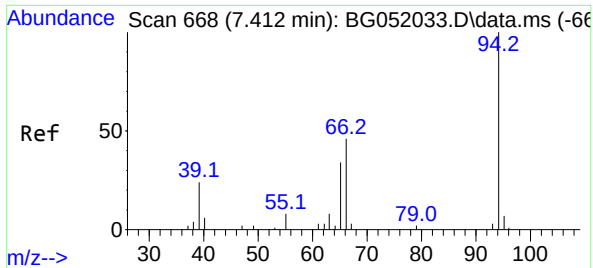

#8
Phenol
Concen: 1.496 ng/ul
RT: 7.413 min Scan# 60
Delta R.T. -0.006 min
Lab File: BG052039.D
Acq: 18 Jan 2022 1:03

Instrument :
BNA_G
ClientSampleId :
BGLX8

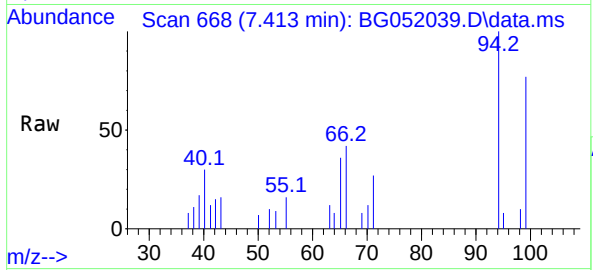

Tgt Ion: 94 Resp: 3548
Ion Ratio Lower Upper
94 100
65 36.3 25.1 37.7
66 42.1 31.6 47.4

