

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052047.D
 Acq On : 18 Jan 2022 11:06
 Operator : CG/JU
 Sample : N1169-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLX2

Quant Time: Jan 18 11:41:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.245	152	24572	20.000	ng/u1	0.00
20) Naphthalene-d8	11.083	136	108763	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.889	164	81300	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.639	188	195226	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.956	240	184761	20.000	ng/u1	# 0.00
88) Perylene-d12	25.452	264	189444	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.569	96	3100	4.508	ng/uL	0.00
4) Pyridine-d5	3.998	84	38628	18.070	ng/u1	0.00
7) Phenol-d5	7.382	99	62906	26.157	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.546	67	37750	24.727	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.770	132	43804	27.510	ng/u1	0.00
15) 4-Methylphenol-d8	8.944	113	51651	27.628	ng/u1	0.00
21) Nitrobenzene-d5	9.414	128	24327	28.306	ng/u1	0.00
24) 2-Nitrophenol-d4	10.149	143	27403	28.830	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.695	165	52105	28.046	ng/u1	0.00
31) 4-Chloroaniline-d4	11.206	131	65121	25.169	ng/u1	0.00
46) Dimethylphthalate-d6	14.278	166	180241	26.821	ng/u1	0.00
49) Acenaphthylene-d8	14.584	160	227030	27.968	ng/u1	0.00
54) 4-Nitrophenol-d4	15.060	143	25398	22.605	ng/u1	0.00
60) Fluorene-d10	15.876	176	162334	27.706	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.982	200	27425	22.268	ng/u1	0.00
73) Anthracene-d10	17.738	188	266007	28.723	ng/u1	0.00
81) Pyrene-d10	20.018	212	310267	29.179	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.205	264	285836	28.660	ng/u1	0.01
Target Compounds						
8) Phenol	7.411	94	3109	1.267	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052047.D
Acq On : 18 Jan 2022 11:06
Operator : CG/JU
Sample : N1169-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLX2

Quant Time: Jan 18 11:41:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

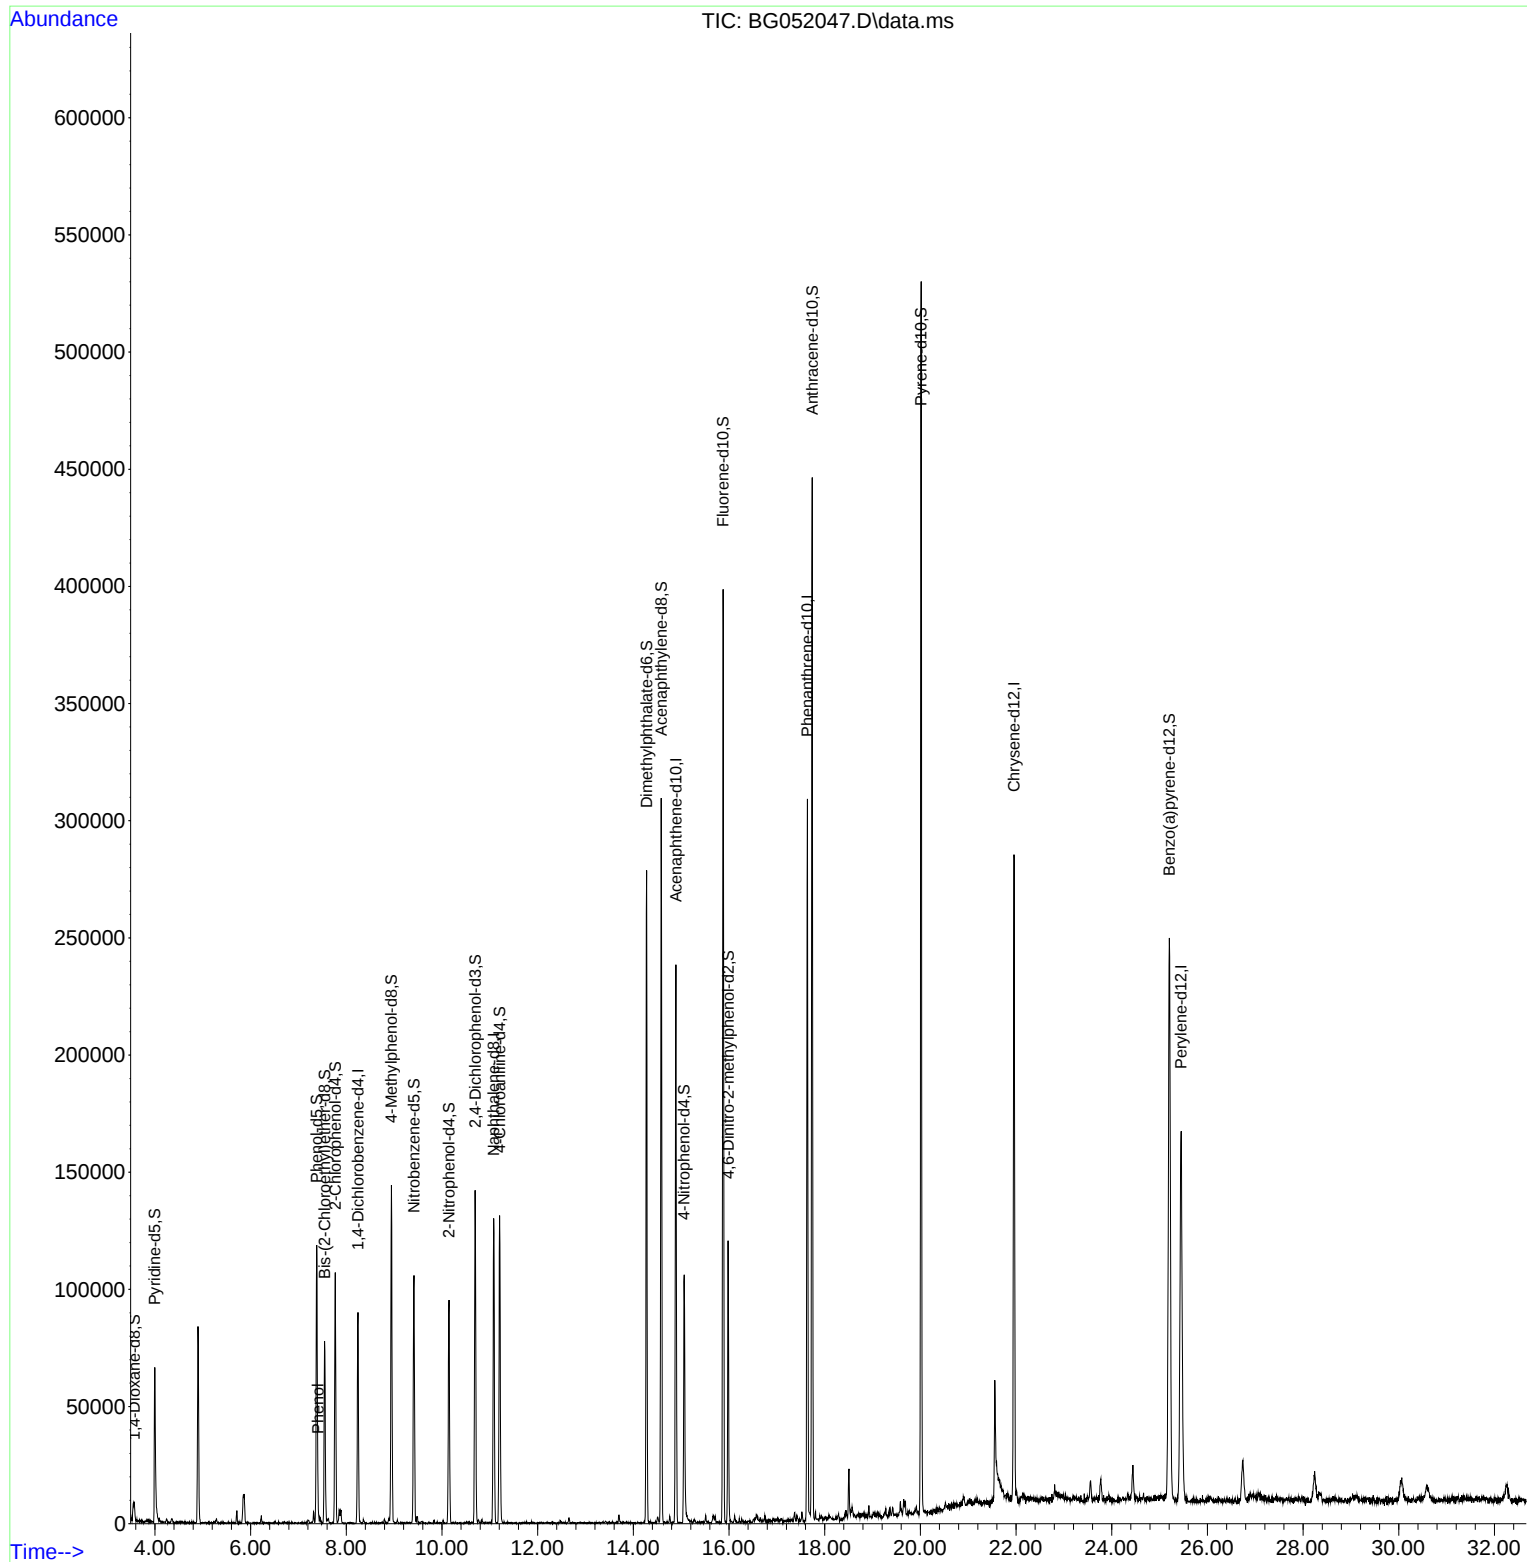

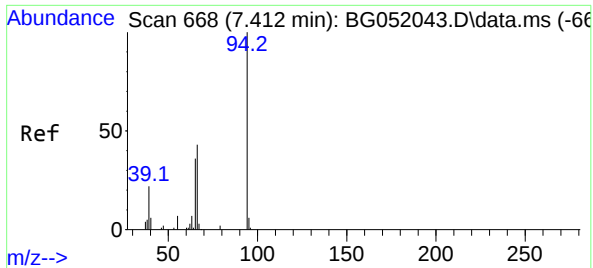

#8
Phenol
Concen: 1.267 ng/ul
RT: 7.411 min Scan# 60
Delta R.T. -0.007 min
Lab File: BG052047.D
Acq: 18 Jan 2022 11:06

Instrument :
BNA_G
ClientSampleId :
BGLX2

Tgt Ion: 94 Resp: 3109

Ion	Ratio	Lower	Upper
94	100		
65	34.6	25.1	37.7
66	45.4	31.6	47.4

