

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052018.D
 Acq On : 17 Jan 2022 10:59
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.518	4	5	9	rVB2	1466	1395	0.13%	0.014%
2	3.571	9	14	23	rVB2	8910	13845	1.33%	0.138%
3	3.794	49	52	56	rBV2	1039	1385	0.13%	0.014%
4	4.000	82	87	103	rBV	106263	182633	17.50%	1.824%
5	4.105	103	105	110	rVB3	1002	1141	0.11%	0.011%
6	4.358	143	148	153	rBV2	7657	12558	1.20%	0.125%
7	4.998	254	257	261	rBB2	941	1400	0.13%	0.014%
8	7.389	657	664	672	rBV	143618	253115	24.25%	2.527%
9	7.554	684	692	699	rBV	97088	169492	16.24%	1.692%
10	7.777	723	730	739	rBV	135561	231273	22.16%	2.309%
11	8.247	803	810	817	rBV	94157	158850	15.22%	1.586%
12	8.952	923	930	941	rBV	171359	298863	28.63%	2.984%
13	9.422	1002	1010	1020	rVB	137457	244490	23.43%	2.441%
14	10.150	1127	1134	1144	rVV	122421	219447	21.03%	2.191%
15	10.702	1220	1228	1237	rVB	177763	319509	30.61%	3.190%
16	11.090	1287	1294	1301	rBV	137091	244056	23.38%	2.437%
17	11.213	1308	1315	1324	rBV	172629	315677	30.25%	3.152%
18	12.664	1556	1562	1567	rVB4	2820	4647	0.45%	0.046%
19	14.286	1831	1838	1845	rVB	353271	528740	50.66%	5.280%
20	14.591	1881	1890	1897	rBV	389282	619547	59.36%	6.186%
21	14.897	1935	1942	1949	rVB	241489	379036	36.32%	3.785%
22	15.073	1965	1972	1989	rBV	164372	294117	28.18%	2.937%
23	15.179	1989	1990	1995	rVV3	1217	1446	0.14%	0.014%
24	15.884	2104	2110	2117	rVB	517589	777854	74.53%	7.767%
25	15.989	2123	2128	2136	rBV	168113	249195	23.88%	2.488%
26	16.130	2148	2152	2155	rVB2	1020	1468	0.14%	0.015%
27	17.646	2402	2410	2417	rBV	335187	510951	48.96%	5.102%
28	17.746	2420	2427	2435	rVV	607777	918652	88.02%	9.173%
29	19.297	2688	2691	2694	rBV4	1200	1422	0.14%	0.014%
30	19.355	2699	2701	2703	rBV2	2496	1762	0.17%	0.018%
31	19.385	2703	2706	2707	rBV4	1213	1098	0.11%	0.011%
32	19.420	2710	2712	2713	rBV	3271	1362	0.13%	0.014%
33	19.444	2713	2716	2718	rBV2	1934	2187	0.21%	0.022%
34	19.514	2725	2728	2729	rBV2	1030	1147	0.11%	0.011%
35	19.549	2733	2734	2737	rVV3	1962	2007	0.19%	0.020%
36	19.590	2737	2741	2745	rVV4	9672	13933	1.33%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052018.D
 Acq On : 17 Jan 2022 10:59
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.661	2748	2753	2760	rVV2	7708	11482	1.10%	0.115%
38	19.755	2768	2769	2771	rBV2	2503	1549	0.15%	0.015%
39	19.778	2771	2773	2775	rVV3	1816	1491	0.14%	0.015%
40	20.025	2807	2815	2821	rBV	750541	1043702	100.00%	10.422%
41	20.143	2833	2835	2837	rBV3	1793	1687	0.16%	0.017%
42	20.160	2837	2838	2840	rBV2	1714	1506	0.14%	0.015%
43	20.260	2853	2855	2857	rBV3	1838	1553	0.15%	0.016%
44	20.430	2882	2884	2885	rVB2	3461	1763	0.17%	0.018%
45	20.448	2885	2887	2889	rBV3	1629	1998	0.19%	0.020%
46	20.530	2899	2901	2904	rBV4	2961	2946	0.28%	0.029%
47	20.707	2930	2931	2932	rBV	2971	1412	0.14%	0.014%
48	20.795	2944	2946	2950	rBV5	3540	4065	0.39%	0.041%
49	21.394	3046	3048	3049	rBV2	3689	2812	0.27%	0.028%
50	21.511	3066	3068	3070	rBV2	4237	2808	0.27%	0.028%
51	21.805	3117	3118	3119	rVB	7081	2496	0.24%	0.025%
52	21.970	3140	3146	3153	rVB2	272005	474319	45.45%	4.736%
53	22.486	3231	3234	3237	rBV5	3728	4282	0.41%	0.043%
54	22.563	3245	3247	3248	rBV2	4993	3456	0.33%	0.035%
55	22.627	3257	3258	3261	rVB3	3644	3267	0.31%	0.033%
56	22.792	3284	3286	3289	rBV4	3781	5438	0.52%	0.054%
57	23.462	3398	3400	3402	rBV3	3212	2859	0.27%	0.029%
58	23.567	3416	3418	3427	rVB9	5776	8097	0.78%	0.081%
59	24.590	3590	3592	3595	rBV4	4544	6243	0.60%	0.062%
60	25.230	3690	3701	3713	rVB	297106	910768	87.26%	9.094%
61	25.471	3732	3742	3755	rVB2	149167	477935	45.79%	4.772%
62	25.688	3777	3779	3780	rBV2	4257	2296	0.22%	0.023%
63	26.898	3983	3985	3987	rBV3	5127	3114	0.30%	0.031%
64	27.204	4035	4037	4038	rBV2	3620	2604	0.25%	0.026%
65	28.332	4227	4229	4232	rBV3	3908	4245	0.41%	0.042%
66	29.254	4384	4386	4391	rBV6	4441	8098	0.78%	0.081%
67	29.518	4429	4431	4432	rBV2	3966	2768	0.27%	0.028%
68	30.370	4574	4576	4579	rBV4	3646	4959	0.48%	0.050%
69	30.417	4582	4584	4587	rBV3	3433	3461	0.33%	0.035%
70	30.493	4596	4597	4600	rBV3	4126	4417	0.42%	0.044%
71	30.593	4611	4614	4615	rBV3	4637	3793	0.36%	0.038%
72	30.852	4656	4658	4661	rVB4	4002	3136	0.30%	0.031%
73	30.934	4670	4672	4673	rBV2	3253	1794	0.17%	0.018%
74	31.333	4738	4740	4742	rBV3	3577	3161	0.30%	0.032%
75	31.580	4780	4782	4783	rVB2	4399	2034	0.19%	0.020%
76	31.633	4789	4791	4792	rBV3	3797	2858	0.27%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052018.D
Acq On : 17 Jan 2022 10:59
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	32.585	4951	4953	4954	rBV2	3143	2270	0.22%	0.023%
----	--------	------	------	------	------	------	------	-------	--------




Sum of corrected areas: 10014642

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052018.D
Acq On : 17 Jan 2022 10:59
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

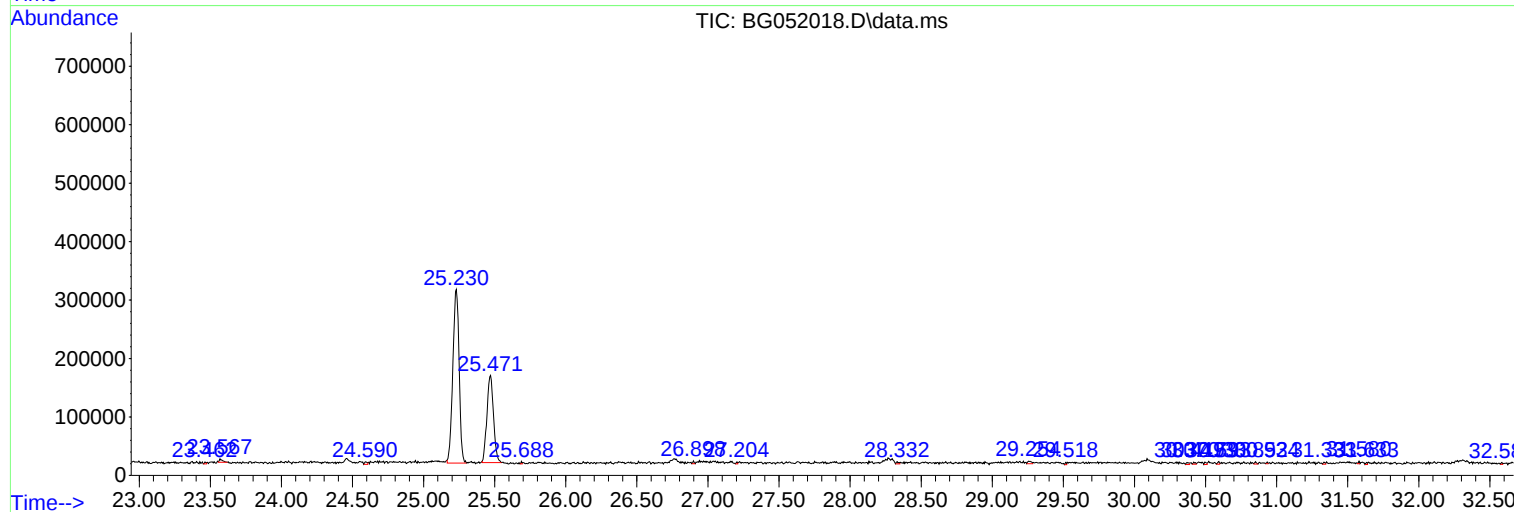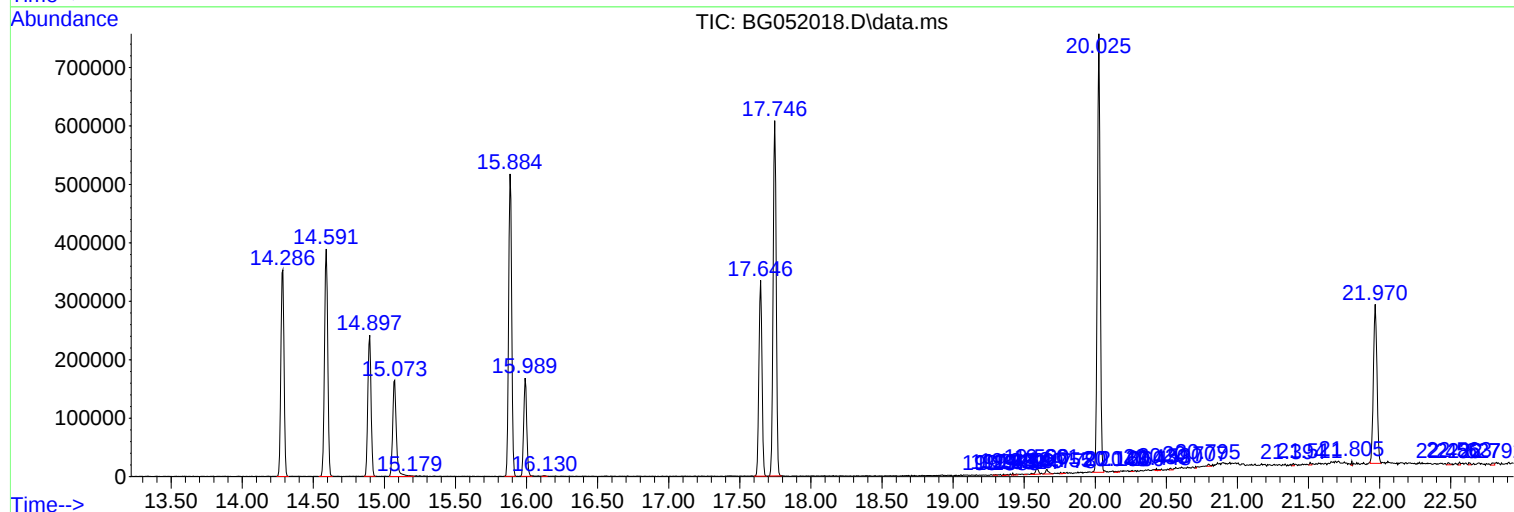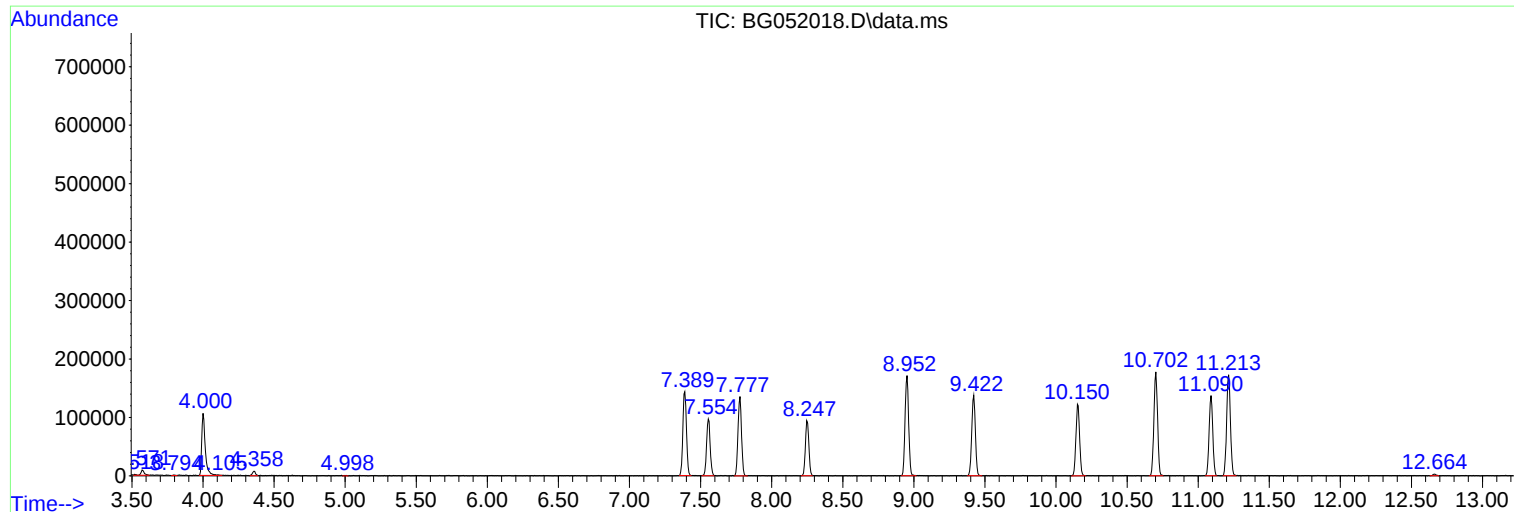

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052018.D
Acq On : 17 Jan 2022 10:59
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052018.D
Acq On : 17 Jan 2022 10:59
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc