

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052019.D
 Acq On : 17 Jan 2022 11:49
 Operator : CG/JU
 Sample : N1132-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.582	11	16	22	rVB2	6725	10603	1.38%	0.126%
2	4.005	84	88	102	rBV	85190	147086	19.17%	1.747%
3	4.246	127	129	132	rBV3	1610	2185	0.28%	0.026%
4	4.352	145	147	148	rBV	2139	1459	0.19%	0.017%
5	4.369	148	150	154	rVB	1851	2282	0.30%	0.027%
6	5.298	304	308	314	rBV2	2965	4467	0.58%	0.053%
7	5.685	370	374	378	rVB	826	1151	0.15%	0.014%
8	5.956	417	420	424	rBV	681	1101	0.14%	0.013%
9	7.401	658	666	677	rBV2	124245	234184	30.52%	2.781%
10	7.565	688	694	702	rVB	84774	140766	18.34%	1.672%
11	7.788	725	732	745	rBV	113579	190911	24.88%	2.267%
12	8.258	806	812	819	rBV	99258	169579	22.10%	2.014%
13	8.963	925	932	943	rBV	137969	250147	32.60%	2.971%
14	9.087	949	953	957	rVB	948	1288	0.17%	0.015%
15	9.427	1004	1011	1019	rVB	115914	206018	26.85%	2.447%
16	9.586	1036	1038	1043	rVB3	1969	2059	0.27%	0.024%
17	9.856	1079	1084	1089	rVB2	4253	6530	0.85%	0.078%
18	10.162	1129	1136	1145	rVB	100081	178583	23.27%	2.121%
19	10.714	1222	1230	1238	rBV	146951	262970	34.27%	3.123%
20	10.843	1248	1252	1262	rBV2	4095	8636	1.13%	0.103%
21	11.101	1288	1296	1303	rBV	143793	256790	33.46%	3.050%
22	11.225	1309	1317	1327	rBV	141615	263310	34.31%	3.127%
23	12.494	1526	1533	1535	rBV3	1508	1617	0.21%	0.019%
24	12.670	1557	1563	1570	rBV3	2594	4243	0.55%	0.050%
25	13.710	1737	1740	1745	rVV2	3329	4498	0.59%	0.053%
26	13.780	1748	1752	1754	rVB	1314	1397	0.18%	0.017%
27	14.291	1832	1839	1848	rBV	278070	409844	53.41%	4.868%
28	14.520	1874	1878	1884	rBV3	2481	3660	0.48%	0.043%
29	14.597	1884	1891	1899	rVV	317944	499572	65.10%	5.933%
30	14.773	1917	1921	1925	rVB	3551	4250	0.55%	0.050%
31	14.902	1936	1943	1952	rBV	246409	393390	51.27%	4.672%
32	15.078	1962	1973	1980	rBV	119015	209233	27.27%	2.485%
33	15.225	1996	1998	2002	rVB2	1340	1272	0.17%	0.015%
34	15.525	2044	2049	2053	rVB3	2879	3512	0.46%	0.042%
35	15.725	2080	2083	2087	rVB3	4242	4822	0.63%	0.057%
36	15.889	2103	2111	2118	rBV	408093	617756	80.51%	7.337%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052019.D
 Acq On : 17 Jan 2022 11:49
 Operator : CG/JU
 Sample : N1132-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.995	2123	2129	2135	rBV	112395	168401	21.95%	2.000%
38	16.101	2143	2147	2148	rBV	1108	1105	0.14%	0.013%
39	16.136	2151	2153	2156	rVB2	2429	2092	0.27%	0.025%
40	16.283	2174	2178	2180	rBV3	3524	3564	0.46%	0.042%
41	16.524	2216	2219	2222	rVB3	1236	1254	0.16%	0.015%
42	16.565	2222	2226	2228	rBV4	4851	6628	0.86%	0.079%
43	16.770	2257	2261	2263	rVB3	2189	2919	0.38%	0.035%
44	16.806	2265	2267	2271	rVB2	841	1203	0.16%	0.014%
45	16.847	2271	2274	2275	rBV	899	1104	0.14%	0.013%
46	16.929	2286	2288	2291	rVB2	1005	1065	0.14%	0.013%
47	16.988	2297	2298	2301	rVB2	1555	1153	0.15%	0.014%
48	17.035	2304	2306	2308	rVB	1368	1241	0.16%	0.015%
49	17.322	2354	2355	2359	rBV3	1520	1549	0.20%	0.018%
50	17.375	2361	2364	2370	rVV4	4822	8068	1.05%	0.096%
51	17.440	2370	2375	2377	rVV4	3740	6012	0.78%	0.071%
52	17.463	2377	2379	2381	rVB2	1478	1363	0.18%	0.016%
53	17.534	2388	2391	2392	rBV2	2076	1587	0.21%	0.019%
54	17.651	2404	2411	2418	rBV	337226	515563	67.19%	6.123%
55	17.745	2421	2427	2435	rVV2	440965	691780	90.15%	8.216%
56	17.822	2437	2440	2444	rVV3	5997	7651	1.00%	0.091%
57	17.881	2448	2450	2453	rVB	1263	1099	0.14%	0.013%
58	18.127	2490	2492	2494	rVB3	3268	2683	0.35%	0.032%
59	18.186	2498	2502	2508	rBV6	2032	4072	0.53%	0.048%
60	18.245	2508	2512	2514	rBV3	1226	1206	0.16%	0.014%
61	18.298	2518	2521	2527	rVB3	3561	5584	0.73%	0.066%
62	18.350	2527	2530	2532	rBV3	1606	1887	0.25%	0.022%
63	18.433	2540	2544	2545	rBV4	1436	1249	0.16%	0.015%
64	18.515	2555	2558	2561	rBV4	5968	7707	1.00%	0.092%
65	18.914	2624	2626	2628	rBV3	1249	1193	0.16%	0.014%
66	18.932	2628	2629	2631	rVV2	1611	1095	0.14%	0.013%
67	19.020	2643	2644	2646	rBV2	1744	1467	0.19%	0.017%
68	19.179	2669	2671	2673	rBV2	1231	1152	0.15%	0.014%
69	19.243	2680	2682	2685	rBV3	1424	1425	0.19%	0.017%
70	19.379	2703	2705	2707	rVB3	2468	2383	0.31%	0.028%
71	19.420	2710	2712	2714	rVV3	1853	1329	0.17%	0.016%
72	19.590	2738	2741	2746	rBV5	7151	8111	1.06%	0.096%
73	19.660	2750	2753	2759	rBV2	4892	8286	1.08%	0.098%
74	19.931	2797	2799	2802	rVB4	4190	3409	0.44%	0.040%
75	20.025	2809	2815	2824	rVB	529261	767341	100.00%	9.114%
76	21.975	3141	3147	3155	rVB	280107	490725	63.95%	5.828%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052019.D
Acq On : 17 Jan 2022 11:49
Operator : CG/JU
Sample : N1132-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	25.235	3692	3702	3713	rVB2	216906	660203	86.04%	7.841%
78	25.476	3734	3743	3760	rVB	161527	519644	67.72%	6.172%




Sum of corrected areas: 8419723

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052019.D
Acq On : 17 Jan 2022 11:49
Operator : CG/JU
Sample : N1132-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

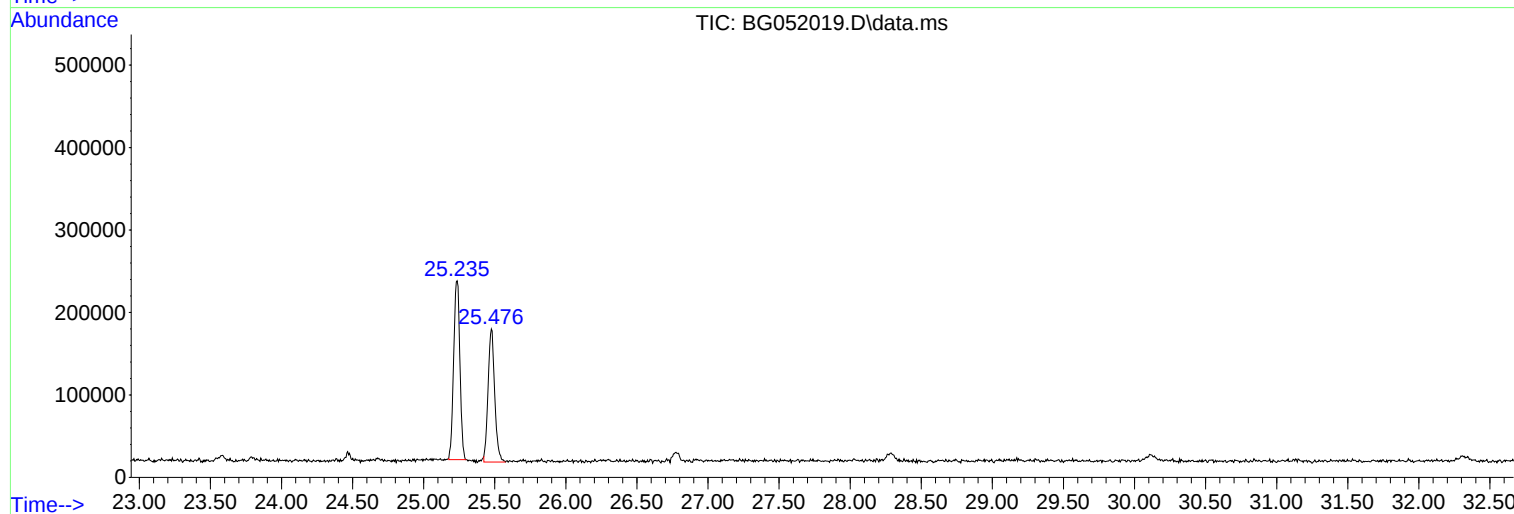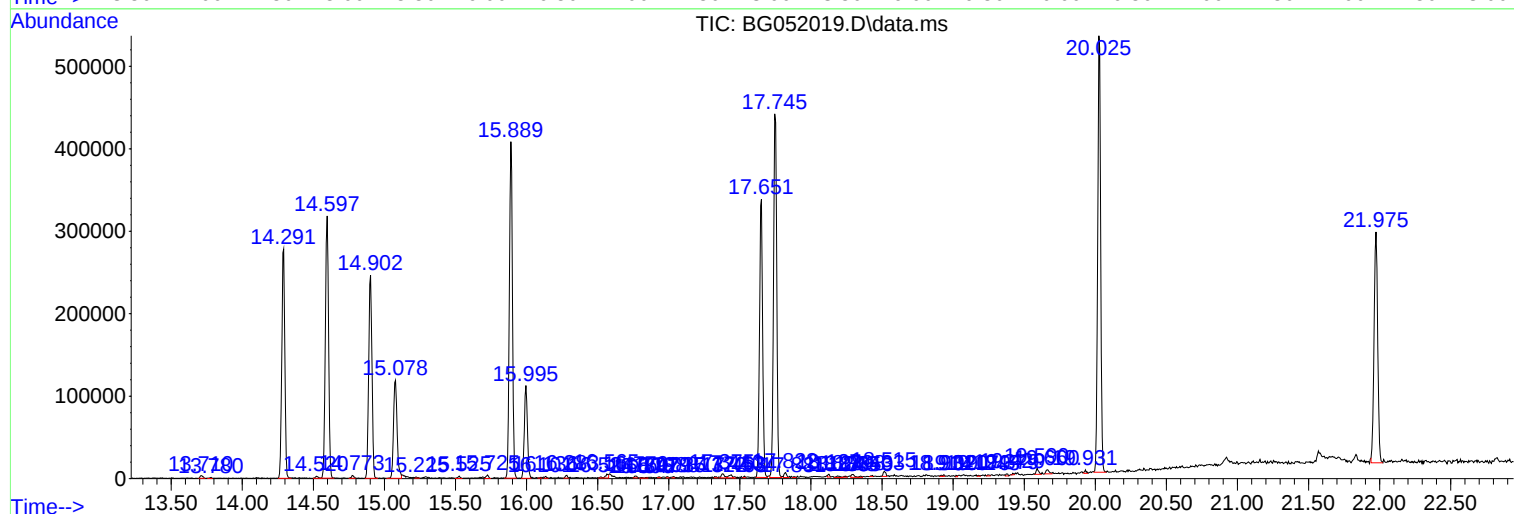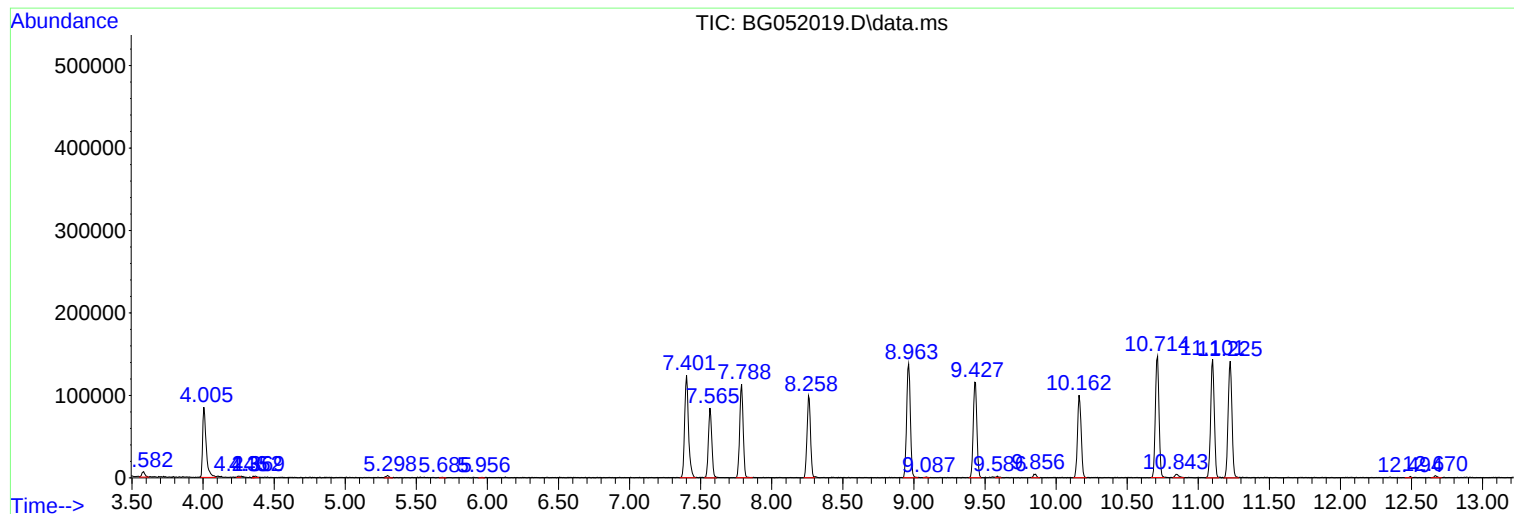

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052019.D
Acq On : 17 Jan 2022 11:49
Operator : CG/JU
Sample : N1132-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052019.D
Acq On : 17 Jan 2022 11:49
Operator : CG/JU
Sample : N1132-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc