

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052024.D
 Acq On : 17 Jan 2022 14:58
 Operator : CG/JU
 Sample : N1169-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	7	14	18	rBV3	6824	10122	1.55%	0.135%
2	3.861	57	63	64	rBV3	1225	1748	0.27%	0.023%
3	3.920	71	73	75	rBV	746	922	0.14%	0.012%
4	4.002	83	87	100	rVB	31955	55743	8.54%	0.744%
5	4.173	112	116	118	rVB3	1487	1616	0.25%	0.022%
6	4.243	126	128	129	rBV	1120	1099	0.17%	0.015%
7	4.355	143	147	149	rBV2	1762	1846	0.28%	0.025%
8	4.543	177	179	181	rBV2	973	1084	0.17%	0.014%
9	4.795	220	222	225	rVB2	1211	1372	0.21%	0.018%
10	5.230	294	296	299	rBV	1084	928	0.14%	0.012%
11	5.289	303	306	310	rVV3	1895	2465	0.38%	0.033%
12	5.506	339	343	347	rBV	483	1027	0.16%	0.014%
13	5.876	404	406	410	rBB	753	1015	0.16%	0.014%
14	5.999	423	427	430	rVV	690	974	0.15%	0.013%
15	6.070	434	439	442	rBB2	574	1026	0.16%	0.014%
16	6.193	457	460	463	rBV2	820	1277	0.20%	0.017%
17	6.569	522	524	529	rVB	960	919	0.14%	0.012%
18	6.616	529	532	536	rBV	652	1081	0.17%	0.014%
19	7.386	655	663	675	rVB	105409	187654	28.74%	2.506%
20	7.550	685	691	699	rBV	70546	119670	18.33%	1.598%
21	7.609	699	701	704	rVB3	1229	1186	0.18%	0.016%
22	7.774	723	729	738	rVB	97299	163411	25.03%	2.182%
23	8.249	802	810	816	rBV	91702	153304	23.48%	2.047%
24	8.948	922	929	936	rBV2	120293	211102	32.33%	2.819%
25	9.418	1001	1009	1017	rVB	105506	181315	27.77%	2.421%
26	9.571	1032	1035	1038	rBV2	1033	1210	0.19%	0.016%
27	9.835	1078	1080	1087	rVB5	1861	2844	0.44%	0.038%
28	10.018	1108	1111	1114	rBV	771	996	0.15%	0.013%
29	10.153	1125	1134	1141	rVB2	90617	157789	24.17%	2.107%
30	10.699	1220	1227	1237	rVB2	120914	227295	34.81%	3.035%
31	10.834	1246	1250	1259	rVB3	3116	5633	0.86%	0.075%
32	10.910	1259	1263	1265	rBV	644	959	0.15%	0.013%
33	11.087	1286	1293	1301	rBV	130416	237691	36.41%	3.174%
34	11.210	1306	1314	1326	rVB	117206	224417	34.37%	2.997%
35	12.485	1528	1531	1533	rBV	1488	1312	0.20%	0.018%
36	12.661	1557	1561	1565	rVB4	1920	3159	0.48%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052024.D
 Acq On : 17 Jan 2022 14:58
 Operator : CG/JU
 Sample : N1169-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	13.266	1660	1664	1665	rBV2	670	989	0.15%	0.013%
38	13.707	1734	1739	1747	rVB2	4770	7487	1.15%	0.100%
39	14.282	1829	1837	1843	rBV	250283	361712	55.40%	4.830%
40	14.388	1853	1855	1859	rBV	941	1171	0.18%	0.016%
41	14.517	1873	1877	1882	rBV4	3827	5862	0.90%	0.078%
42	14.588	1882	1889	1896	rVV	284185	438421	67.15%	5.855%
43	14.658	1897	1901	1904	rBV	831	989	0.15%	0.013%
44	14.770	1916	1920	1925	rVB4	3820	4643	0.71%	0.062%
45	14.893	1933	1941	1950	rVB	243786	374088	57.30%	4.996%
46	14.970	1950	1954	1956	rBV	744	991	0.15%	0.013%
47	15.070	1965	1971	1986	rBV	96845	176927	27.10%	2.363%
48	15.293	2007	2009	2011	rVB2	1002	924	0.14%	0.012%
49	15.463	2036	2038	2041	rVB2	1160	983	0.15%	0.013%
50	15.516	2041	2047	2052	rBV3	4359	4980	0.76%	0.067%
51	15.675	2069	2074	2078	rBV3	2525	4938	0.76%	0.066%
52	15.716	2078	2081	2084	rVB3	2500	3155	0.48%	0.042%
53	15.886	2103	2110	2117	rVB	354821	546687	83.73%	7.301%
54	15.986	2119	2127	2137	rVB	85519	134450	20.59%	1.796%
55	16.121	2142	2150	2154	rBV3	3301	6159	0.94%	0.082%
56	16.215	2162	2166	2169	rBV3	1465	2035	0.31%	0.027%
57	16.268	2172	2175	2181	rVB3	2447	2708	0.41%	0.036%
58	16.327	2181	2185	2191	rBV4	2107	3000	0.46%	0.040%
59	16.409	2195	2199	2200	rBV2	1390	1498	0.23%	0.020%
60	16.427	2200	2202	2205	rVB2	1230	918	0.14%	0.012%
61	16.462	2206	2208	2211	rBV	1143	1279	0.20%	0.017%
62	16.556	2220	2224	2228	rBV4	2875	4891	0.75%	0.065%
63	16.662	2239	2242	2243	rBV2	1348	1068	0.16%	0.014%
64	16.761	2252	2259	2265	rBV5	2534	5625	0.86%	0.075%
65	16.867	2273	2277	2283	rVB4	1592	2865	0.44%	0.038%
66	16.932	2283	2288	2291	rBV4	1490	2726	0.42%	0.036%
67	16.979	2294	2296	2300	rBV3	1962	2966	0.45%	0.040%
68	17.020	2300	2303	2306	rVV3	1383	1954	0.30%	0.026%
69	17.096	2312	2316	2319	rBV4	2335	3169	0.49%	0.042%
70	17.331	2351	2356	2357	rBV4	1729	1697	0.26%	0.023%
71	17.372	2360	2363	2366	rBV3	4467	4672	0.72%	0.062%
72	17.413	2368	2370	2372	rBV2	1285	1466	0.22%	0.020%
73	17.531	2387	2390	2395	rBV4	5312	6797	1.04%	0.091%
74	17.643	2399	2409	2415	rBV	318247	481963	73.82%	6.436%
75	17.701	2417	2419	2420	rVV	3187	2510	0.38%	0.034%
76	17.742	2420	2426	2433	rVB2	403492	602588	92.29%	8.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052024.D
 Acq On : 17 Jan 2022 14:58
 Operator : CG/JU
 Sample : N1169-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	17.866	2445	2447	2449	rBV3	1583	1142	0.17%	0.015%
78	17.907	2449	2454	2457	rBV4	3567	5514	0.84%	0.074%
79	18.030	2473	2475	2478	rVB4	1453	1522	0.23%	0.020%
80	18.112	2487	2489	2490	rBV2	1484	1185	0.18%	0.016%
81	18.171	2497	2499	2502	rVB3	2064	1871	0.29%	0.025%
82	18.195	2502	2503	2506	rBV2	1798	1895	0.29%	0.025%
83	18.289	2516	2519	2526	rVB6	4363	6784	1.04%	0.091%
84	18.347	2526	2529	2531	rBV3	2380	2430	0.37%	0.032%
85	18.365	2531	2532	2536	rBV4	1868	2058	0.32%	0.027%
86	18.394	2536	2537	2539	rBV2	1280	1300	0.20%	0.017%
87	18.471	2548	2550	2553	rBV4	1656	1115	0.17%	0.015%
88	18.582	2566	2569	2574	rVB	6769	8541	1.31%	0.114%
89	18.800	2604	2606	2607	rBV2	3059	2518	0.39%	0.034%
90	18.929	2624	2628	2632	rVB6	3921	5873	0.90%	0.078%
91	19.023	2642	2644	2645	rBV2	2108	1586	0.24%	0.021%
92	19.587	2736	2740	2743	rBV6	6219	9651	1.48%	0.129%
93	20.022	2808	2814	2822	rVB	462437	652902	100.00%	8.719%
94	21.567	3073	3077	3084	rBV9	18888	44122	6.76%	0.589%
95	21.966	3138	3145	3153	rVB	267389	465748	71.34%	6.220%
96	25.221	3690	3699	3713	rVB2	196719	588286	90.10%	7.856%
97	25.467	3732	3741	3755	rVB2	156688	500947	76.73%	6.690%




Sum of corrected areas: 7488152

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052024.D
Acq On : 17 Jan 2022 14:58
Operator : CG/JU
Sample : N1169-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

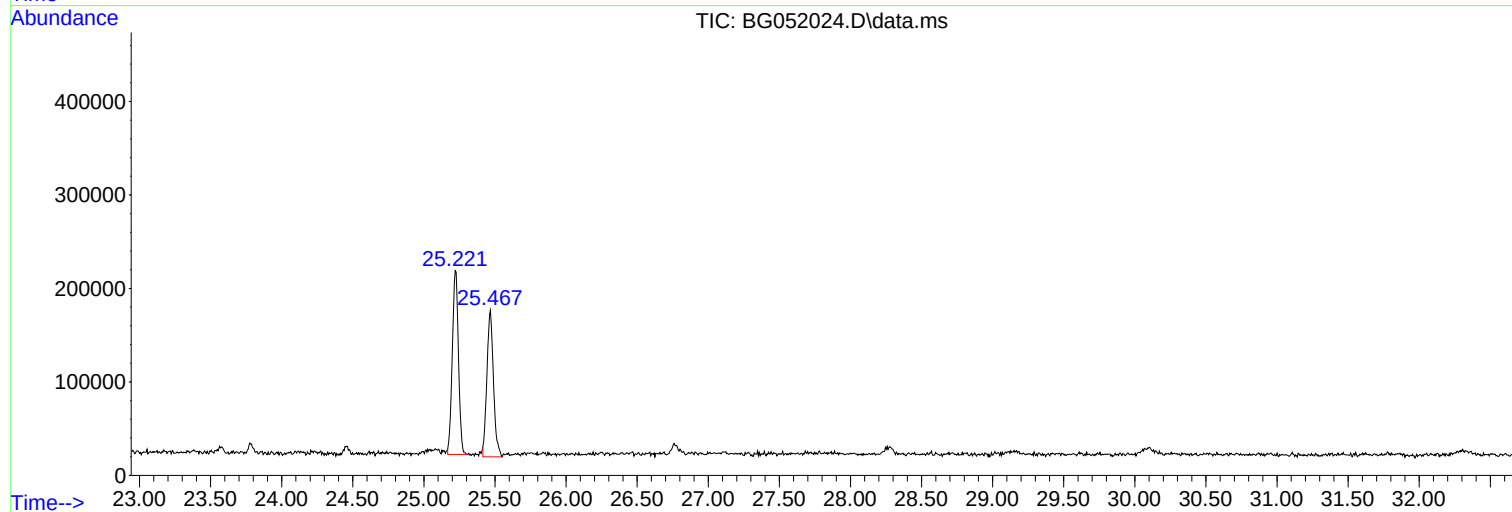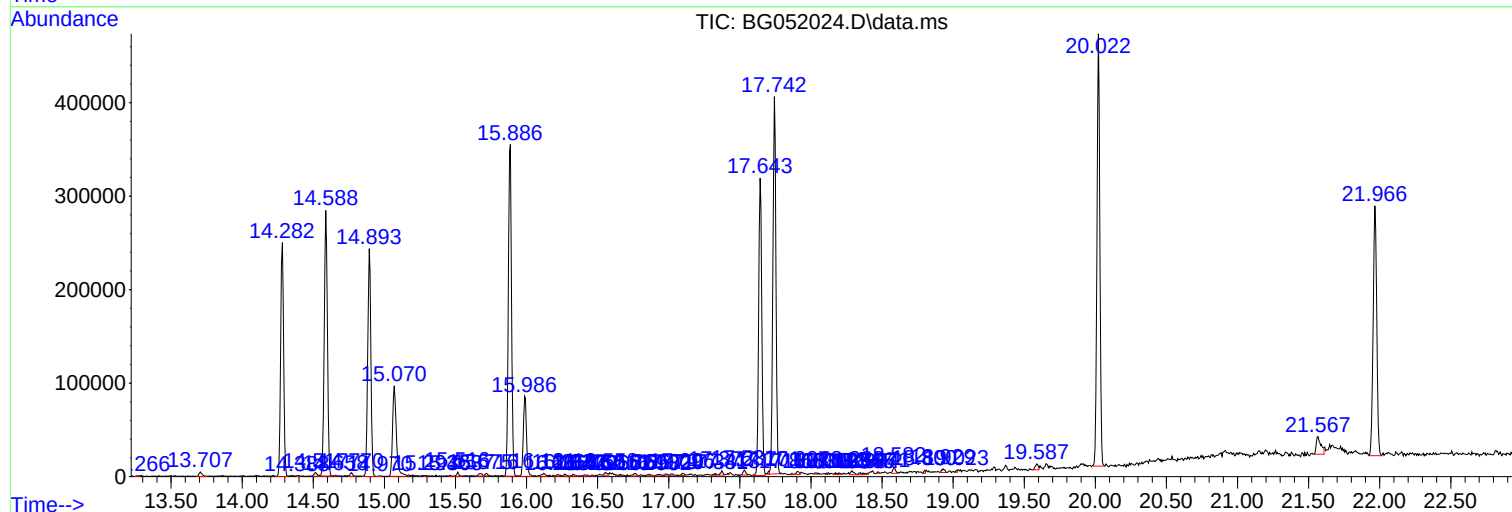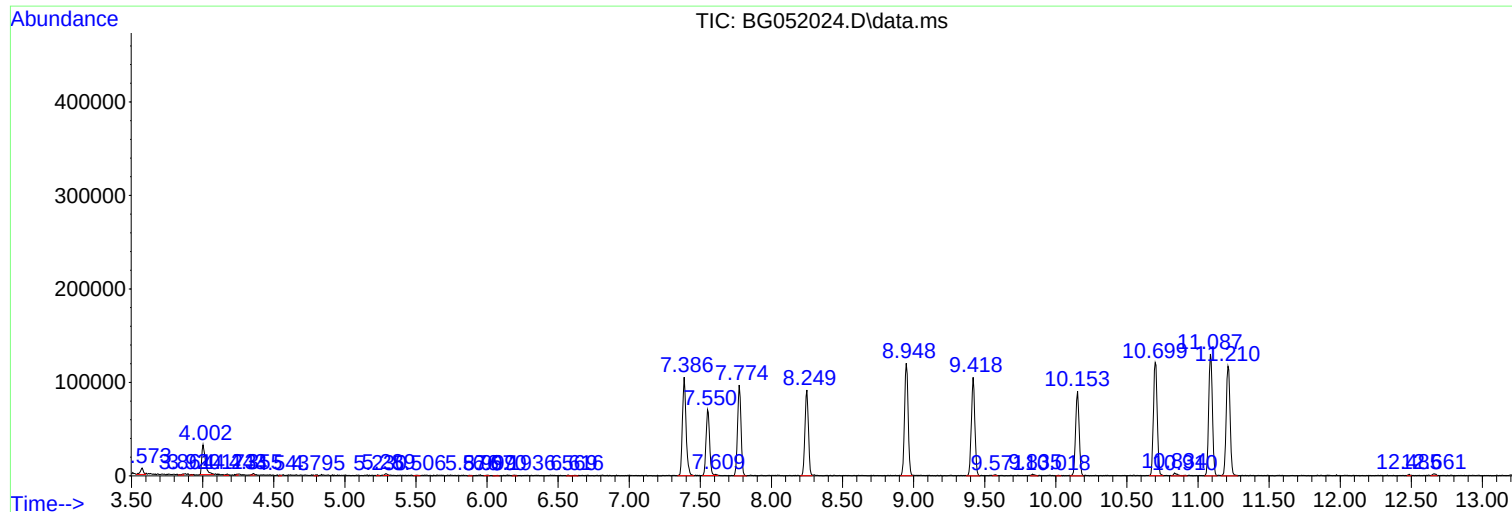

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052024.D
Acq On : 17 Jan 2022 14:58
Operator : CG/JU
Sample : N1169-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052024.D
Acq On : 17 Jan 2022 14:58
Operator : CG/JU
Sample : N1169-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------