

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052034.D
 Acq On : 17 Jan 2022 21:54
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	10	14	19	rVB2	9751	14695	0.79%	0.080%
2	3.996	82	86	101	rBV	233351	379897	20.34%	2.062%
3	4.355	142	147	153	rBV	16059	24628	1.32%	0.134%
4	7.386	652	663	672	rBV	281143	492666	26.37%	2.674%
5	7.550	684	691	698	rBV	202191	339938	18.20%	1.845%
6	7.774	721	729	737	rBV	254514	435141	23.29%	2.362%
7	8.244	803	809	818	rBV	167507	295614	15.82%	1.604%
8	8.948	921	929	939	rBV	325106	571212	30.58%	3.100%
9	9.418	1000	1009	1017	rBV	257274	466601	24.98%	2.533%
10	10.153	1125	1134	1141	rBV	222184	408566	21.87%	2.218%
11	10.699	1218	1227	1241	rBV	320024	573772	30.71%	3.114%
12	11.087	1284	1293	1303	rBV	258798	466703	24.98%	2.533%
13	11.210	1306	1314	1330	rBV	325904	601731	32.21%	3.266%
14	12.661	1556	1561	1566	rBV3	4926	8889	0.48%	0.048%
15	14.282	1829	1837	1844	rBV	619943	923706	49.45%	5.014%
16	14.588	1880	1889	1896	rBV	690579	1086410	58.16%	5.897%
17	14.893	1934	1941	1950	rVB	417099	687501	36.80%	3.732%
18	15.070	1963	1971	1981	rBV	306842	528399	28.29%	2.868%
19	15.880	2100	2109	2120	rBV	897006	1372918	73.49%	7.452%
20	15.986	2120	2127	2137	rVV	315590	471231	25.23%	2.558%
21	16.051	2137	2138	2142	rVV4	2542	2815	0.15%	0.015%
22	16.121	2148	2150	2154	rVB	3403	3236	0.17%	0.018%
23	17.425	2369	2372	2378	rVB3	2463	3889	0.21%	0.021%
24	17.643	2402	2409	2416	rBV	581043	893659	47.84%	4.850%
25	17.742	2419	2426	2435	rVB2	1031936	1593951	85.33%	8.651%
26	19.182	2670	2671	2676	rBV2	1592	1971	0.11%	0.011%
27	19.252	2680	2683	2687	rBV5	1759	2204	0.12%	0.012%
28	19.522	2724	2729	2732	rBV4	999	1968	0.11%	0.011%
29	19.587	2734	2740	2745	rBV3	15131	24821	1.33%	0.135%
30	19.658	2748	2752	2756	rBV2	14196	19376	1.04%	0.105%
31	19.787	2772	2774	2777	rBV3	2048	1928	0.10%	0.010%
32	20.022	2807	2814	2824	rVB	1351648	1868063	100.00%	10.139%
33	20.950	2971	2972	2973	rBV	4458	2744	0.15%	0.015%
34	21.114	2998	3000	3002	rBV3	3026	3282	0.18%	0.018%
35	21.320	3033	3035	3036	rBV2	3013	2325	0.12%	0.013%
36	21.661	3086	3093	3094	rBV7	12350	22994	1.23%	0.125%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052034.D
 Acq On : 17 Jan 2022 21:54
 Operator : CG/JU
 Sample : PB142047BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	21.825	3117	3121	3122	rBV4	4325	5895	0.32%	0.032%
38	21.966	3138	3145	3154	rVB	507456	886517	47.46%	4.812%
39	22.283	3197	3199	3201	rVB3	4647	3711	0.20%	0.020%
40	22.307	3201	3203	3206	rBV3	3557	3969	0.21%	0.022%
41	22.542	3237	3243	3245	rBV7	3787	7569	0.41%	0.041%
42	23.082	3333	3335	3338	rBV4	4631	4496	0.24%	0.024%
43	23.494	3403	3405	3408	rBV3	4779	5147	0.28%	0.028%
44	23.523	3408	3410	3411	rBV2	5074	3355	0.18%	0.018%
45	23.570	3414	3418	3423	rVB6	15053	27085	1.45%	0.147%
46	23.646	3429	3431	3434	rBV3	6308	9015	0.48%	0.049%
47	24.457	3563	3569	3580	rVB5	19979	47760	2.56%	0.259%
48	25.215	3687	3698	3712	rVB2	553592	1686659	90.29%	9.155%
49	25.461	3729	3740	3755	rVB3	284431	932480	49.92%	5.061%
50	25.649	3770	3772	3773	rBV2	3595	2991	0.16%	0.016%
51	26.695	3948	3950	3952	rBV3	4358	3226	0.17%	0.018%
52	26.748	3952	3959	3970	rVV6	24571	80169	4.29%	0.435%
53	27.747	4127	4129	4130	rBV2	3924	2847	0.15%	0.015%
54	28.258	4208	4216	4227	rVB8	21615	74724	4.00%	0.406%
55	28.434	4244	4246	4249	rBV4	3867	3546	0.19%	0.019%
56	31.295	4731	4733	4736	rBV4	3431	2948	0.16%	0.016%
57	31.682	4797	4799	4800	rVB2	4457	2197	0.12%	0.012%
58	31.700	4800	4802	4803	rBV2	3872	2678	0.14%	0.015%
59	31.735	4807	4808	4809	rBV	4070	2385	0.13%	0.013%
60	32.235	4889	4893	4895	rBV5	6081	8621	0.46%	0.047%
61	32.264	4895	4898	4900	rBV3	6827	9910	0.53%	0.054%
62	32.593	4952	4954	4956	rBV3	5039	4821	0.26%	0.026%




Sum of corrected areas: 18424165

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052034.D
Acq On : 17 Jan 2022 21:54
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

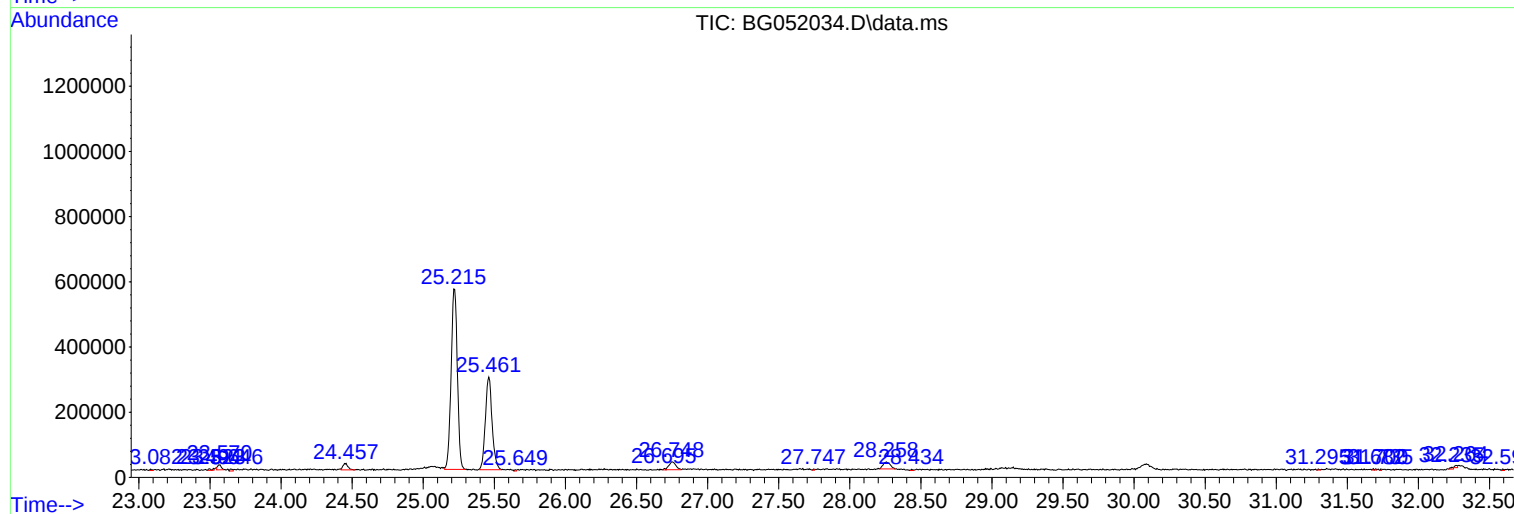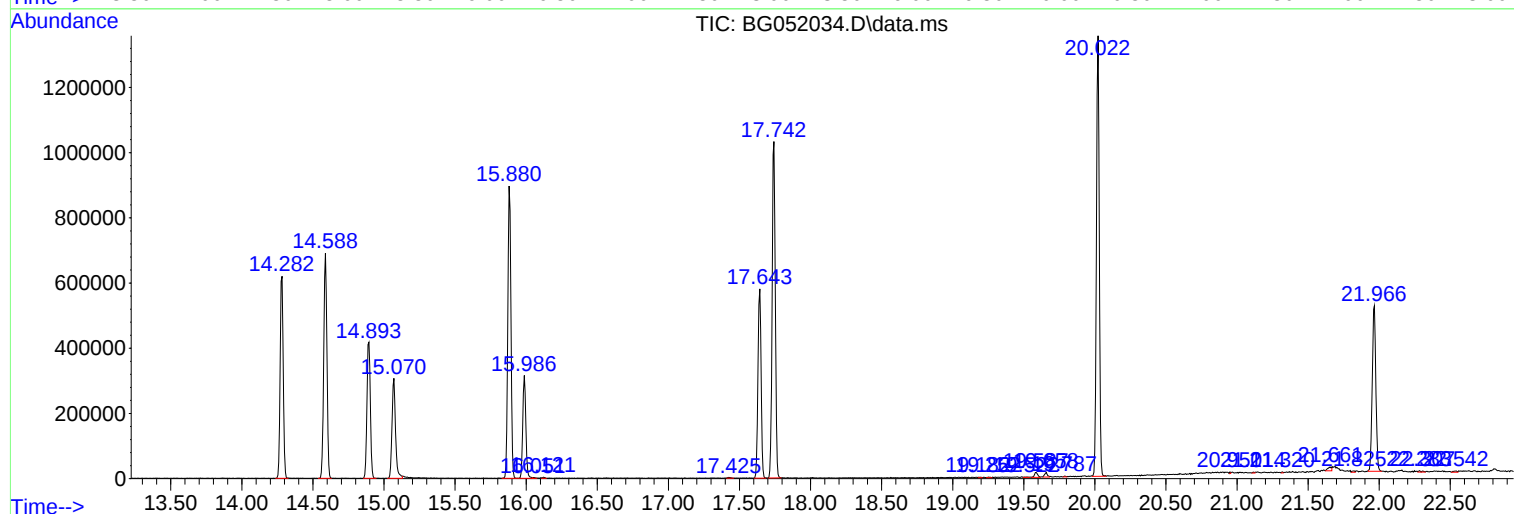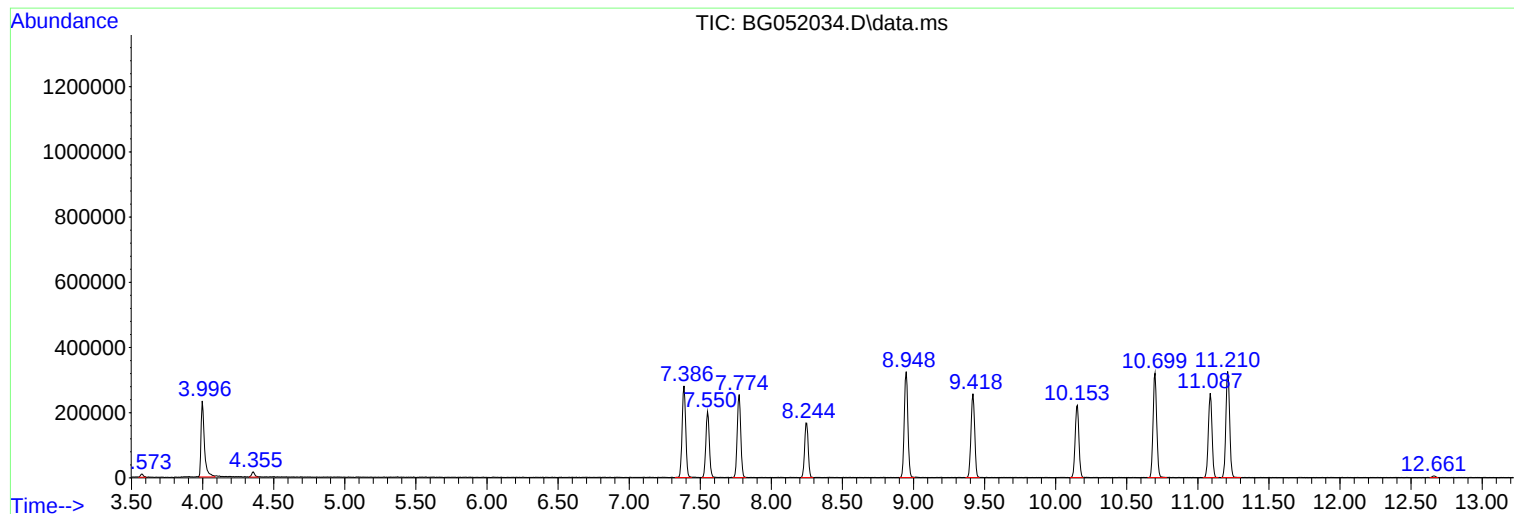

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052034.D
Acq On : 17 Jan 2022 21:54
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052034.D
Acq On : 17 Jan 2022 21:54
Operator : CG/JU
Sample : PB142047BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
