

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052051.D
 Acq On : 18 Jan 2022 14:18
 Operator : CG/JU
 Sample : N1169-01DL 30X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.383	659	663	670	rBV2	2935	4656	0.21%	0.108%
2	7.553	686	692	696	rBB	2607	3603	0.17%	0.084%
3	7.770	724	729	735	rVB	2458	3653	0.17%	0.085%
4	8.246	803	810	817	rBV2	77934	136414	6.29%	3.166%
5	8.951	925	930	934	rVB2	2337	4217	0.19%	0.098%
6	9.415	1005	1009	1013	rVB2	2475	3986	0.18%	0.092%
7	10.149	1129	1134	1139	rBB2	2573	3879	0.18%	0.090%
8	10.702	1223	1228	1233	rVB3	2703	4516	0.21%	0.105%
9	11.083	1285	1293	1300	rVB	117085	210212	9.69%	4.878%
10	11.213	1311	1315	1321	rVB3	2555	4671	0.22%	0.108%
11	12.482	1526	1531	1539	rVB3	2540	3560	0.16%	0.083%
12	13.421	1688	1691	1695	rVV2	2525	3439	0.16%	0.080%
13	13.686	1732	1736	1744	rBV7	5886	13451	0.62%	0.312%
14	13.797	1750	1755	1756	rBV4	2861	3813	0.18%	0.088%
15	14.038	1791	1796	1797	rBV4	1458	2620	0.12%	0.061%
16	14.097	1803	1806	1808	rBV3	2617	3370	0.16%	0.078%
17	14.209	1821	1825	1828	rBV6	2647	4059	0.19%	0.094%
18	14.273	1833	1836	1840	rVV2	7997	10762	0.50%	0.250%
19	14.320	1840	1844	1847	rVV6	4112	6484	0.30%	0.150%
20	14.350	1847	1849	1853	rVB3	4707	4865	0.22%	0.113%
21	14.444	1862	1865	1867	rBV3	1966	2203	0.10%	0.051%
22	14.543	1879	1882	1885	rBV5	2587	3635	0.17%	0.084%
23	14.585	1885	1889	1893	rVB2	11124	14251	0.66%	0.331%
24	14.643	1896	1899	1903	rBV6	5214	8200	0.38%	0.190%
25	14.720	1910	1912	1916	rBV5	3903	4318	0.20%	0.100%
26	14.767	1918	1920	1923	rVB3	3565	4222	0.19%	0.098%
27	14.796	1923	1925	1929	rVB4	2985	4034	0.19%	0.094%
28	14.890	1929	1941	1949	rBV	215508	349344	16.11%	8.107%
29	14.966	1951	1954	1955	rBV3	4443	4067	0.19%	0.094%
30	15.002	1959	1960	1963	rBV3	3032	2402	0.11%	0.056%
31	15.049	1966	1968	1972	rVB5	3643	2912	0.13%	0.068%
32	15.231	1997	1999	2001	rBV3	3086	2371	0.11%	0.055%
33	15.272	2005	2006	2009	rVB3	5017	3892	0.18%	0.090%
34	15.331	2014	2016	2021	rVB6	4031	6164	0.28%	0.143%
35	15.483	2040	2042	2044	rBV3	4170	3446	0.16%	0.080%
36	15.548	2050	2053	2056	rBV5	4040	6553	0.30%	0.152%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052051.D
 Acq On : 18 Jan 2022 14:18
 Operator : CG/JU
 Sample : N1169-01DL 30X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.613	2059	2064	2070	rBV8	6369	11618	0.54%	0.270%
38	15.671	2072	2074	2075	rBV2	7884	5739	0.26%	0.133%
39	15.771	2089	2091	2096	rVB6	5891	5804	0.27%	0.135%
40	15.877	2105	2109	2115	rBV3	12773	23246	1.07%	0.539%
41	15.994	2127	2129	2130	rBV2	6423	5082	0.23%	0.118%
42	16.975	2291	2296	2301	rBV9	18245	33956	1.57%	0.788%
43	17.639	2404	2409	2417	rVB	251275	381965	17.61%	8.864%
44	21.822	3115	3121	3128	rVB	1544171	2168725	100.00%	50.327%
45	21.963	3138	3145	3151	rVB	210045	377304	17.40%	8.756%
46	25.211	3696	3698	3704	rVB6	13521	19131	0.88%	0.444%
47	25.452	3730	3739	3749	rVB2	129943	398021	18.35%	9.236%
48	25.828	3801	3803	3804	rBV2	5293	3465	0.16%	0.080%
49	30.304	4563	4565	4567	rBV3	4851	4469	0.21%	0.104%
50	30.481	4593	4595	4596	rBV2	4959	3692	0.17%	0.086%
51	30.992	4680	4682	4685	rBV4	4467	4065	0.19%	0.094%
52	32.613	4956	4958	4961	rBV3	4171	4770	0.22%	0.111%




Sum of corrected areas: 4309296

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052051.D
Acq On : 18 Jan 2022 14:18
Operator : CG/JU
Sample : N1169-01DL 30X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

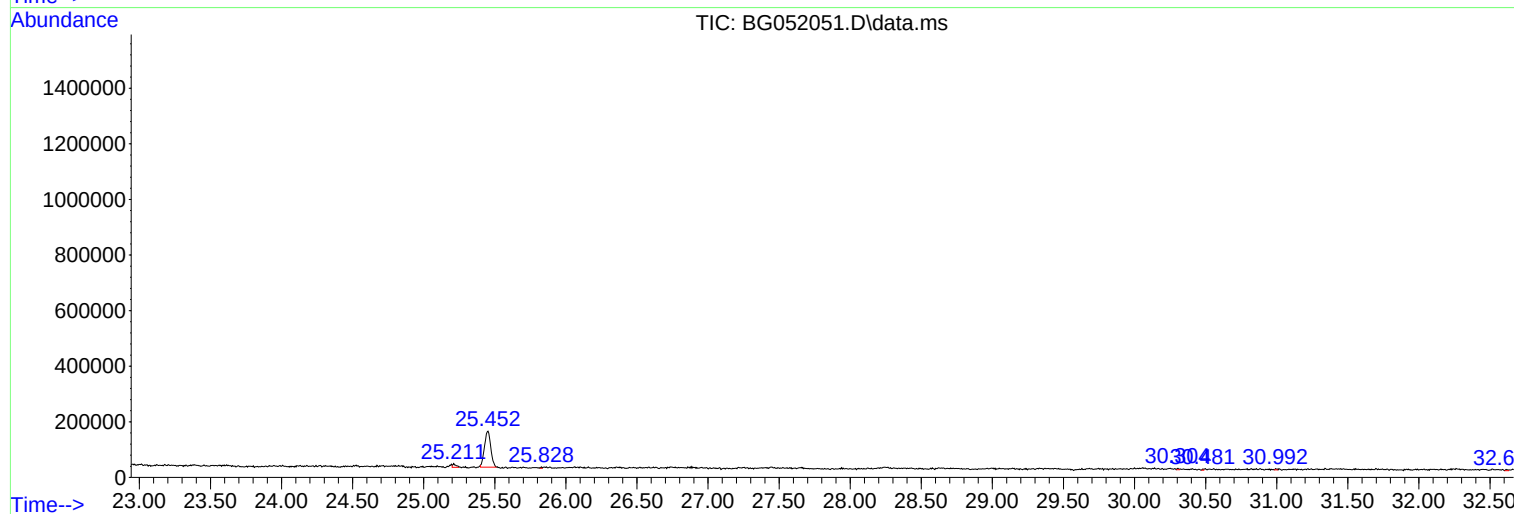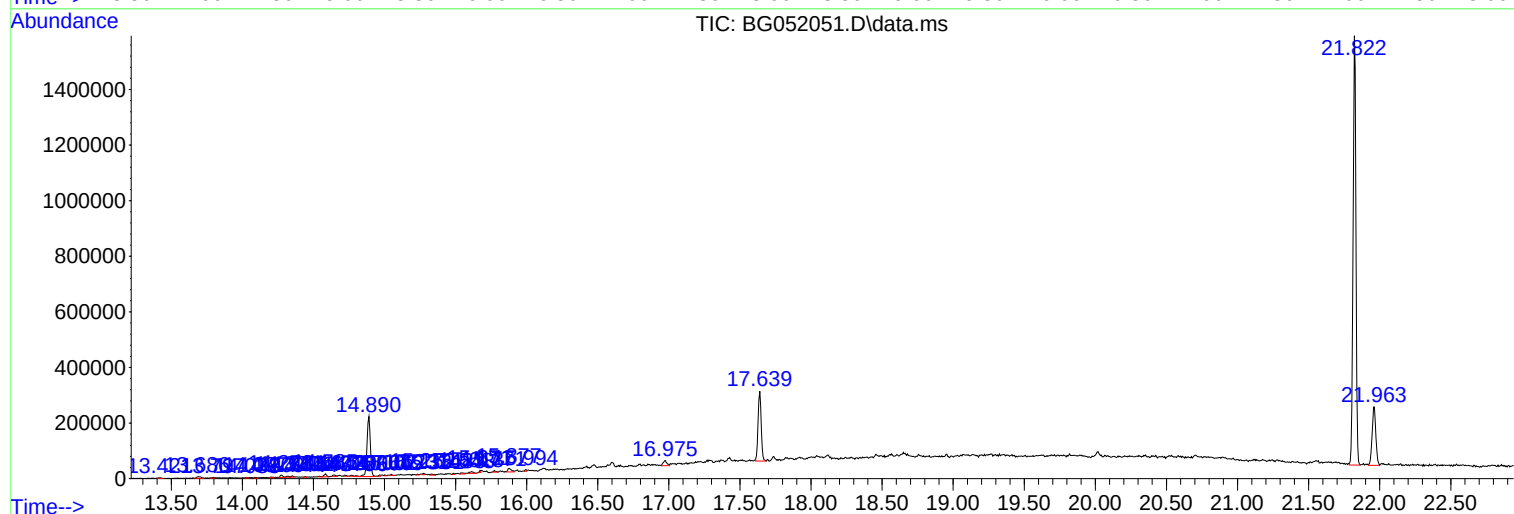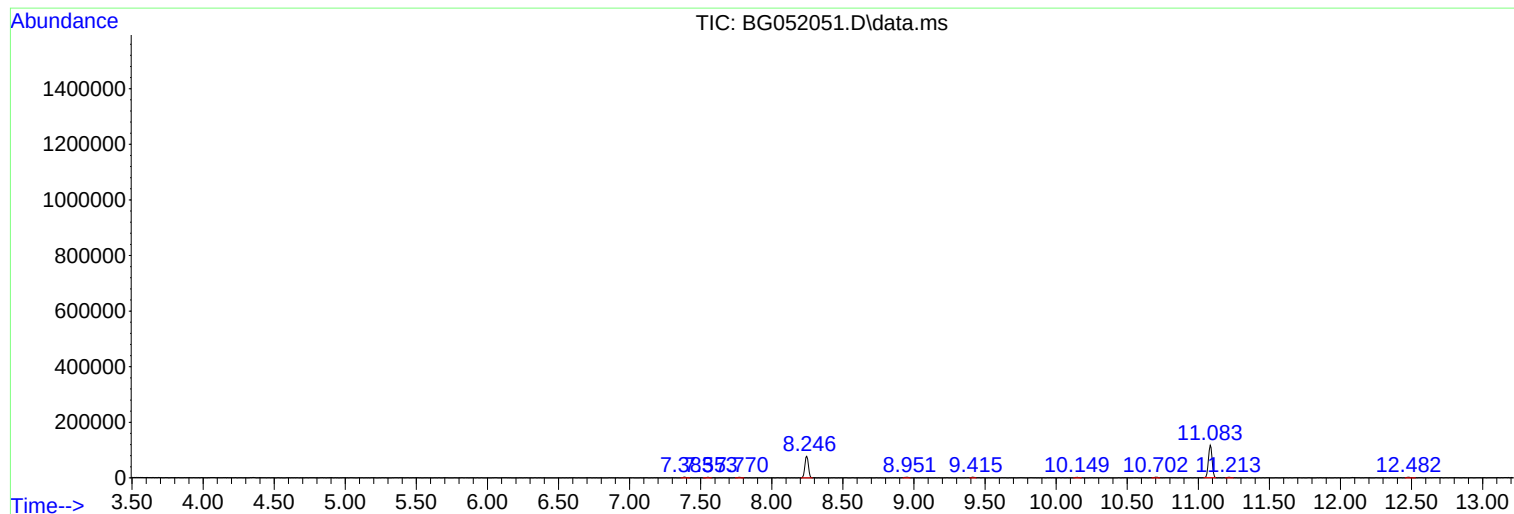

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052051.D
Acq On : 18 Jan 2022 14:18
Operator : CG/JU
Sample : N1169-01DL 30X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052051.D
Acq On : 18 Jan 2022 14:18
Operator : CG/JU
Sample : N1169-01DL 30X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
