

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052057.D
 Acq On : 18 Jan 2022 18:05
 Operator : CG/JU
 Sample : PB142117BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	7	14	18	rBV3	6608	10096	1.29%	0.125%
2	3.995	80	86	105	rBV	83143	142799	18.29%	1.765%
3	4.348	142	146	147	rBV2	1696	2369	0.30%	0.029%
4	7.385	652	663	672	rBV	109970	195602	25.05%	2.417%
5	7.549	684	691	699	rBV	73771	129257	16.55%	1.597%
6	7.767	722	728	735	rBV2	103865	176155	22.56%	2.177%
7	8.243	801	809	816	rBV	83964	140362	17.97%	1.735%
8	8.942	921	928	937	rBV	139580	238116	30.49%	2.943%
9	9.412	1001	1008	1018	rBV	103470	189505	24.27%	2.342%
10	10.146	1126	1133	1141	rVB	99158	172420	22.08%	2.131%
11	10.692	1218	1226	1235	rBV	139907	250240	32.04%	3.093%
12	11.080	1285	1292	1300	rVB	122547	221887	28.41%	2.742%
13	11.209	1306	1314	1324	rBV	133114	248828	31.86%	3.075%
14	12.648	1555	1559	1565	rBV3	2061	2897	0.37%	0.036%
15	14.276	1829	1836	1843	rVB	278690	406311	52.03%	5.022%
16	14.581	1881	1888	1895	rBV	307682	480933	61.59%	5.944%
17	14.887	1934	1940	1947	rBV	228317	344763	44.15%	4.261%
18	15.063	1960	1970	1979	rBV	111239	190088	24.34%	2.349%
19	15.874	2101	2108	2115	rBV	400641	601483	77.02%	7.434%
20	15.979	2120	2126	2135	rBV	104524	161360	20.66%	1.994%
21	16.114	2146	2149	2153	rBV2	2018	2556	0.33%	0.032%
22	17.636	2400	2408	2417	rVV	294978	440212	56.37%	5.440%
23	17.736	2418	2425	2432	rVV2	439753	685664	87.80%	8.474%
24	18.840	2610	2613	2619	rBV2	851	1603	0.21%	0.020%
25	19.580	2732	2739	2742	rVV5	6132	9786	1.25%	0.121%
26	19.657	2747	2752	2755	rVV2	4846	7598	0.97%	0.094%
27	20.015	2806	2813	2819	rBV	563051	780925	100.00%	9.651%
28	20.297	2859	2861	2862	rBV2	2090	1665	0.21%	0.021%
29	20.467	2887	2890	2892	rBV2	1811	2314	0.30%	0.029%
30	20.544	2900	2903	2906	rBV5	2077	2208	0.28%	0.027%
31	20.626	2914	2917	2918	rBV3	1838	2006	0.26%	0.025%
32	20.755	2937	2939	2940	rVB2	2626	1601	0.21%	0.020%
33	20.773	2940	2942	2943	rBV2	2542	1916	0.25%	0.024%
34	20.949	2970	2972	2975	rVB4	1669	1721	0.22%	0.021%
35	21.113	2999	3000	3003	rVB3	3149	2570	0.33%	0.032%
36	21.137	3003	3004	3005	rBV	3720	1829	0.23%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052057.D
 Acq On : 18 Jan 2022 18:05
 Operator : CG/JU
 Sample : PB142117BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	21.260	3024	3025	3027	rBV2	3169	2259	0.29%	0.028%
38	21.472	3058	3061	3062	rBV3	2181	2089	0.27%	0.026%
39	21.854	3124	3126	3129	rBV3	2613	2881	0.37%	0.036%
40	21.954	3136	3143	3153	rVB2	247449	442437	56.66%	5.468%
41	22.230	3187	3190	3192	rVB4	2953	2869	0.37%	0.035%
42	22.647	3260	3261	3263	rBV2	2062	1629	0.21%	0.020%
43	22.799	3283	3287	3292	rVV6	4377	8597	1.10%	0.106%
44	22.970	3313	3316	3318	rBV4	2928	3289	0.42%	0.041%
45	23.046	3327	3329	3330	rBV2	1881	1797	0.23%	0.022%
46	23.475	3400	3402	3403	rBV2	2525	1790	0.23%	0.022%
47	23.557	3410	3416	3421	rVB6	7081	14051	1.80%	0.174%
48	23.710	3440	3442	3448	rBV5	2253	3363	0.43%	0.042%
49	23.763	3450	3451	3454	rBV3	2673	1798	0.23%	0.022%
50	24.074	3502	3504	3506	rBV3	2388	1925	0.25%	0.024%
51	24.092	3506	3507	3510	rVV2	3322	2164	0.28%	0.027%
52	24.115	3510	3511	3515	rVB4	3585	3343	0.43%	0.041%
53	24.433	3561	3565	3571	rVB7	9282	18774	2.40%	0.232%
54	24.485	3573	3574	3577	rBV3	2604	2956	0.38%	0.037%
55	24.650	3598	3602	3603	rBV4	2102	2087	0.27%	0.026%
56	24.767	3621	3622	3625	rBV3	3199	1983	0.25%	0.025%
57	24.891	3642	3643	3645	rBV2	3304	2011	0.26%	0.025%
58	25.202	3685	3696	3709	rVB2	239849	716760	91.78%	8.858%
59	25.443	3724	3737	3751	rVB2	140126	472778	60.54%	5.843%
60	25.754	3788	3790	3792	rBV3	2187	1845	0.24%	0.023%
61	25.854	3805	3807	3809	rBV3	1957	1697	0.22%	0.021%
62	25.977	3826	3828	3830	rBV3	2980	3278	0.42%	0.041%
63	26.030	3835	3837	3838	rVB2	2785	1622	0.21%	0.020%
64	26.289	3879	3881	3884	rBV3	1932	1938	0.25%	0.024%
65	26.348	3890	3891	3893	rBV2	2421	2057	0.26%	0.025%
66	26.424	3902	3904	3906	rBV3	2406	1728	0.22%	0.021%
67	26.465	3909	3911	3914	rBV4	2118	2218	0.28%	0.027%
68	26.594	3931	3933	3936	rBV3	2028	2270	0.29%	0.028%
69	26.647	3940	3942	3945	rBV4	2573	2909	0.37%	0.036%
70	26.724	3949	3955	3963	rVV7	9633	29086	3.72%	0.359%
71	27.029	4005	4007	4009	rVB3	2391	1890	0.24%	0.023%
72	27.070	4012	4014	4016	rVB3	2895	2302	0.29%	0.028%
73	27.094	4016	4018	4019	rBV2	3169	1805	0.23%	0.022%
74	27.346	4059	4061	4065	rBV5	2490	3513	0.45%	0.043%
75	27.499	4085	4087	4090	rBV4	2074	1667	0.21%	0.021%
76	27.581	4099	4101	4103	rBV3	3035	1763	0.23%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
 Data File : BG052057.D
 Acq On : 18 Jan 2022 18:05
 Operator : CG/JU
 Sample : PB142117BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	28.045	4178	4180	4182	rBV3	1990	1955	0.25%	0.024%
78	28.069	4182	4184	4185	rBV2	2395	1726	0.22%	0.021%
79	28.104	4188	4190	4192	rBV3	1928	1753	0.22%	0.022%
80	28.210	4204	4208	4209	rBV4	8148	8790	1.13%	0.109%
81	28.456	4247	4250	4251	rBV3	2778	3100	0.40%	0.038%
82	28.979	4337	4339	4341	rBV3	2208	2255	0.29%	0.028%
83	29.150	4365	4368	4369	rBV3	2252	2636	0.34%	0.033%
84	29.443	4417	4418	4420	rBV2	3188	2536	0.32%	0.031%
85	29.849	4485	4487	4490	rVV4	2032	2141	0.27%	0.026%
86	29.907	4494	4497	4500	rBV5	2092	2855	0.37%	0.035%
87	30.137	4534	4536	4537	rBV2	2054	1740	0.22%	0.022%
88	30.184	4542	4544	4547	rBV4	2640	2962	0.38%	0.037%
89	30.389	4577	4579	4581	rBV3	2568	1799	0.23%	0.022%
90	30.442	4585	4588	4591	rBV5	2748	3826	0.49%	0.047%
91	30.495	4595	4597	4598	rBV2	2100	1619	0.21%	0.020%
92	30.859	4657	4659	4662	rBV4	2336	1839	0.24%	0.023%
93	31.135	4704	4706	4711	rVB5	2397	2158	0.28%	0.027%
94	31.329	4737	4739	4742	rBV4	2094	2196	0.28%	0.027%
95	31.423	4754	4755	4757	rBV2	2523	1594	0.20%	0.020%
96	31.905	4835	4837	4840	rBV4	3269	3245	0.42%	0.040%
97	31.999	4851	4853	4856	rBV3	1918	1572	0.20%	0.019%
98	32.087	4866	4868	4869	rBV2	3243	2170	0.28%	0.027%
99	32.210	4886	4889	4890	rBV3	3514	3506	0.45%	0.043%
100	32.310	4904	4906	4908	rBV3	2874	2585	0.33%	0.032%




Sum of corrected areas: 8091421

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052057.D
Acq On : 18 Jan 2022 18:05
Operator : CG/JU
Sample : PB142117BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

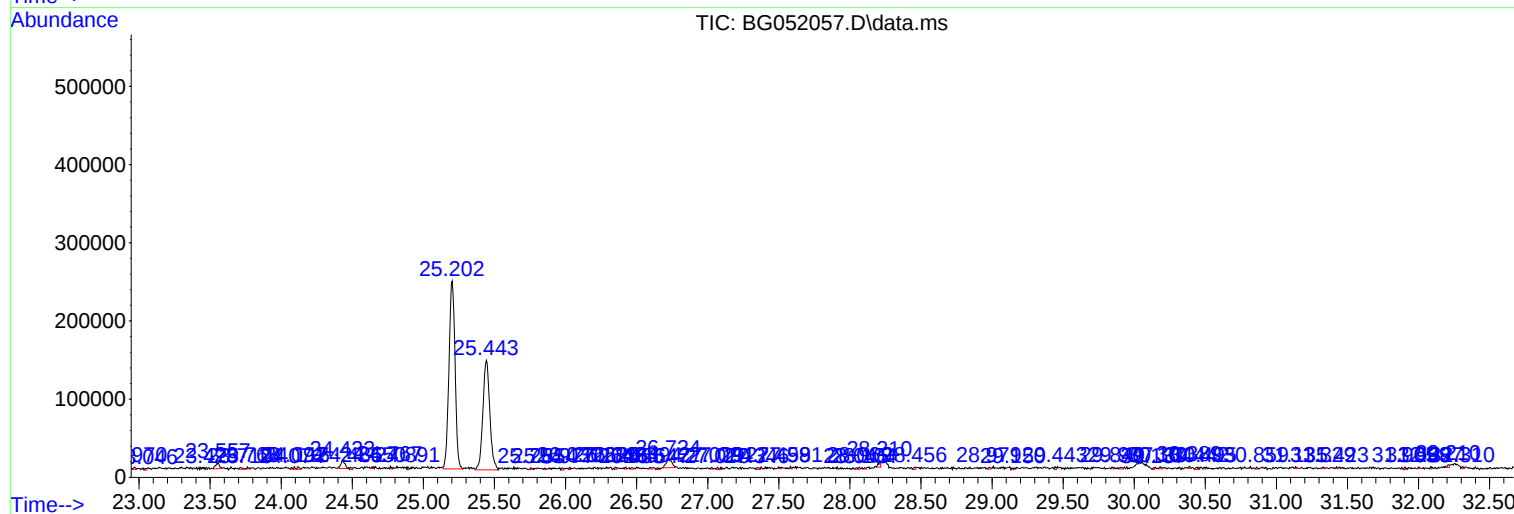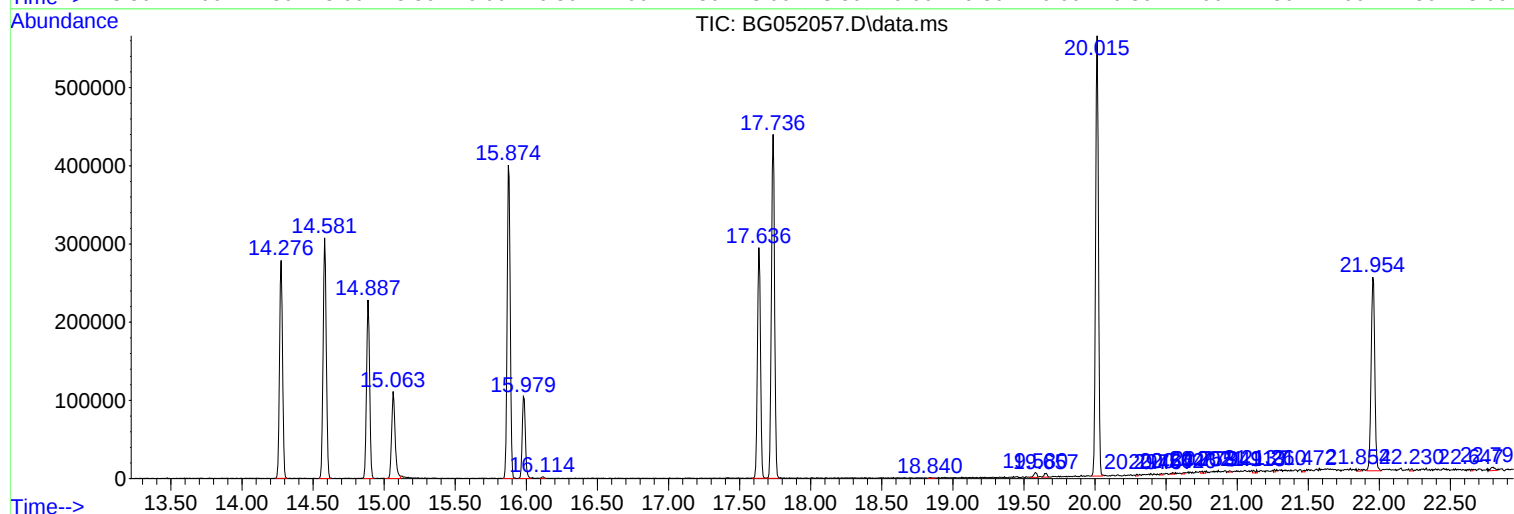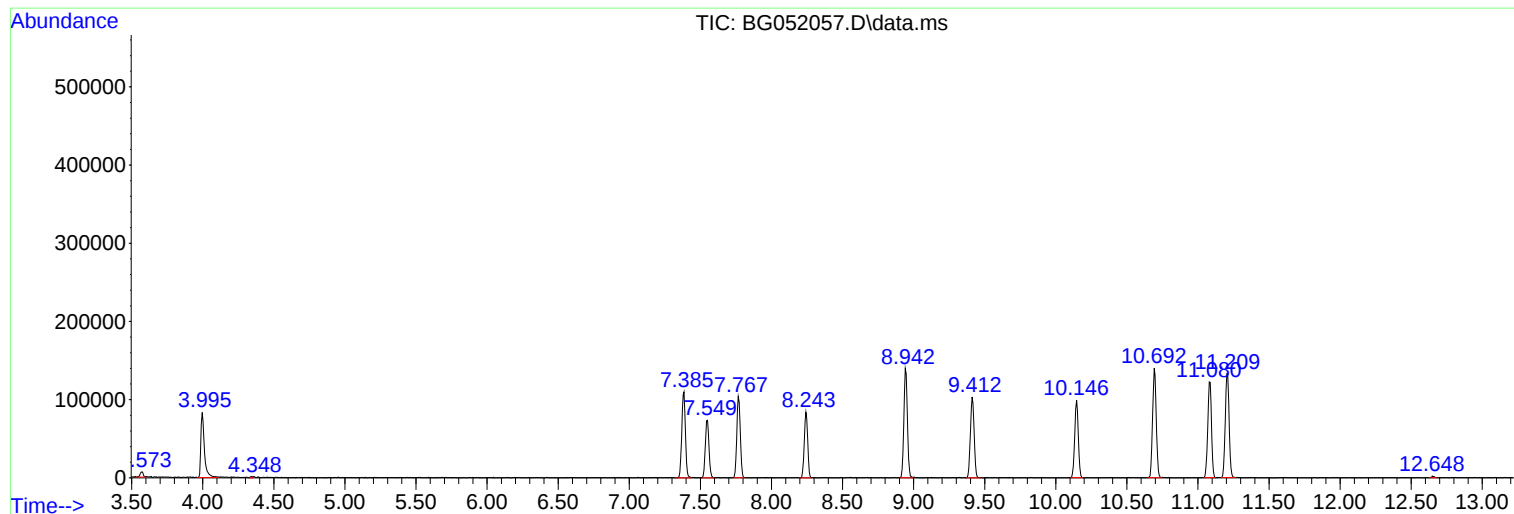

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052057.D
Acq On : 18 Jan 2022 18:05
Operator : CG/JU
Sample : PB142117BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011722\
Data File : BG052057.D
Acq On : 18 Jan 2022 18:05
Operator : CG/JU
Sample : PB142117BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc