
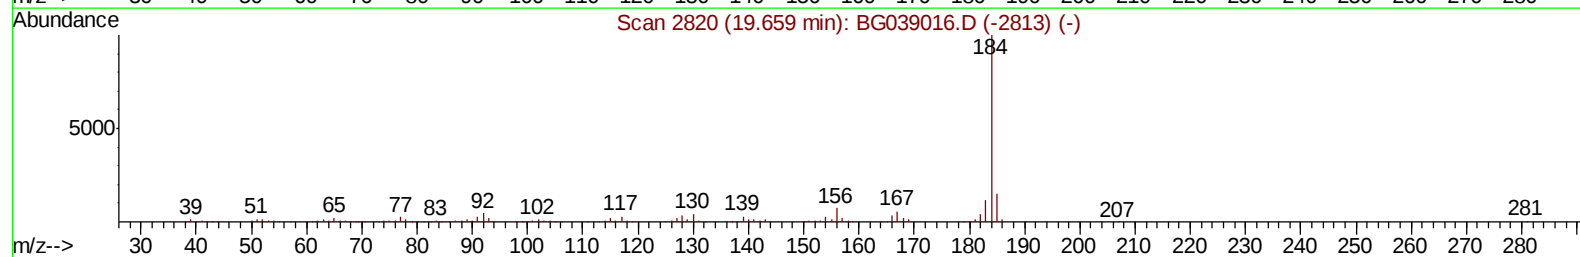
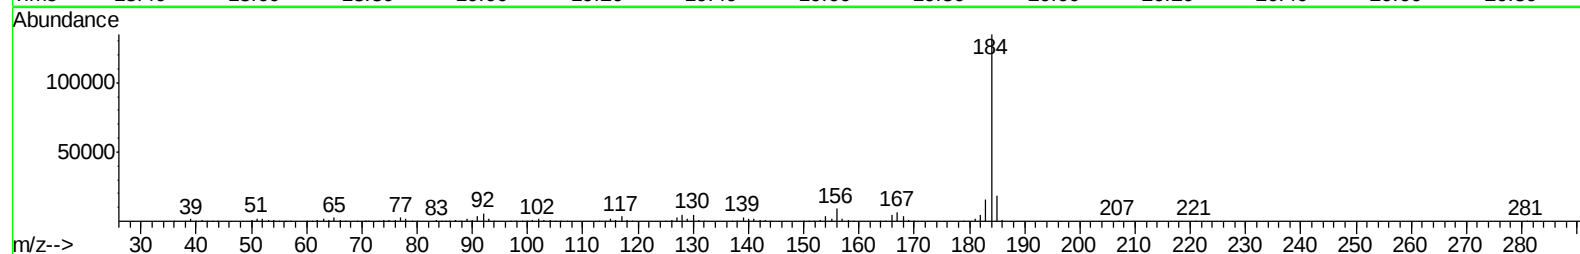


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011819\
 Data File : BG039212.D
 Acq On : 18 Jan 2019 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 22:42:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

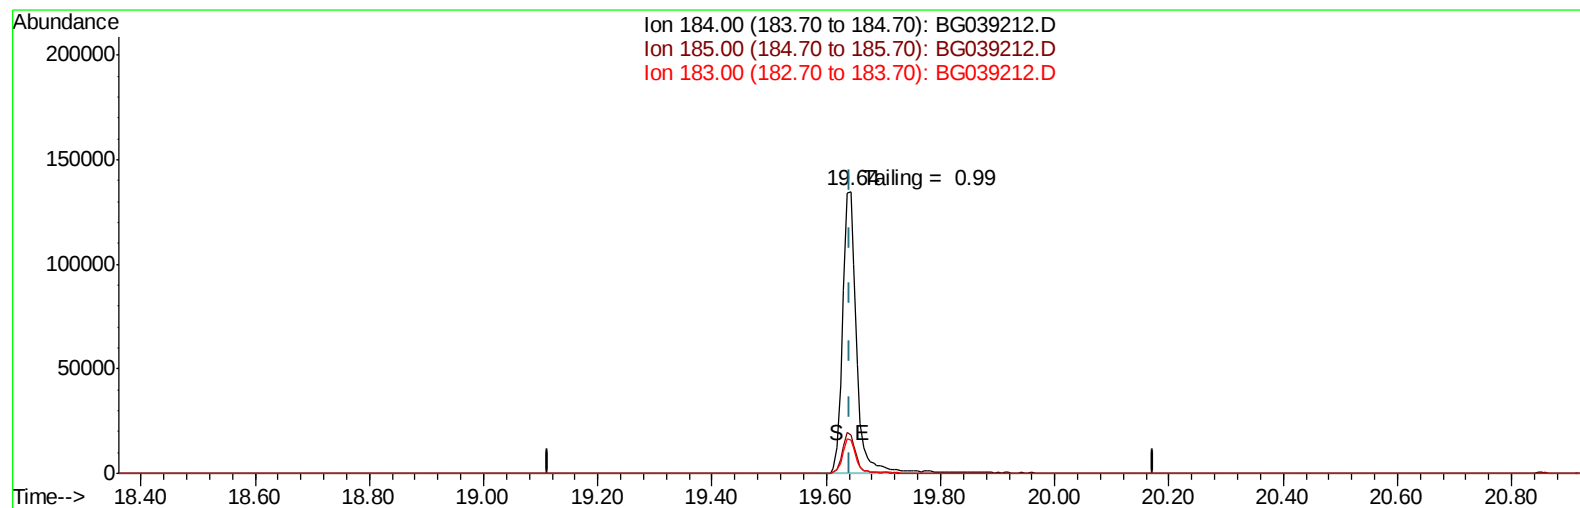

TIC: BG039212.D

(77) Benzidine




19.642min (-0.000) 0.00ng

response 226750

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	13.59
183.00	11.90	11.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011819\
Data File : BG039212.D
Acq On : 18 Jan 2019 11:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 22:42:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

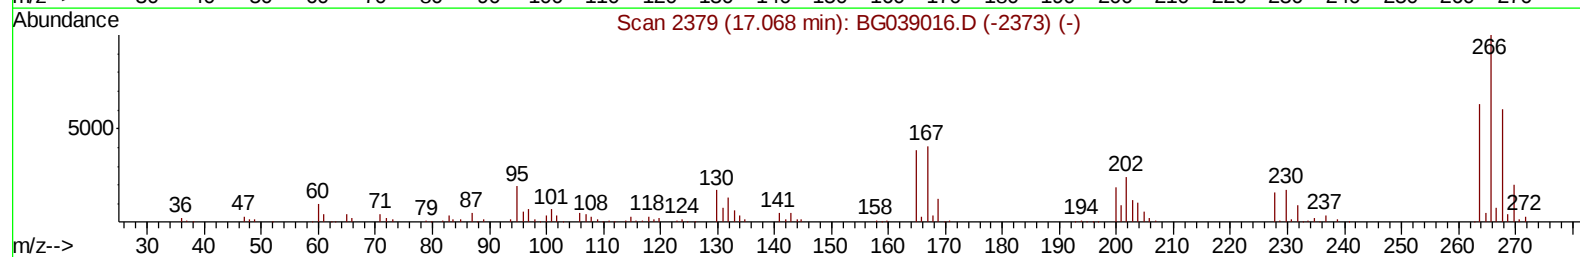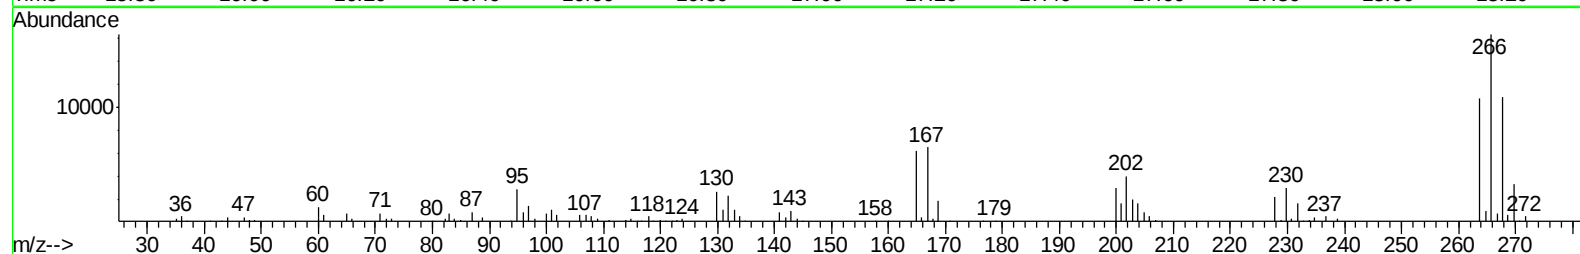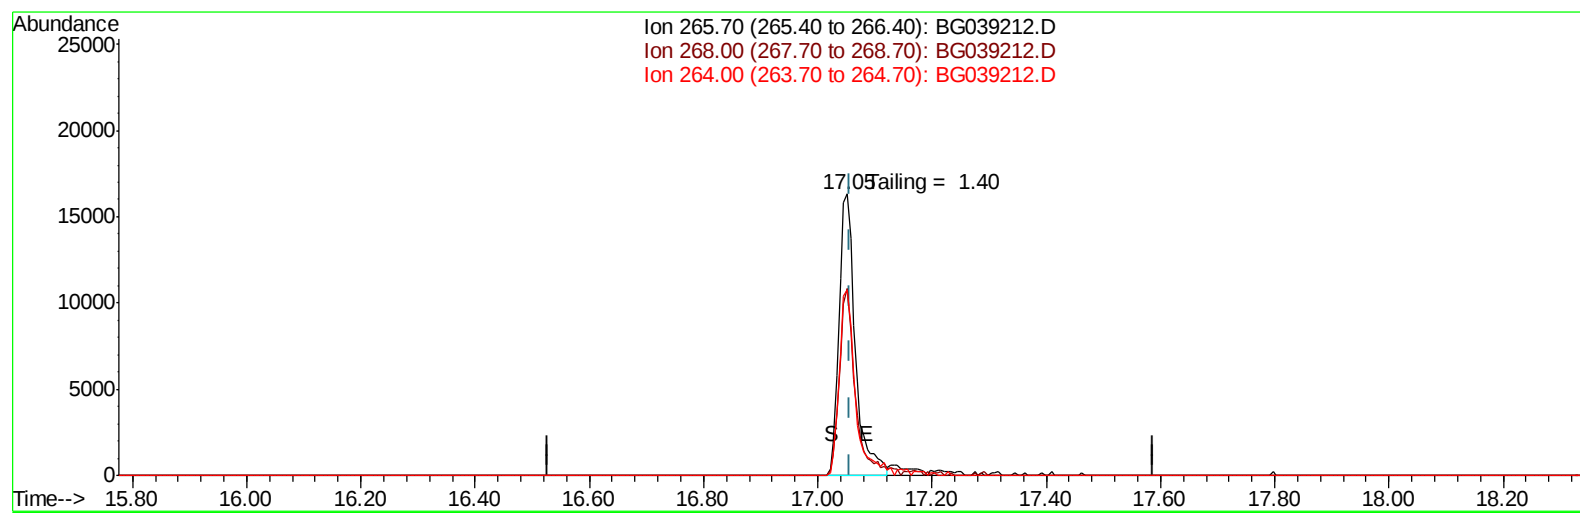

TIC: BG039212.D

(70) Pentachlorophenol (C)

17.051min (-0.006) 24740.54ng

response 32356

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	70.74
264.00	68.20	65.80
0.00	0.00	0.00