

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
 Data File : BG039222.D
 Acq On : 18 Jan 2019 19:14
 Operator : JU/SJ
 Sample : K1148-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 T-1

Quant Time: Jan 18 22:32:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	15933	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	58519	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	44978	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	120884	20.00	ng	0.00
76) Chrysene-d12	21.67	240	124792	20.00	ng	0.00
87) Perylene-d12	24.93	264	134778	20.00	ng	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.56	112	54460	64.84	ng	0.00
7) Phenol-d6	7.17	99	49214	40.71	ng	0.00
23) Nitrobenzene-d5	9.19	82	109009	101.93	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	110713	146.84	ng	0.00
45) 2-Fluorobiphenyl	13.27	172	316604	96.33	ng	0.00
79) Terphenyl-d14	20.00	244	617199	91.49	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
Data File : BG039222.D
Acq On : 18 Jan 2019 19:14
Operator : JU/SJ
Sample : K1148-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
T-1

Quant Time: Jan 18 22:32:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

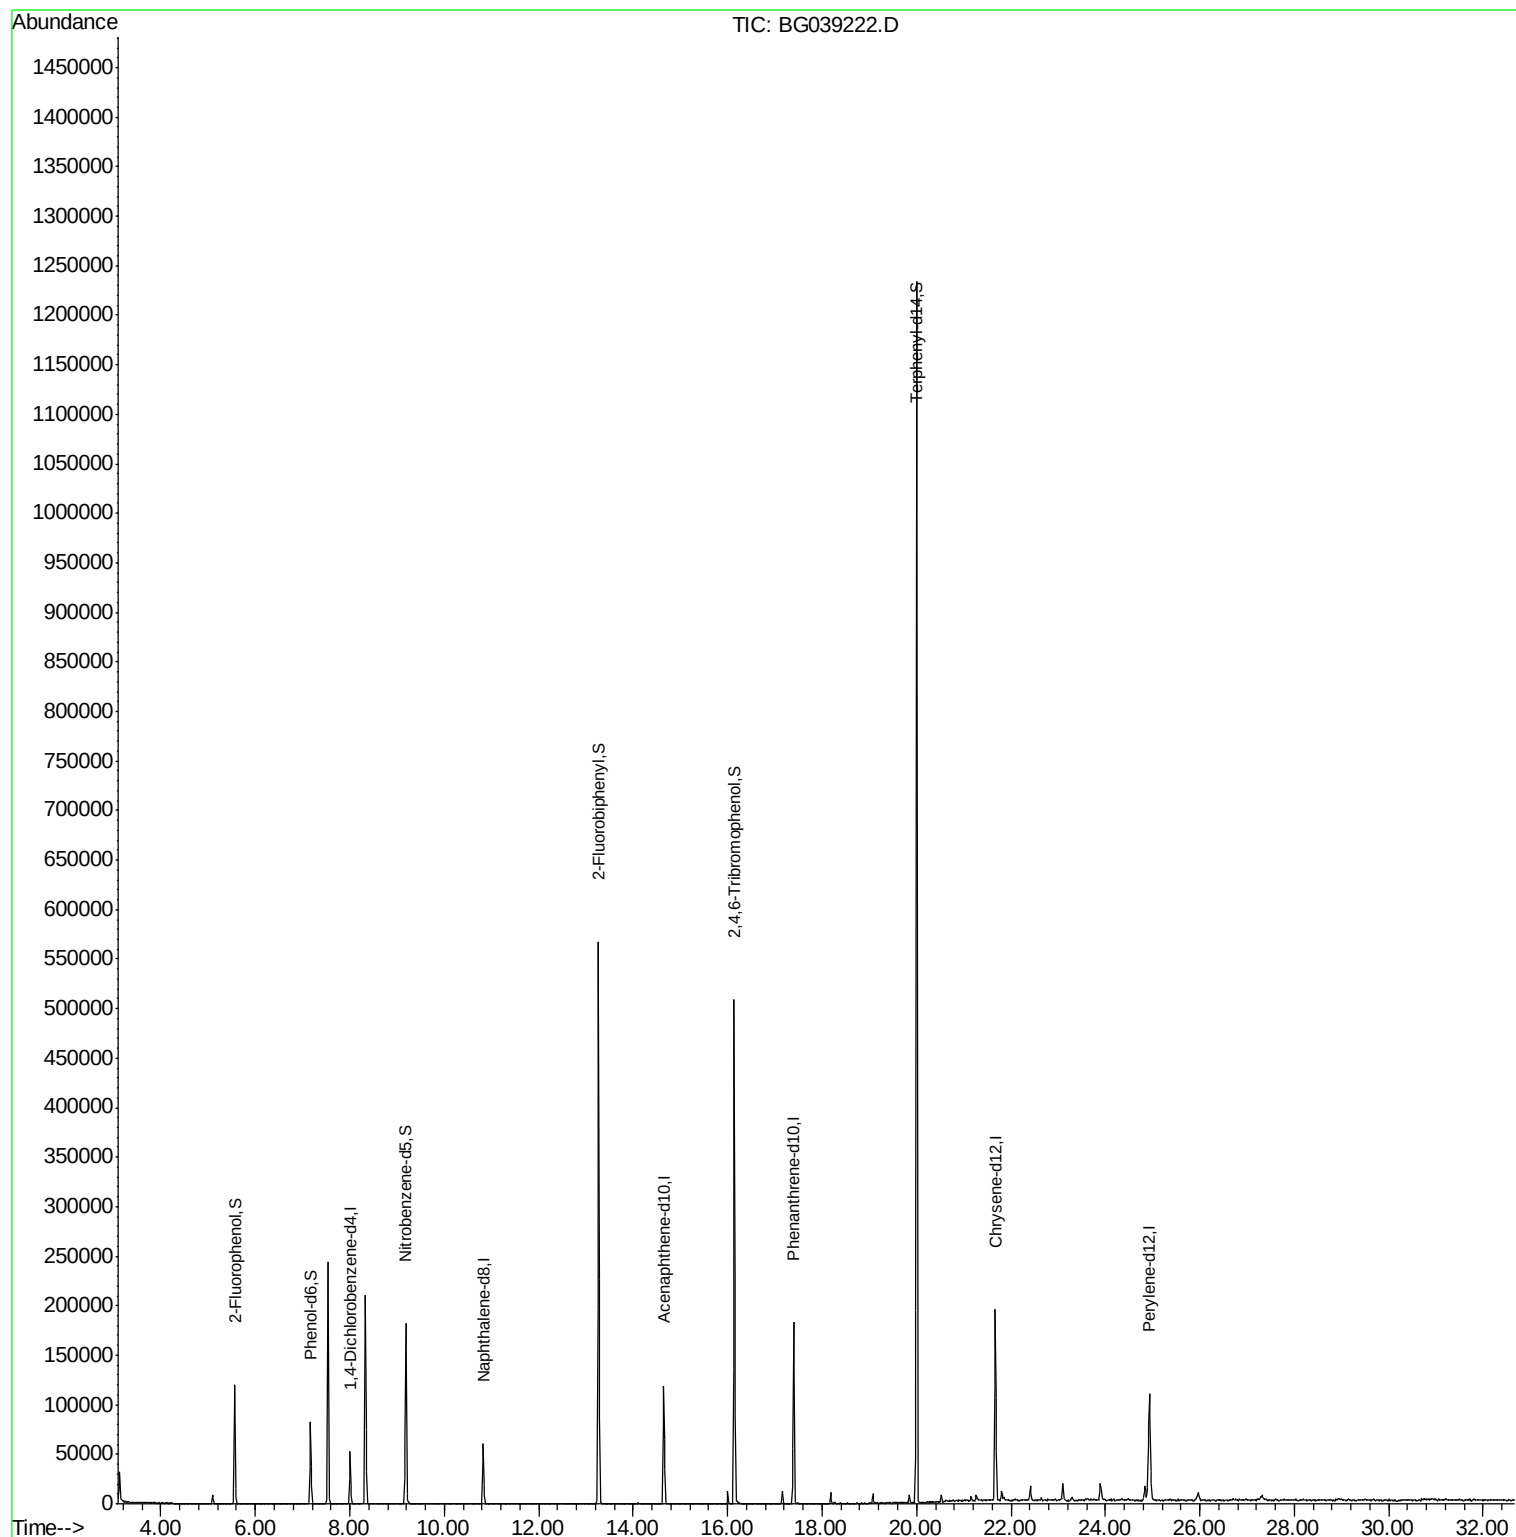

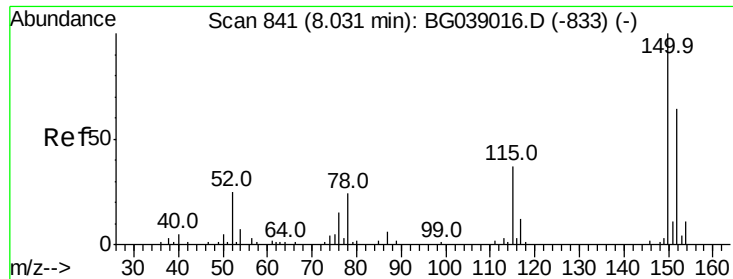


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039222.D
Acq: 18 Jan 2019 19:14

Instrument :
BNA_G
ClientSampleId :
T-1

Tot Ion:152 Resp: 15933
Ion Ratio Lower Upper
152 100
150 155.0 124.7 187.1
115 50.7 46.5 69.7

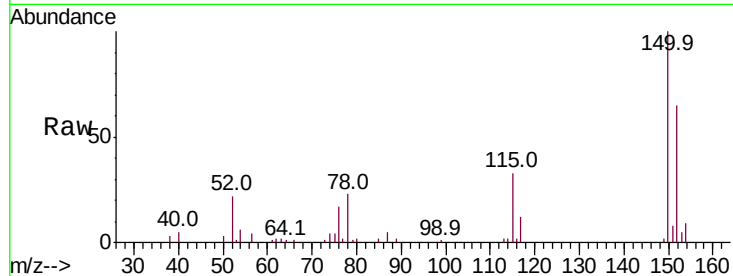


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

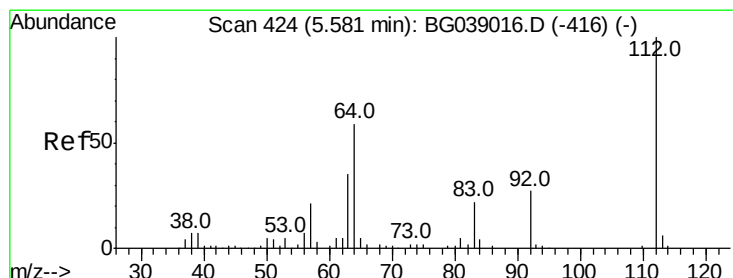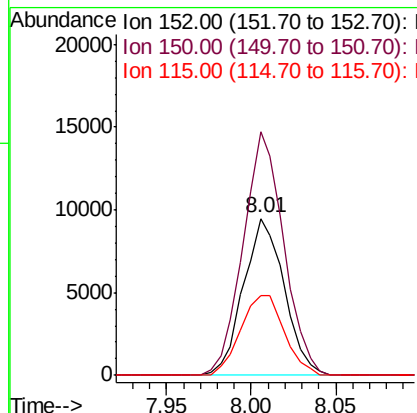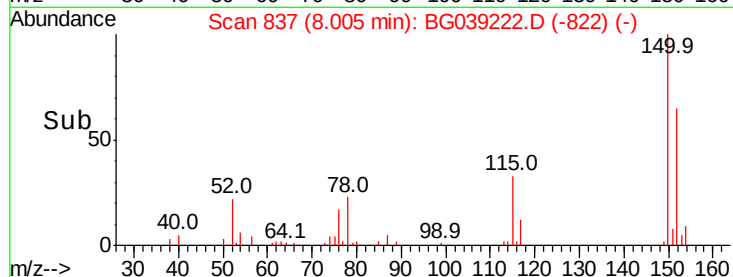



#5


2-Fluorophenol
Concen: 64.840 ng
RT: 5.56 min Scan# 421
Delta R.T. -0.00 min
Lab File: BG039222.D
Acq: 18 Jan 2019 19:14

Tgt Ion:112 Resp: 54460
Ion Ratio Lower Upper
112 100
64 62.6 47.0 70.6
63 34.5 28.0 42.0

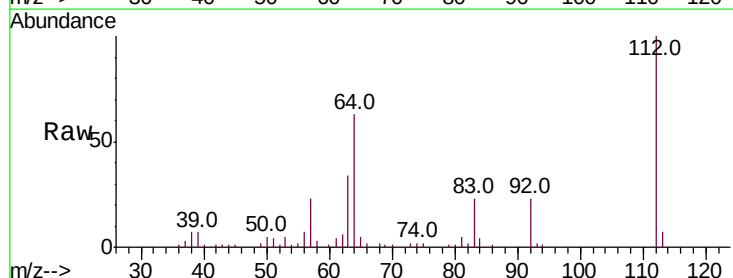

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

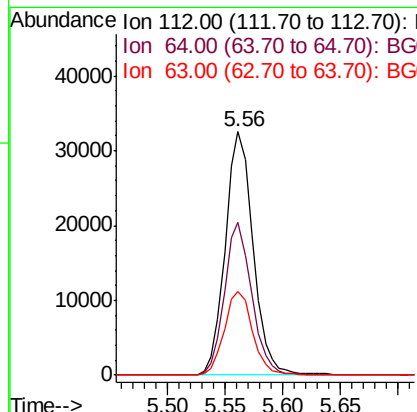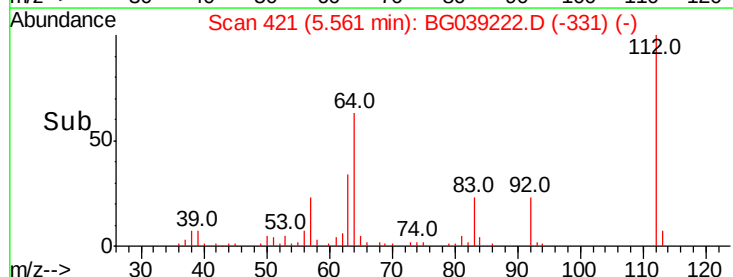

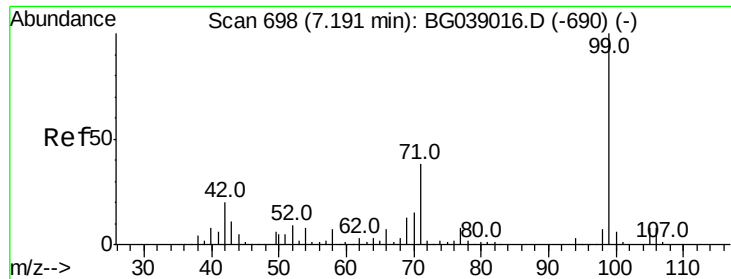

#7

Phenol-d6

Concen: 40.715 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG039222.D

Acq: 18 Jan 2019 19:14

Instrument :

BNA_G

ClientSampleId :

T-1


Tot Ion: 99 Resp: 49214

Ion Ratio Lower Upper




99 100

42 20.4 15.8 23.6

71 36.9 30.2 45.4

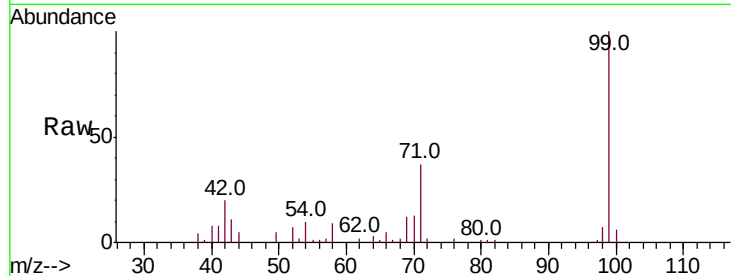

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

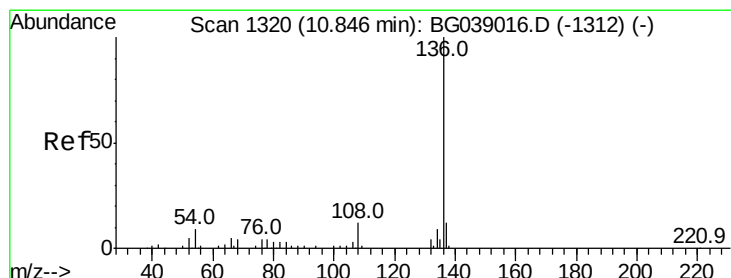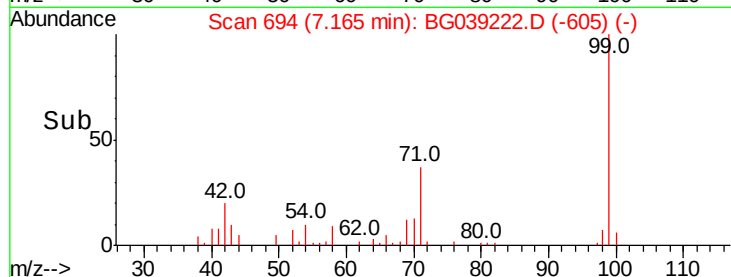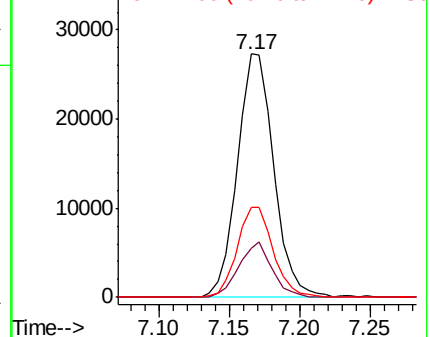

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1317

Delta R.T. -0.00 min

Lab File: BG039222.D

Acq: 18 Jan 2019 19:14

Tgt Ion: 136 Resp: 58519


Ion Ratio Lower Upper

136 100



137 11.5 9.4 14.2


54 9.0 7.2 10.8

68 4.4 3.5 5.3

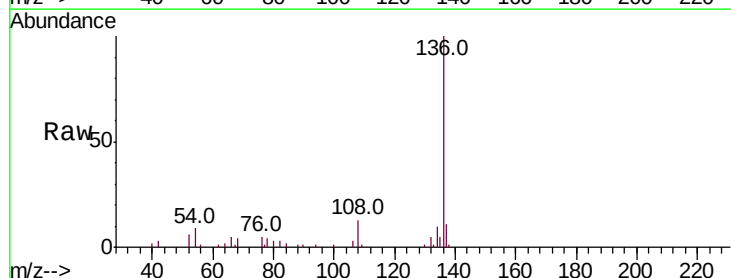

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

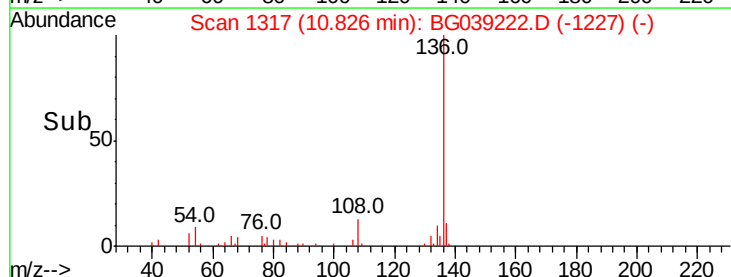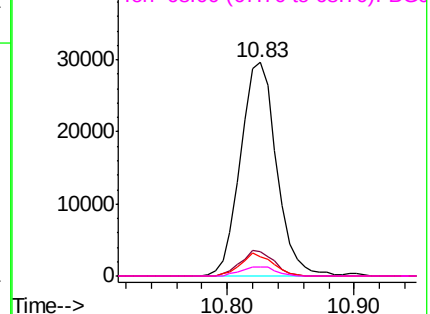


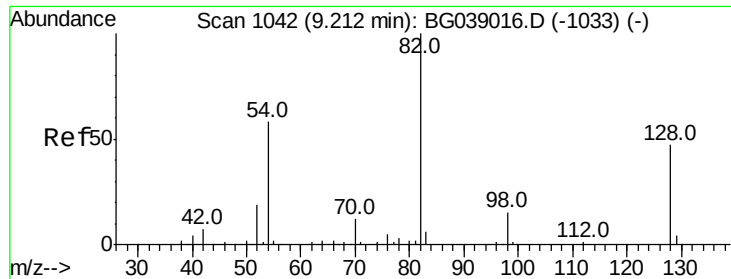




#23
 Nitrobenzene-d5
 Concen: 101.931 ng
 RT: 9.19 min Scan# 1038
 Delta R.T. -0.00 min
 Lab File: BG039222.D
 Acq: 18 Jan 2019 19:14

Instrument :
 BNA_G
 ClientSampleId :
 T-1

Tot Ion	82	Resp	109009
Ion Ratio	Lower	Upper	
82	100		
128	43.4	37.3	55.9
54	60.0	46.4	69.6

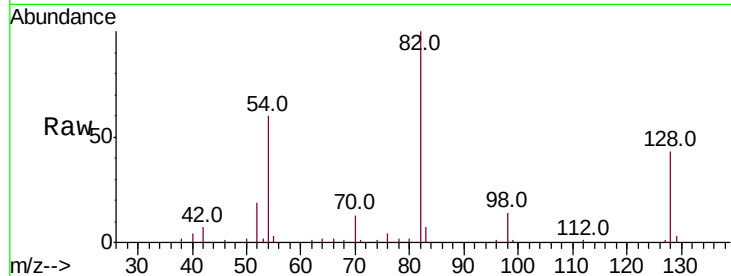


Abundance Ion 82.00 (81.70 to 82.70): BG039016.D (-1033) (-)

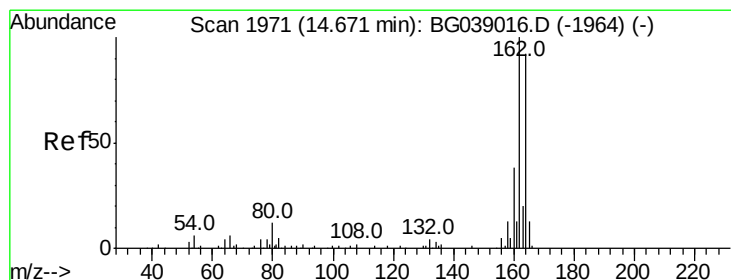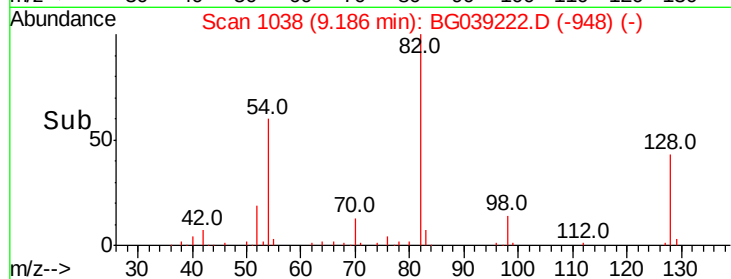
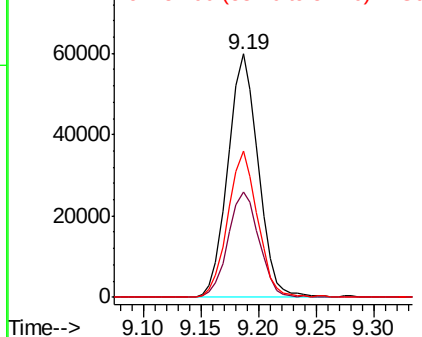



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.65 min Scan# 1968
 Delta R.T. -0.00 min
 Lab File: BG039222.D
 Acq: 18 Jan 2019 19:14

Tgt Ion	164	Resp	44978
Ion Ratio	Lower	Upper	
164	100		
162	99.8	87.2	130.8
160	44.8	33.3	49.9

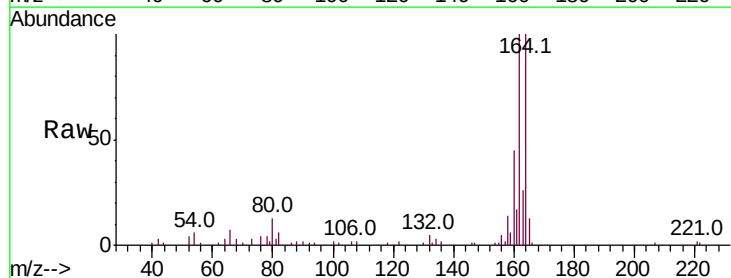

Abundance Ion 164.00 (163.70 to 164.70): BG039016.D (-1964) (-)

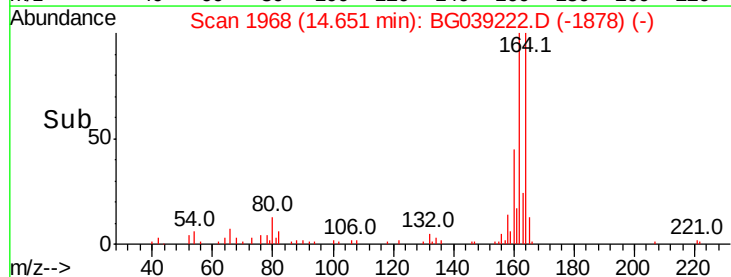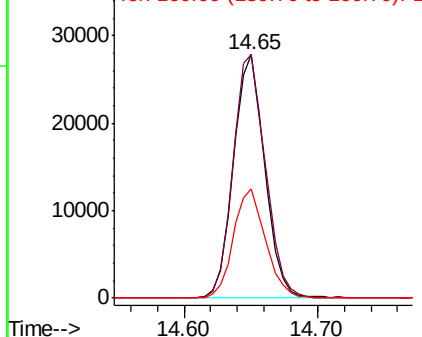


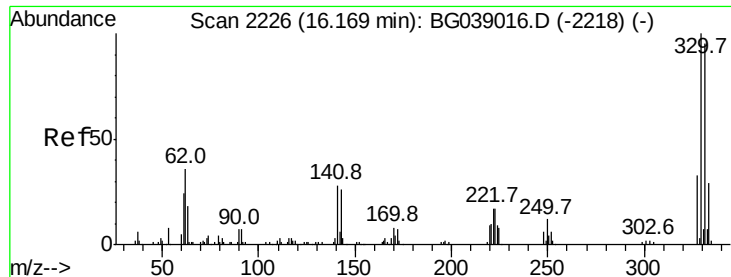




#42
 2,4,6-Tribromophenol
 Concen: 146.843 ng
 RT: 16.14 min Scan# 2222
 Delta R.T. -0.01 min
 Lab File: BG039222.D
 Acq: 18 Jan 2019 19:14

Instrument :
 BNA_G
 ClientSampleId :
 T-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.3	75.7	113.5
141	31.1	24.9	37.3

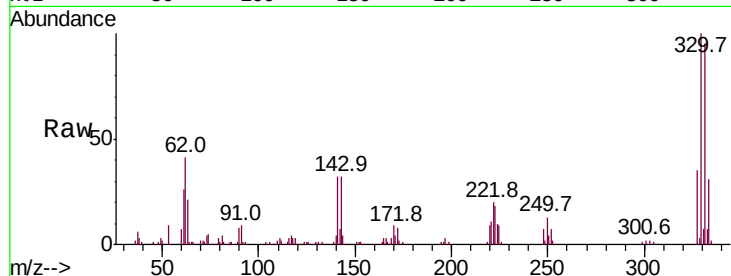


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

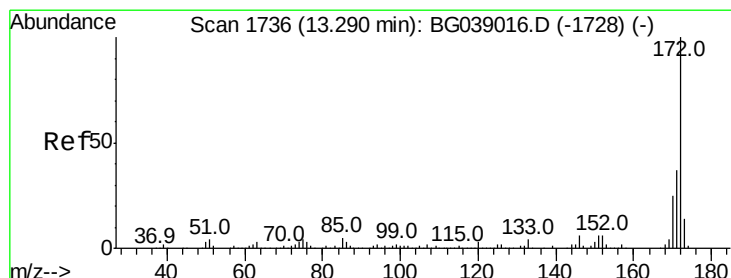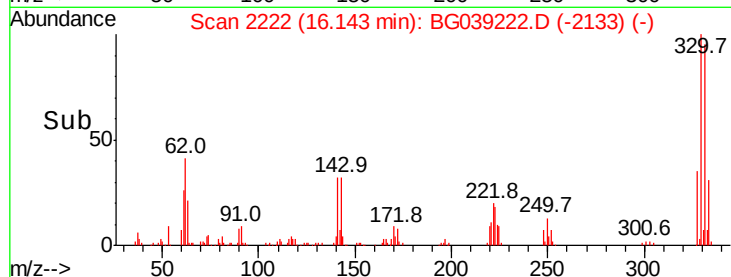
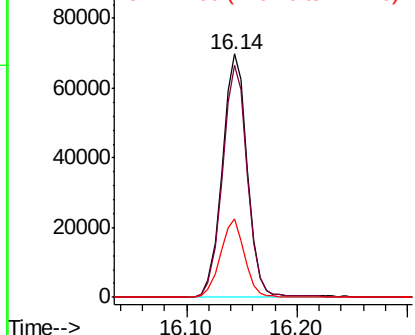



#45
 2-Fluorobiphenyl
 Concen: 96.334 ng
 RT: 13.27 min Scan# 1733
 Delta R.T. -0.00 min
 Lab File: BG039222.D
 Acq: 18 Jan 2019 19:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	29.4	44.0
170	24.3	20.1	30.1

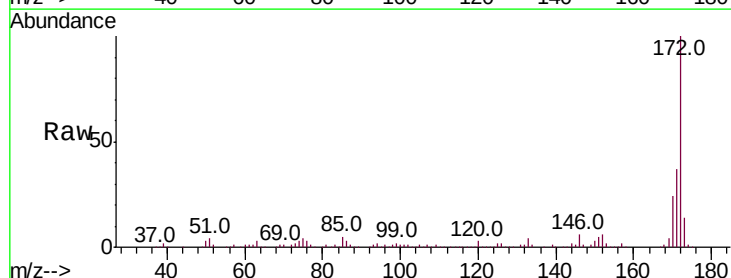

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

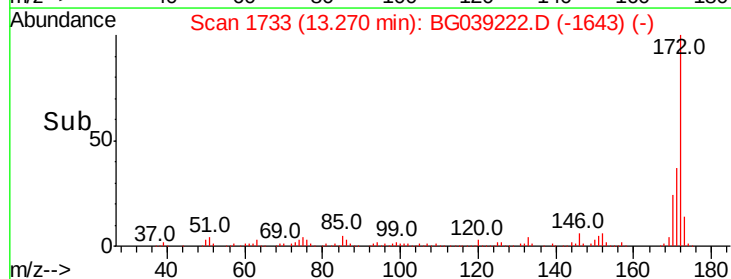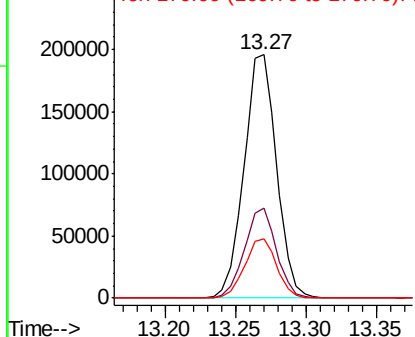


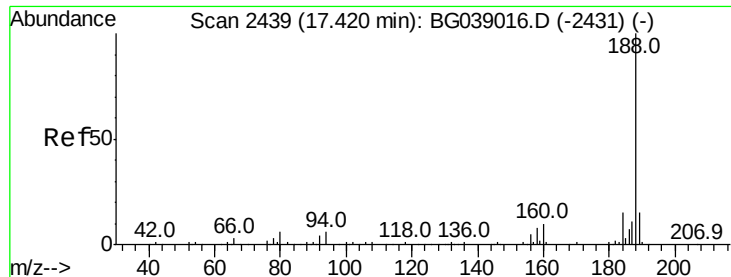




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.40 min Scan# 2436
Delta R.T. -0.00 min
Lab File: BG039222.D
Acq: 18 Jan 2019 19:14

Instrument :
BNA_G
ClientSampled :
T-1

Tot Ion:188 Resp: 120884
Ion Ratio Lower Upper
188 100
94 5.9 5.0 7.4
80 6.7 4.7 7.1

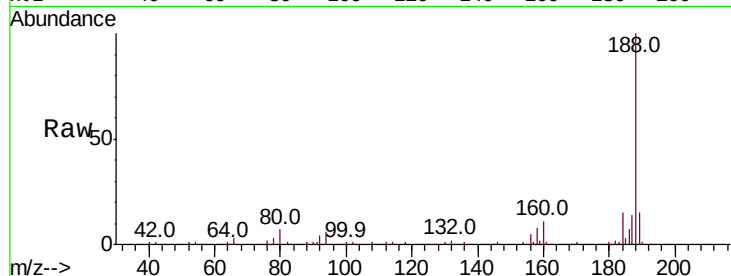


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

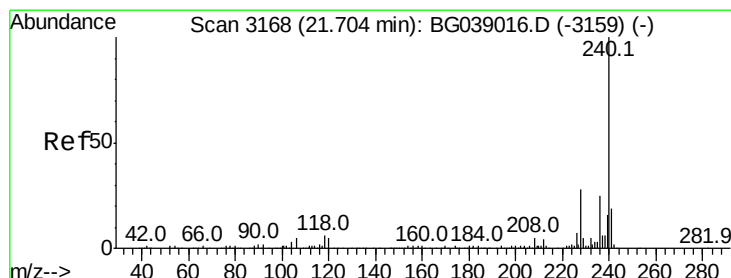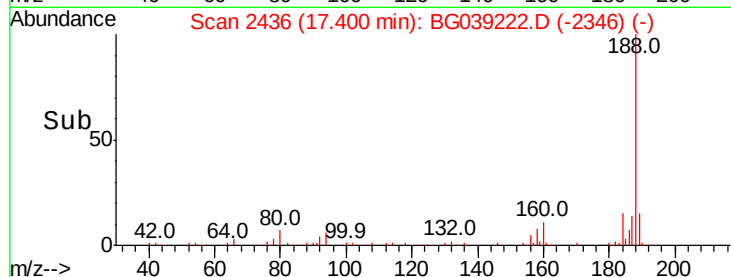
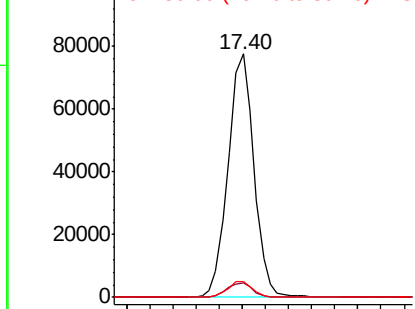



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3163
Delta R.T. -0.01 min
Lab File: BG039222.D
Acq: 18 Jan 2019 19:14

Tgt Ion:240 Resp: 124792
Ion Ratio Lower Upper
240 100
120 6.4 4.3 6.5
236 26.6 20.1 30.1

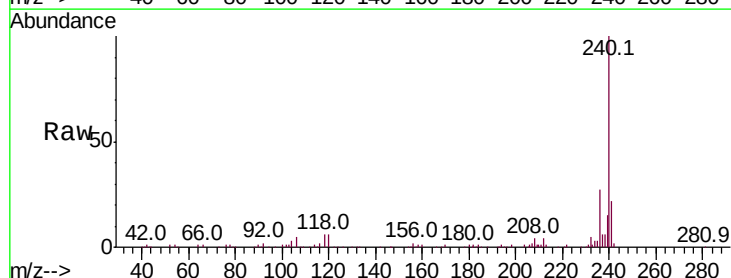

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

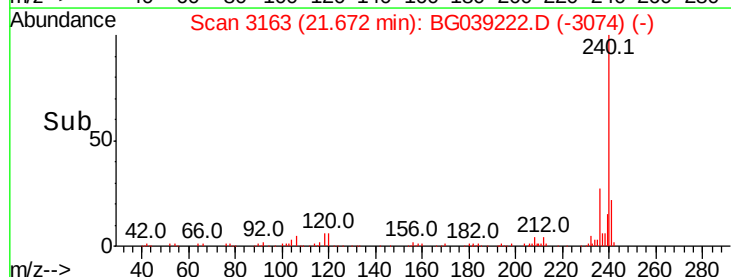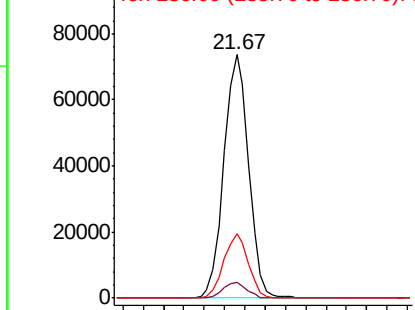

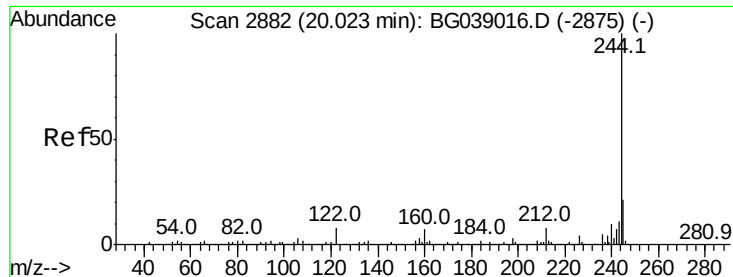

#79

Terphenyl-d14

Concen: 91.492 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG039222.D

Acq: 18 Jan 2019 19:14

Instrument :

BNA_G

ClientSampleId :

T-1


Tot Ion:244 Resp: 617199

Ion Ratio Lower Upper

244 100

212 7.5 6.1 9.1




122 6.9 6.1 9.1

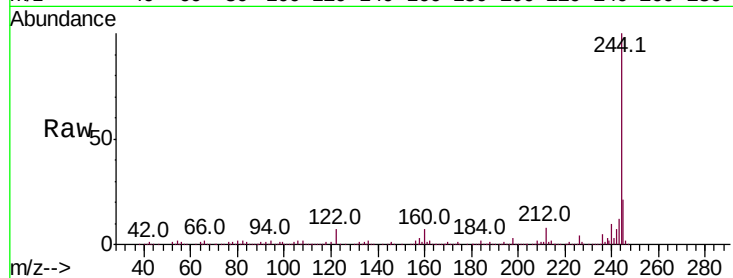

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

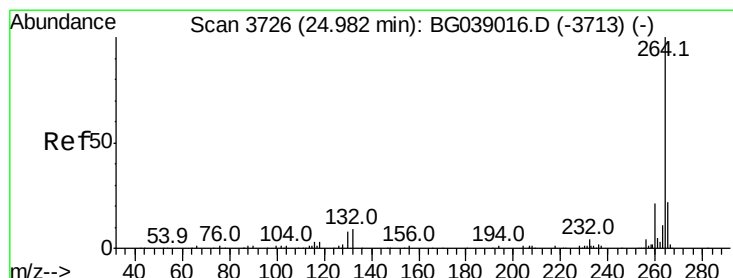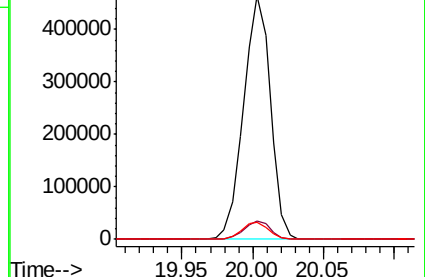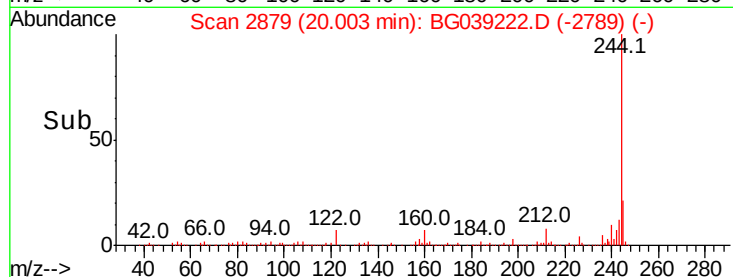

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3718

Delta R.T. -0.02 min

Lab File: BG039222.D

Acq: 18 Jan 2019 19:14


Tgt Ion:264 Resp: 134778

Ion Ratio Lower Upper

264 100

260 21.9 17.0 25.6

265 21.2 17.2 25.8

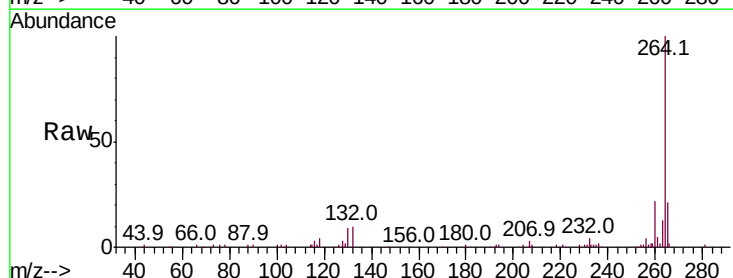

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

