

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
 Data File : BG039224.D
 Acq On : 18 Jan 2019 20:32
 Operator : JU/SJ
 Sample : K1178-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-03

Quant Time: Jan 18 22:36:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	15022	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	73046	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	43272	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	114863	20.00	ng	0.00
76) Chrysene-d12	21.67	240	115564	20.00	ng	-0.01
87) Perylene-d12	24.93	264	123155	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	73883	93.30	ng	0.00
7) Phenol-d6	7.17	99	80349	70.50	ng	0.00
23) Nitrobenzene-d5	9.19	82	92439	69.25	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	102617	141.47	ng	-0.01
45) 2-Fluorobiphenyl	13.27	172	277805	87.86	ng	0.00
79) Terphenyl-d14	20.00	244	562683	90.07	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
Data File : BG039224.D
Acq On : 18 Jan 2019 20:32
Operator : JU/SJ
Sample : K1178-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-03

Quant Time: Jan 18 22:36:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

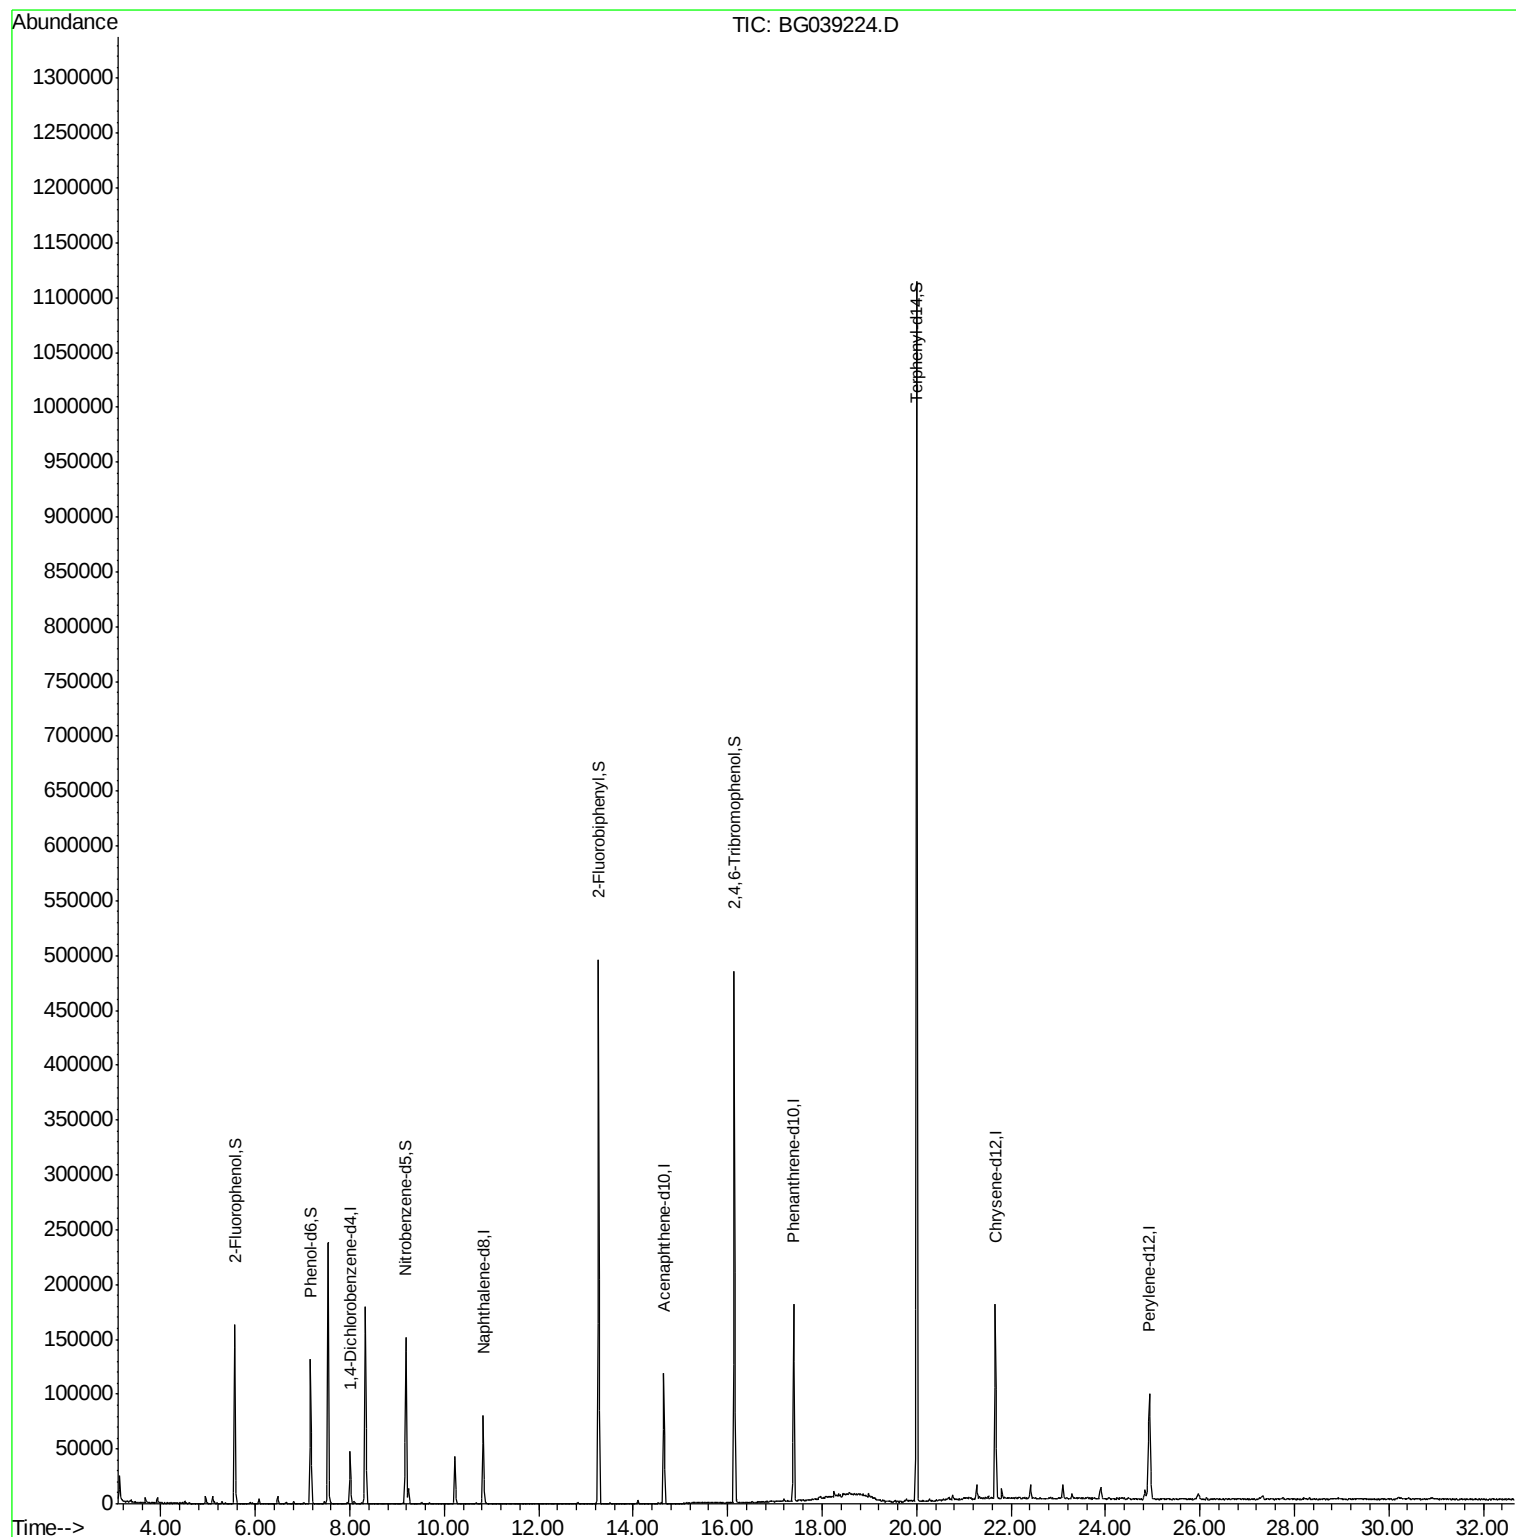




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 838
Delta R.T. -0.00 min
Lab File: BG039224.D
Acq: 18 Jan 2019 20:32

Instrument :
BNA_G
ClientSampleId :
MW-03

Tot Ion:152 Resp: 15022
Ion Ratio Lower Upper
152 100
150 147.1 124.7 187.1
115 50.3 46.5 69.7

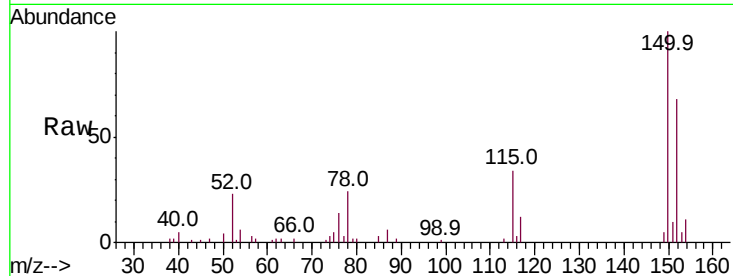


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

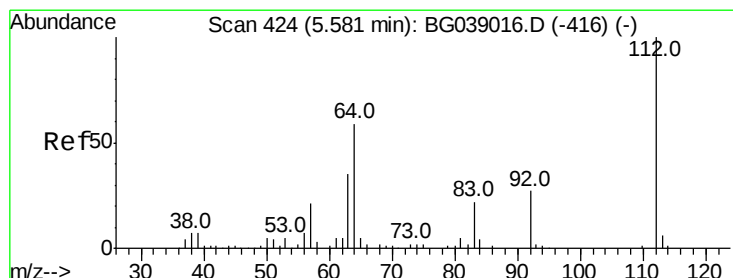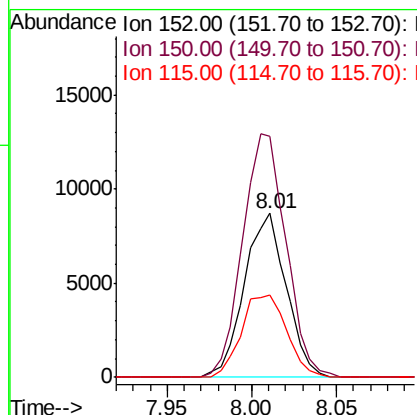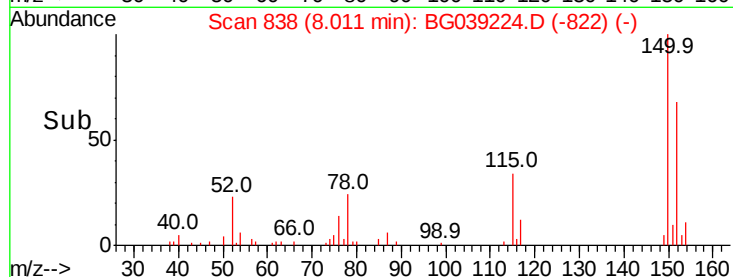



#5


2-Fluorophenol
Concen: 93.300 ng
RT: 5.56 min Scan# 421
Delta R.T. -0.00 min
Lab File: BG039224.D
Acq: 18 Jan 2019 20:32

Tgt Ion:112 Resp: 73883
Ion Ratio Lower Upper
112 100
64 59.6 47.0 70.6
63 34.2 28.0 42.0

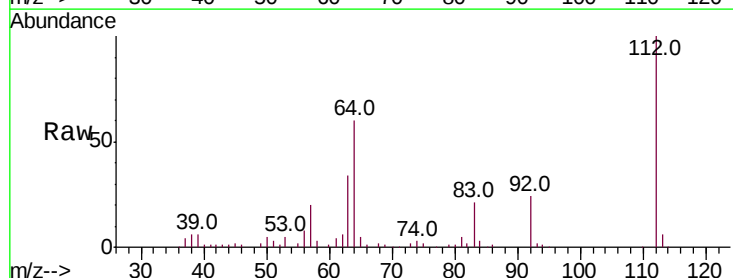

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

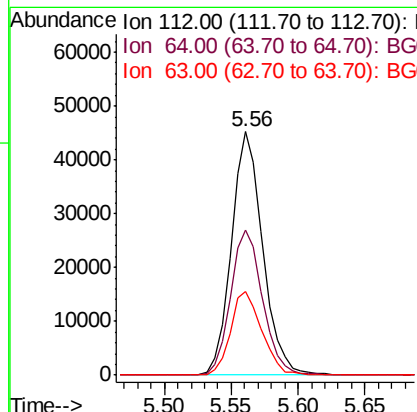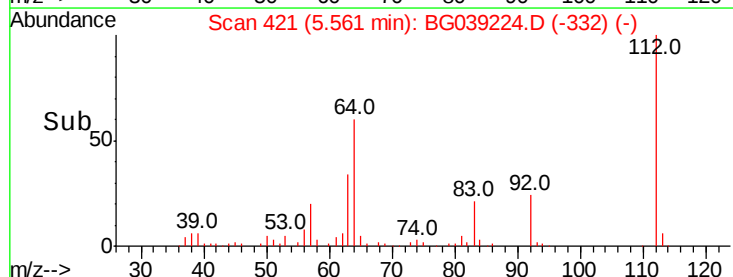

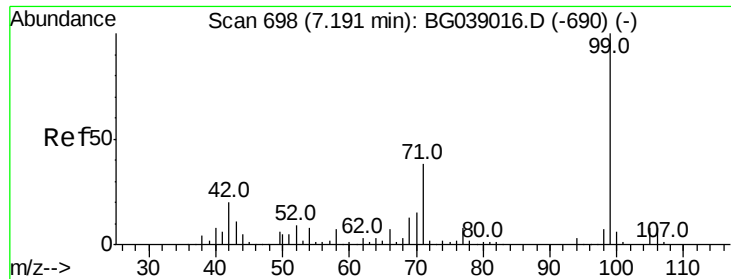

#7

Phenol-d6

Concen: 70.504 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.00 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32

Instrument :

BNA_G

ClientSampleId :

MW-03


Tot Ion: 99 Resp: 80349

Ion Ratio Lower Upper




99 100

42 18.7 15.8 23.6

71 34.9 30.2 45.4

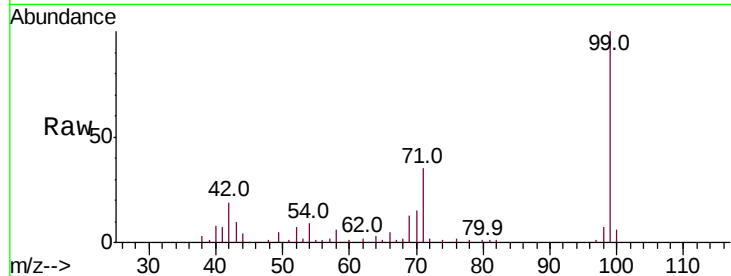

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

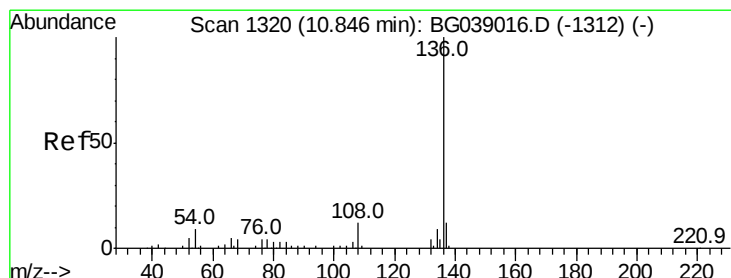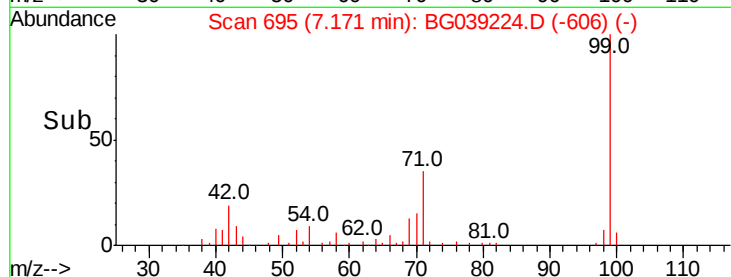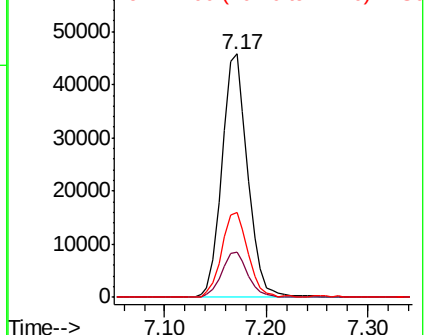

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1317

Delta R.T. -0.00 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32

Tgt Ion: 136 Resp: 73046


Ion Ratio Lower Upper

136 100



137 11.4 9.4 14.2


54 9.9 7.2 10.8

68 4.5 3.5 5.3

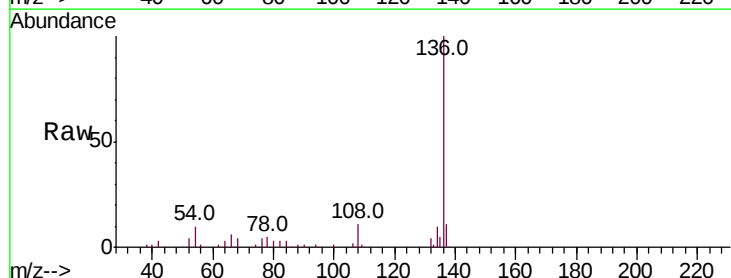

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



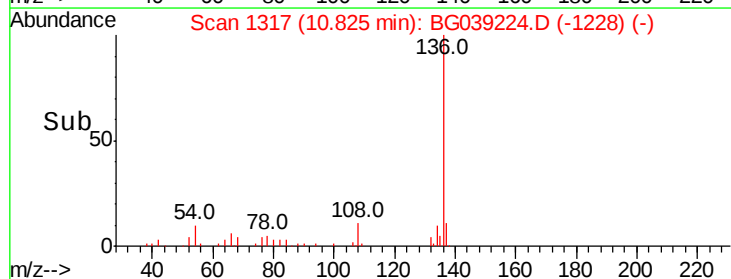
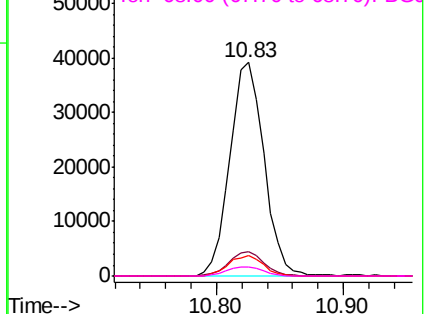


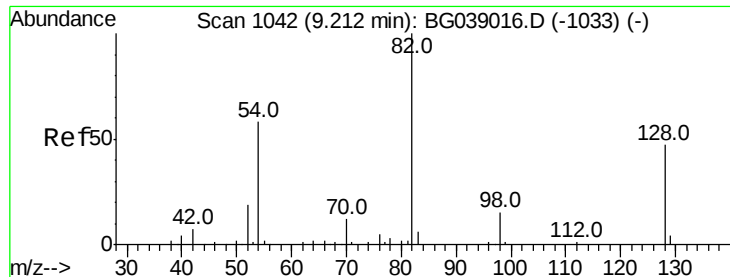

#23
Nitrobenzene-d5
Concen: 69.247 ng
RT: 9.19 min Scan# 1038
Delta R.T. -0.00 min
Lab File: BG039224.D
Acq: 18 Jan 2019 20:32




Instrument :
BNA_G
ClientSampleId :
MW-03


Tot Ion: 82 Resp: 92439
Ion Ratio Lower Upper
82 100
128 43.2 37.3 55.9
54 59.5 46.4 69.6

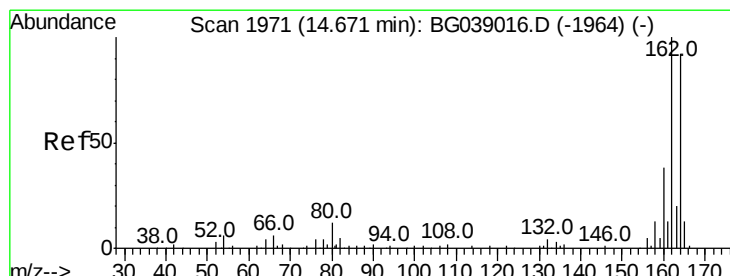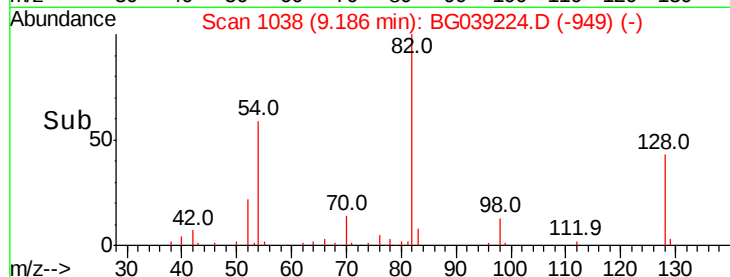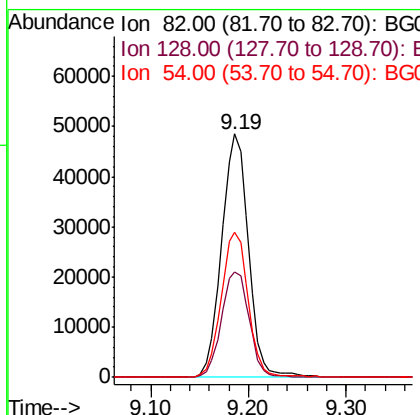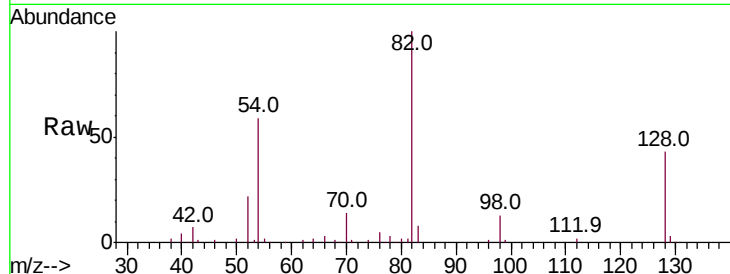

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1968
Delta R.T. -0.00 min
Lab File: BG039224.D
Acq: 18 Jan 2019 20:32

Tgt Ion:164 Resp: 43272
Ion Ratio Lower Upper
164 100
162 101.0 87.2 130.8
160 42.6 33.3 49.9

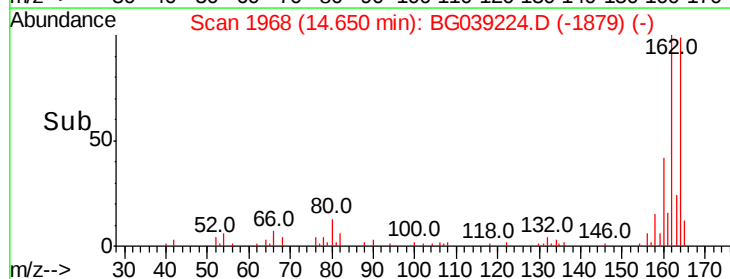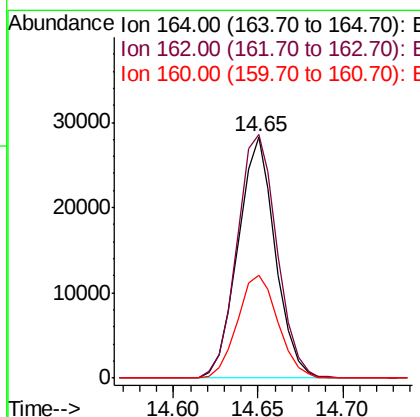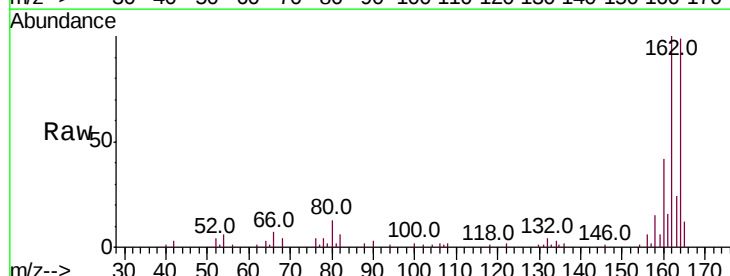


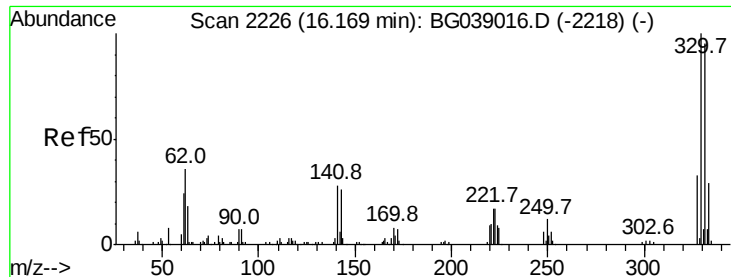




#42
 2,4,6-Tribromophenol
 Concen: 141.471 ng
 RT: 16.14 min Scan# 2222
 Delta R.T. -0.01 min
 Lab File: BG039224.D
 Acq: 18 Jan 2019 20:32

Instrument :
 BNA_G
 ClientSampleId :
 MW-03

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	75.7	113.5
141	31.7	24.9	37.3

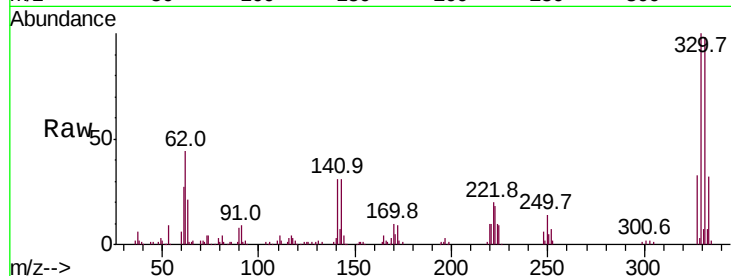


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

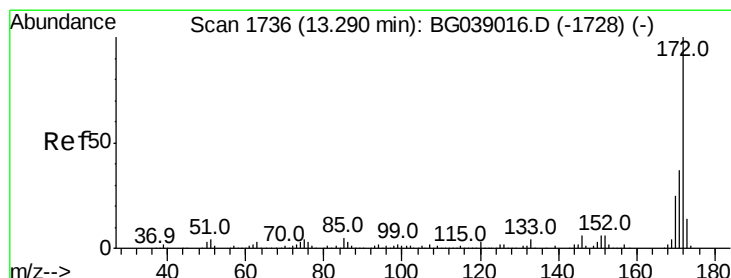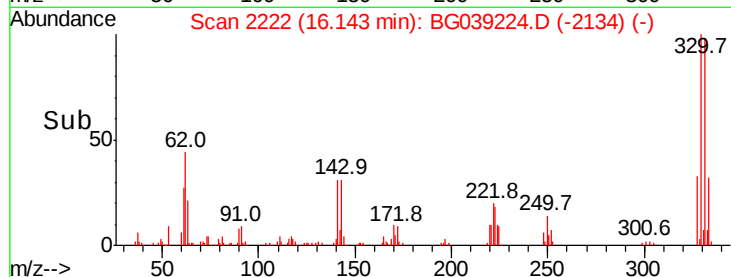
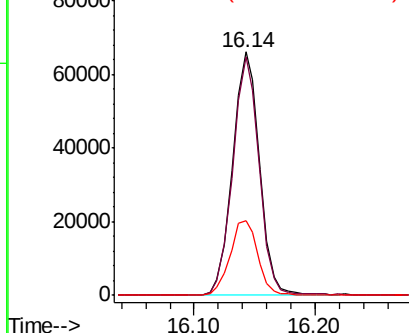



#45
 2-Fluorobiphenyl
 Concen: 87.861 ng
 RT: 13.27 min Scan# 1733
 Delta R.T. -0.00 min
 Lab File: BG039224.D
 Acq: 18 Jan 2019 20:32

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.4	44.0
170	23.4	20.1	30.1

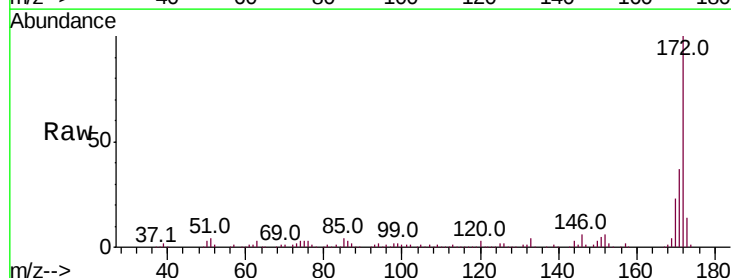

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

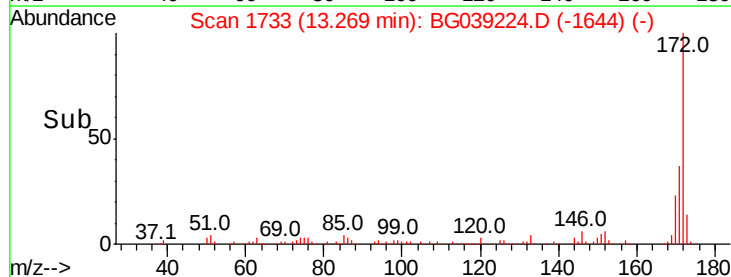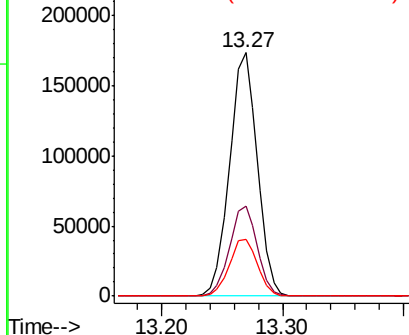

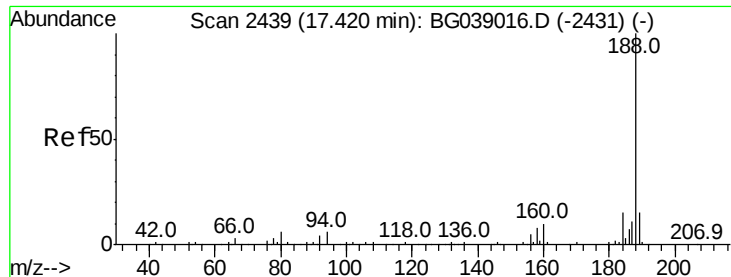

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2436

Delta R.T. -0.00 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32

Instrument :

BNA_G

ClientSampled :

MW-03


Tot Ion:188 Resp: 114863

Ion Ratio Lower Upper

188 100

94 5.1 5.0 7.4




80 6.1 4.7 7.1

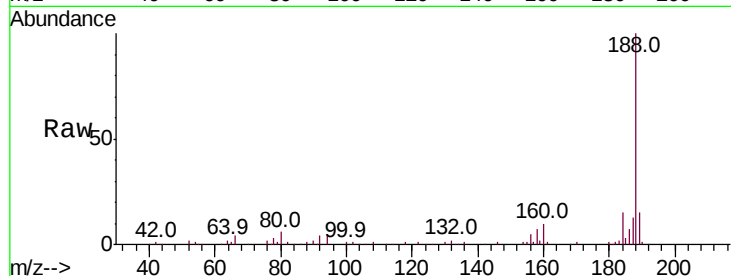

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

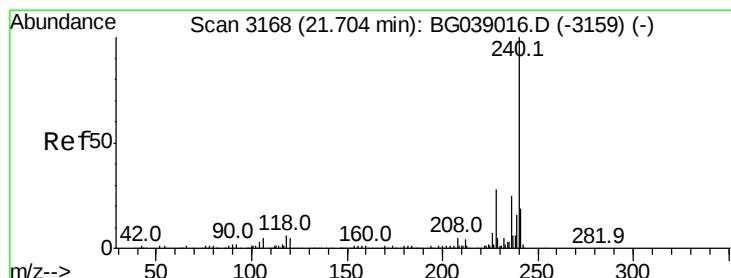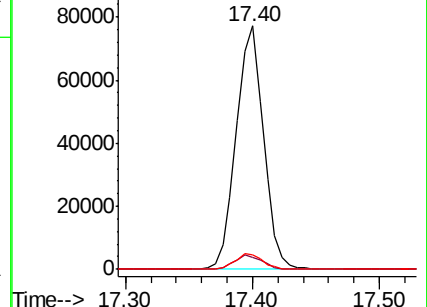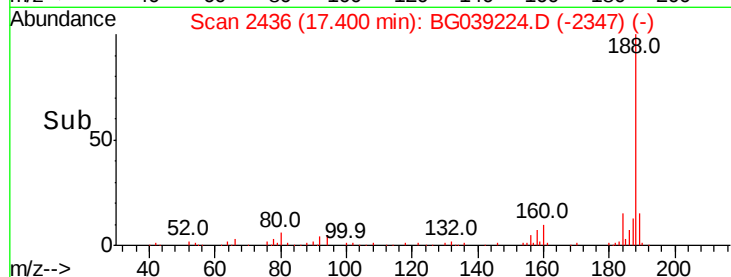

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3163

Delta R.T. -0.01 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32


Tgt Ion:240 Resp: 115564

Ion Ratio Lower Upper

240 100

120 5.9 4.3 6.5



236 24.6 20.1 30.1

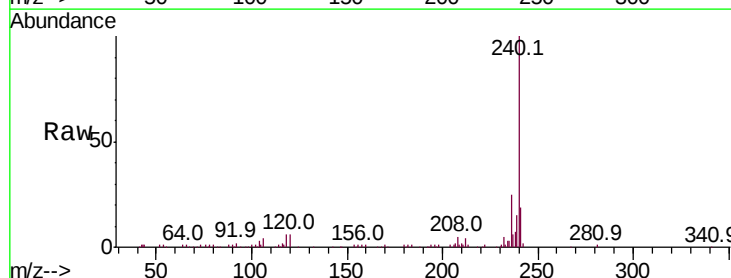


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

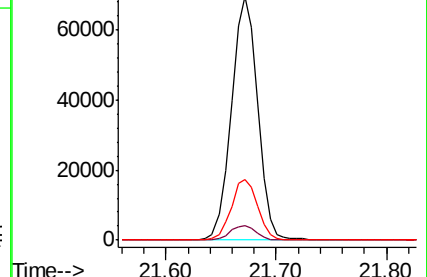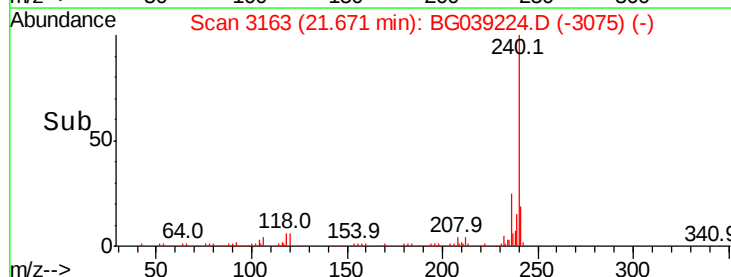

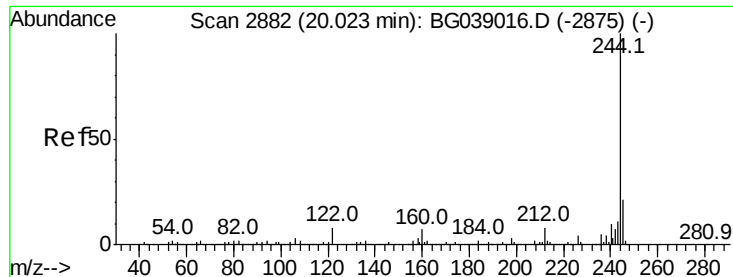

#79

Terphenyl-d14

Concen: 90.072 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32

Instrument :

BNA_G

ClientSampleId :

MW-03


Tot Ion:244 Resp: 562683

Ion Ratio Lower Upper

244 100

212 7.2 6.1 9.1




122 7.2 6.1 9.1

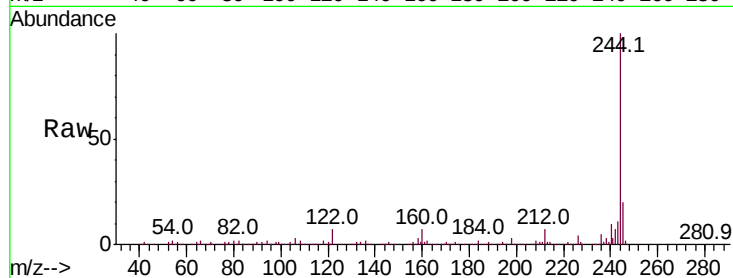

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

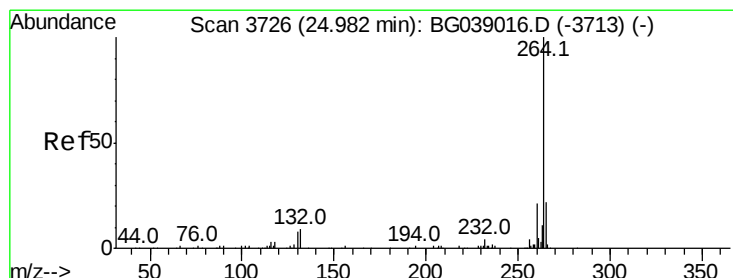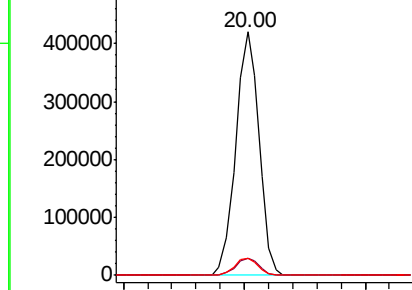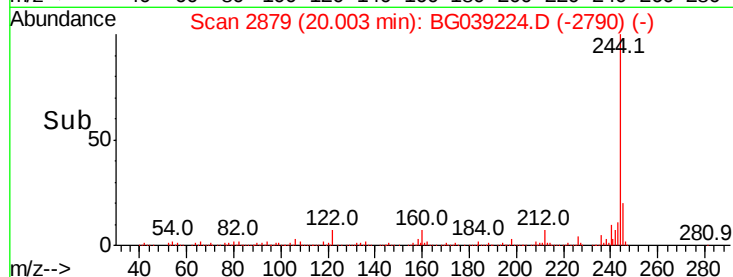

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3718

Delta R.T. -0.02 min

Lab File: BG039224.D

Acq: 18 Jan 2019 20:32


Tgt Ion:264 Resp: 123155

Ion Ratio Lower Upper

264 100

260 22.6 17.0 25.6

265 21.9 17.2 25.8

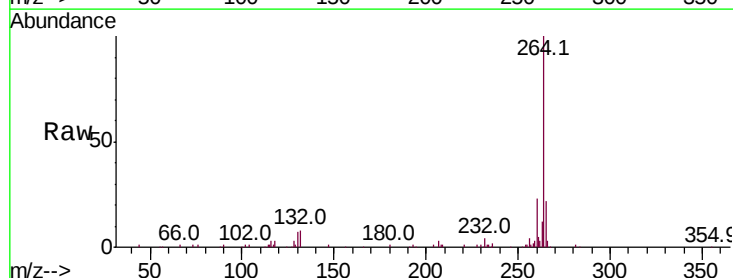

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

