

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
 Data File : BG039215.D
 Acq On : 18 Jan 2019 14:30
 Operator : JU/SJ
 Sample : PB116467BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB116467BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	336	341	349	rBV	13965	22769	1.72%	0.397%
2	5.562	414	421	435	rVB	262319	429240	32.50%	7.483%
3	7.172	688	695	705	rBV	240048	411337	31.14%	7.171%
4	7.536	750	757	769	rVB	224315	390758	29.58%	6.812%
5	8.006	831	837	844	rBB	45059	74871	5.67%	1.305%
6	8.330	884	892	900	rBV	166008	283737	21.48%	4.946%
7	9.181	1030	1037	1050	rBV	133096	243807	18.46%	4.250%
8	10.827	1310	1317	1328	rBV	58082	106803	8.09%	1.862%
9	13.271	1726	1733	1744	rBV	445144	691166	52.32%	12.049%
10	14.652	1962	1968	1980	rVB2	120791	204577	15.49%	3.566%
11	16.144	2215	2222	2235	rBV	395695	621616	47.06%	10.837%
12	17.401	2429	2436	2449	rBV	162129	250879	18.99%	4.374%
13	20.004	2873	2879	2887	rBV	975643	1320925	100.00%	23.028%
14	21.673	3156	3163	3175	rVB	195772	319482	24.19%	5.570%
15	22.413	3284	3289	3298	rVB3	13381	21186	1.60%	0.369%
16	23.100	3400	3406	3413	rVB2	12946	23958	1.81%	0.418%
17	23.900	3535	3542	3549	rBV3	7980	18757	1.42%	0.327%
18	24.840	3693	3702	3707	rBV6	6900	16519	1.25%	0.288%
19	24.928	3707	3717	3733	rVB2	94130	283866	21.49%	4.949%


Sum of corrected areas: 5736253

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
Data File : BG039215.D
Acq On : 18 Jan 2019 14:30
Operator : JU/SJ
Sample : PB116467BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116467BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

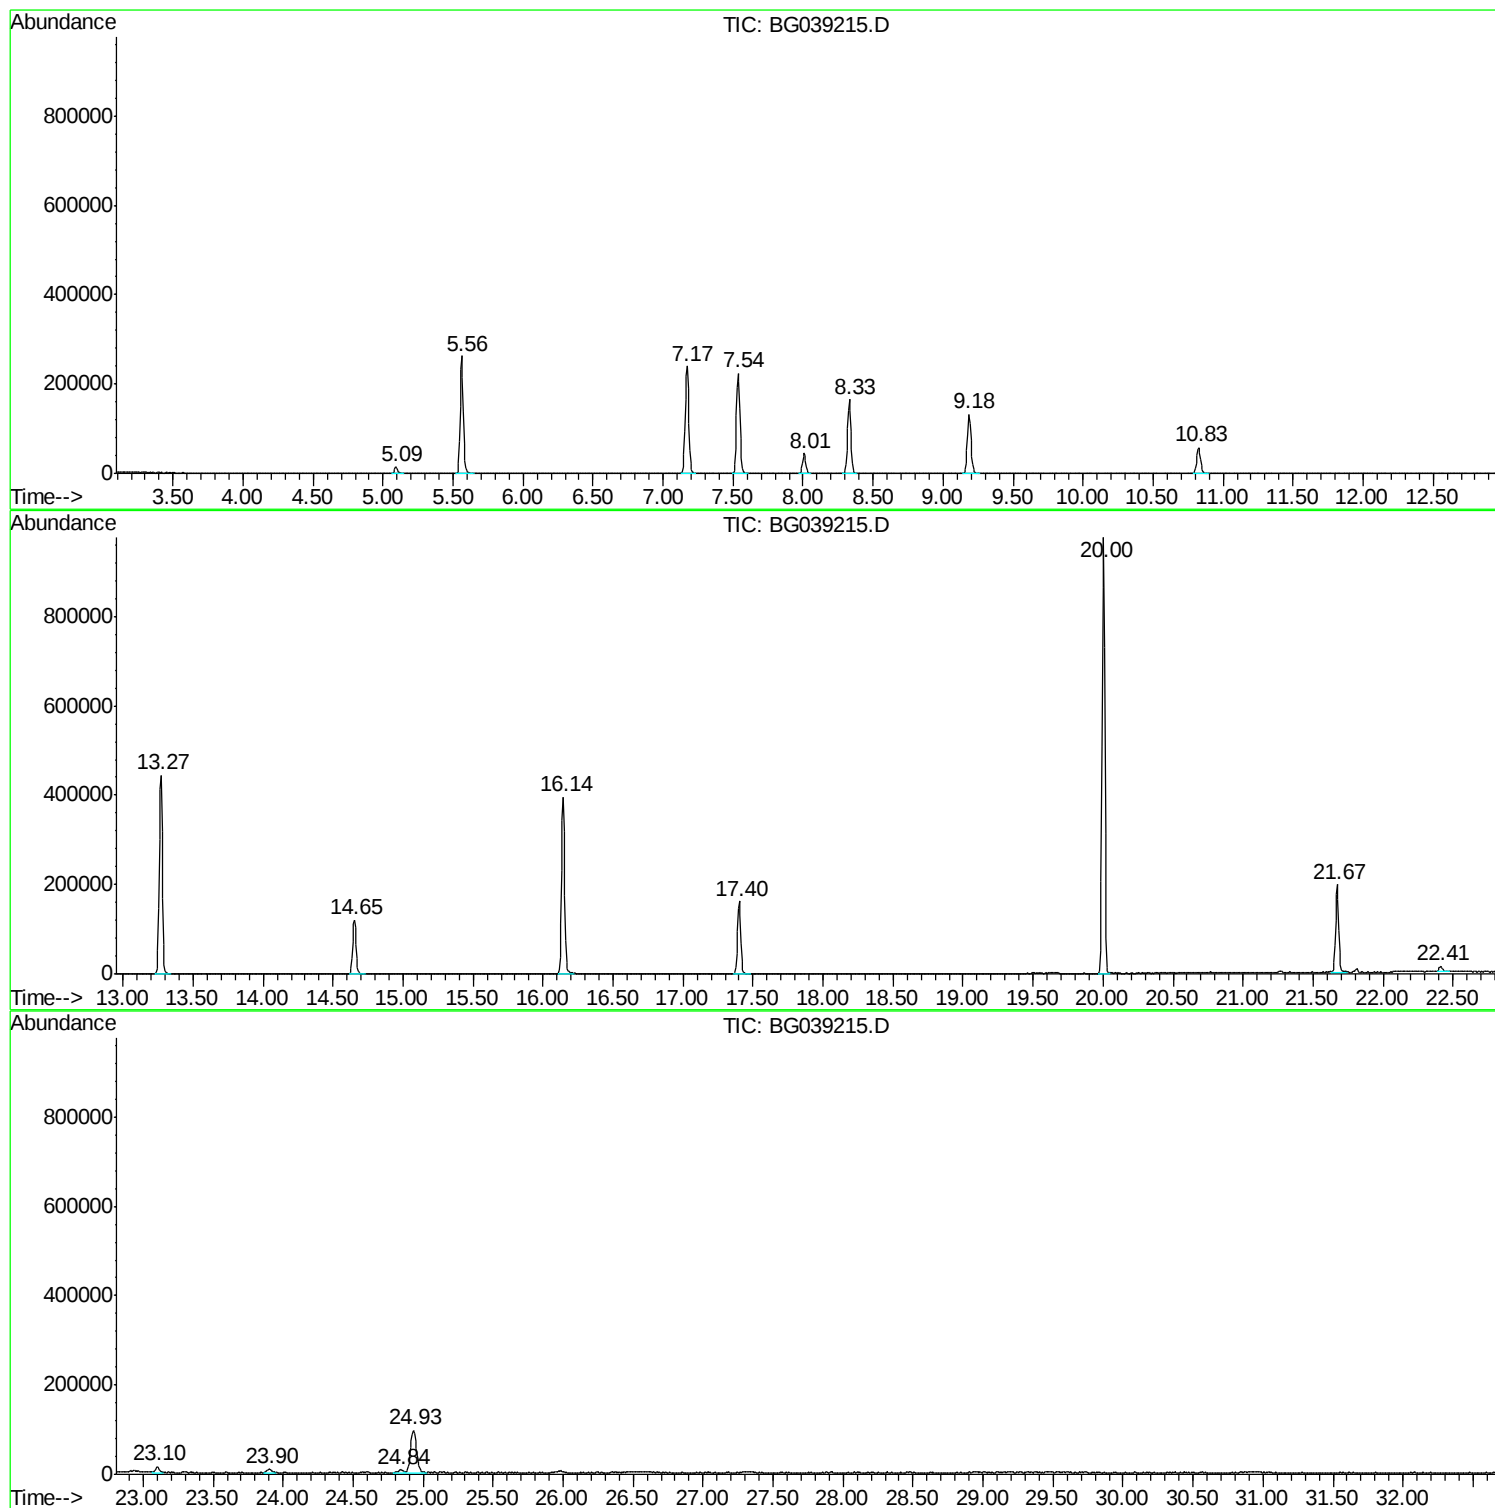

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
Data File : BG039215.D
Acq On : 18 Jan 2019 14:30
Operator : JU/SJ
Sample : PB116467BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116467BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.09	6.08 ng	22769	1,4-Dichlorobenzene-d4	8.01

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			5-Hexen-2-one	98	C6H10O	000109-49-9	9
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9
4			Diacetamide	101	C4H7NO2	000625-77-4	7
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7

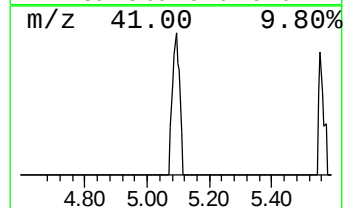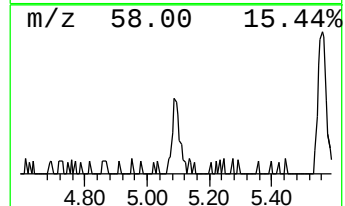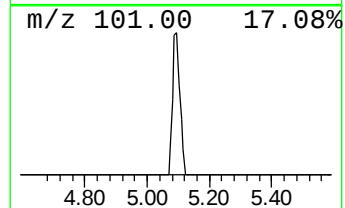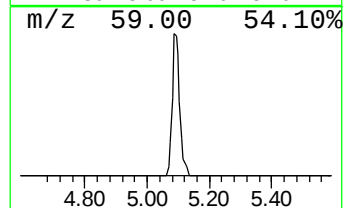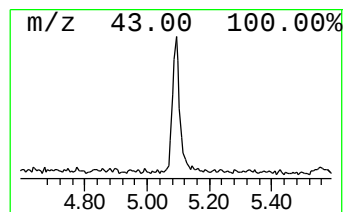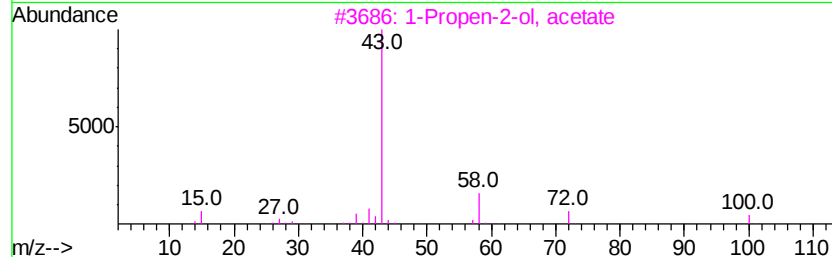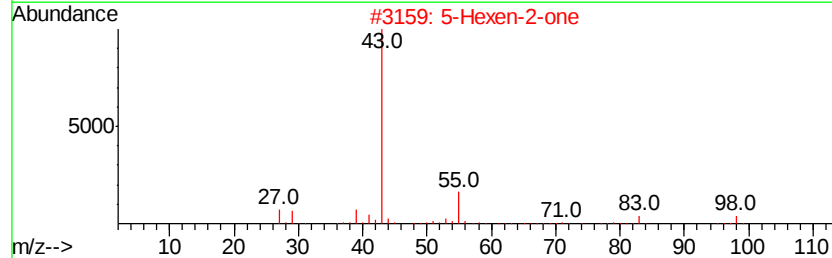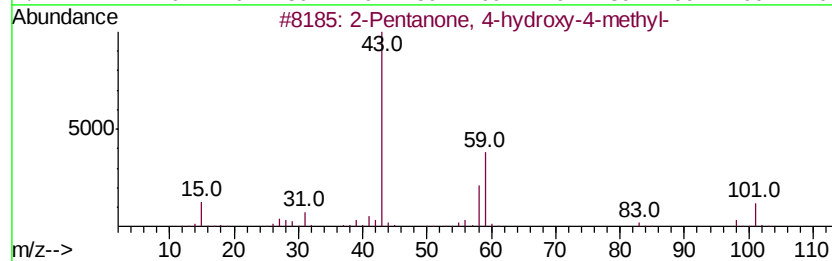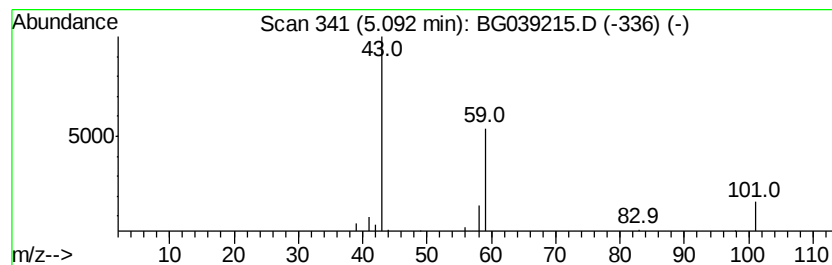

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011819\
Data File : BG039215.D
Acq On : 18 Jan 2019 14:30
Operator : JU/SJ
Sample : PB116467BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
PB116467BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	104.38 ng	390758	1,4-Dichlorobenzene-d4	8.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Aminoindole	132	C8H8N2	005192-03-0	27
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	23
5		N-(3,4-Methylenedioxyphenyl)isop...	267	C17H17NO2	1000378-96-6	12

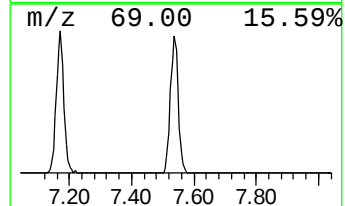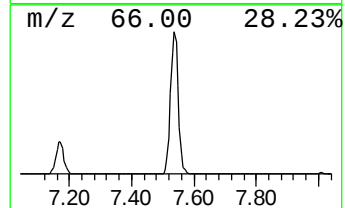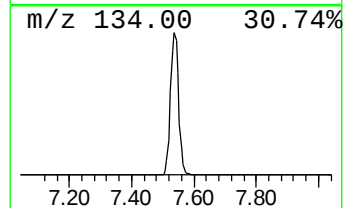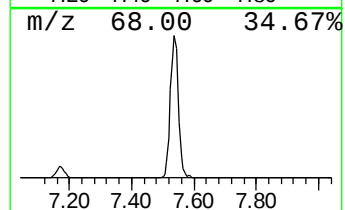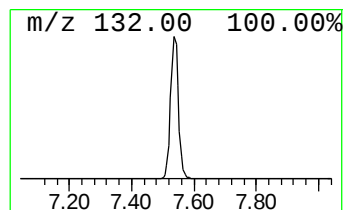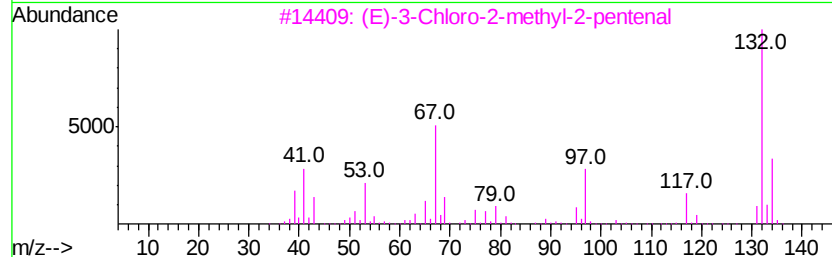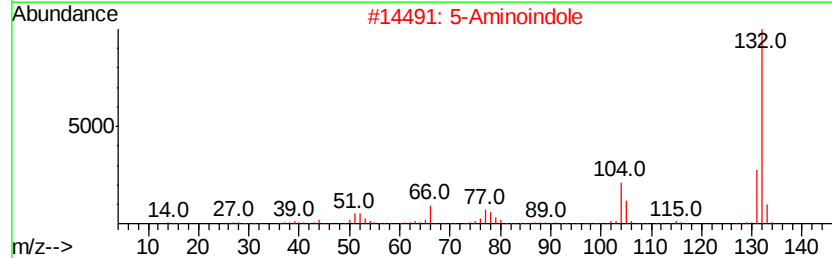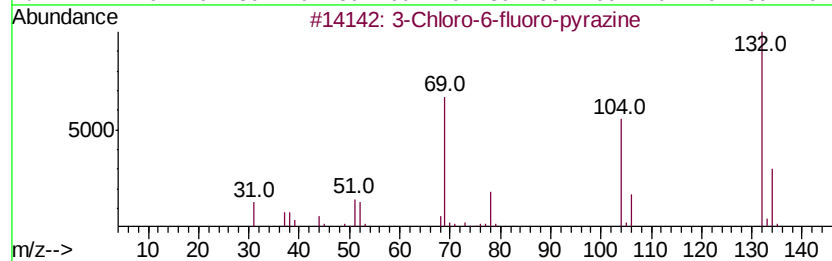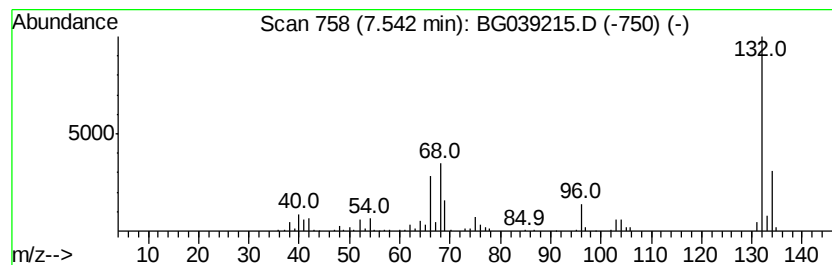

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG011819\
Data File : BG039215.D
Acq On : 18 Jan 2019 14:30
Operator : JU/SJ
Sample : PB116467BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116467BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.09	6.1	ng	22769	1	8.01	74871	20.0
unknown7.54	7.54	104.4	ng	390758	1	8.01	74871	20.0