


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011819\
 Data File : BG039212.D
 Acq On : 18 Jan 2019 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 04:20:14 2019

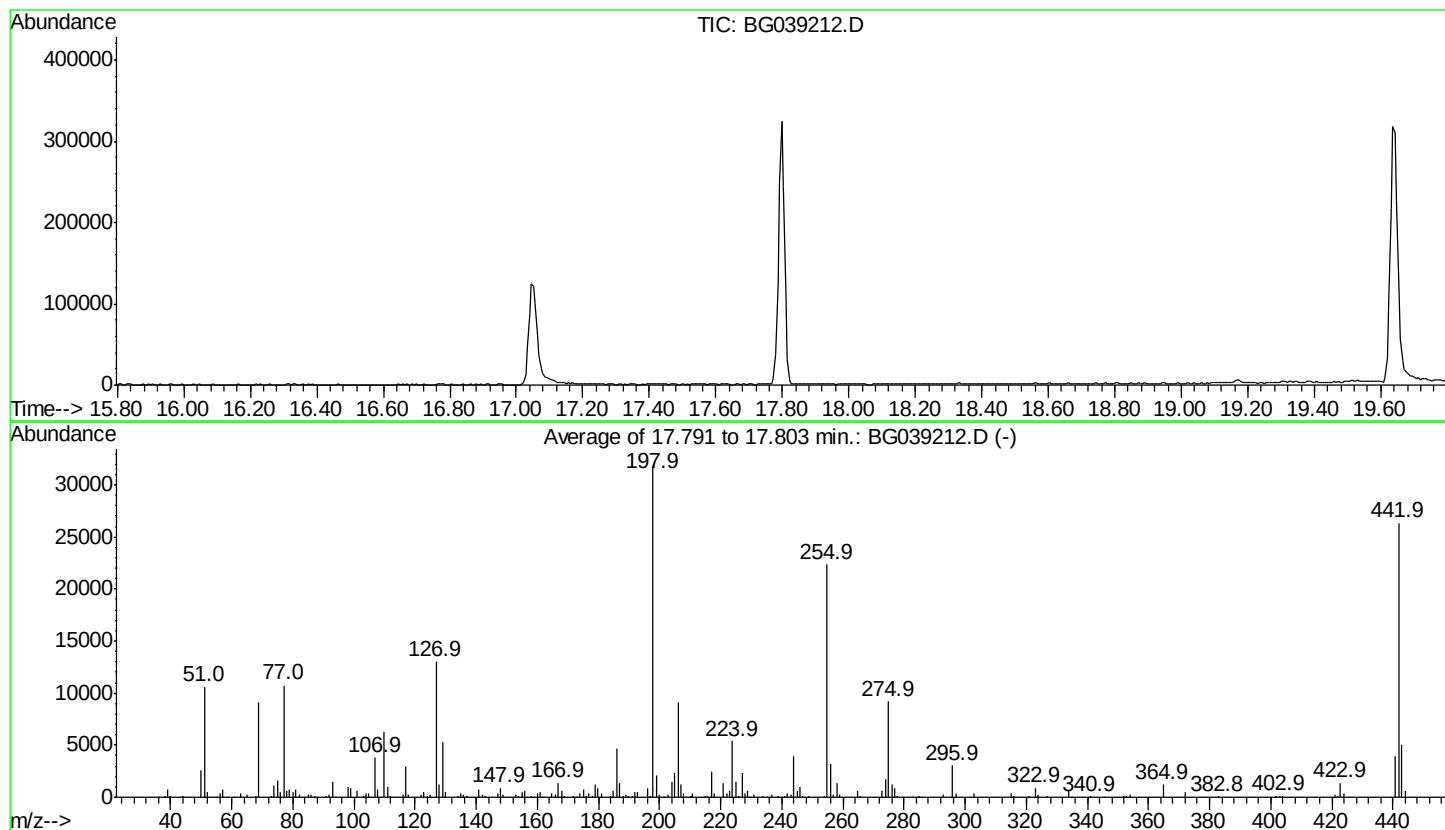

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	10577	PASS
68	69	0.00	2	1.4	124	PASS
69	198	0.00	100	28.6	9106	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	13026	PASS
197	198	0.00	2	0.3	101	PASS
198	198	100	100	100.0	31850	PASS
199	198	5	9	6.5	2086	PASS
275	198	10	60	28.9	9209	PASS
365	198	1	100	3.8	1216	PASS
441	198	0.01	100	12.2	3900	PASS
442	198	50	100	82.8	26357	PASS
443	442	15	24	19.3	5086	PASS