
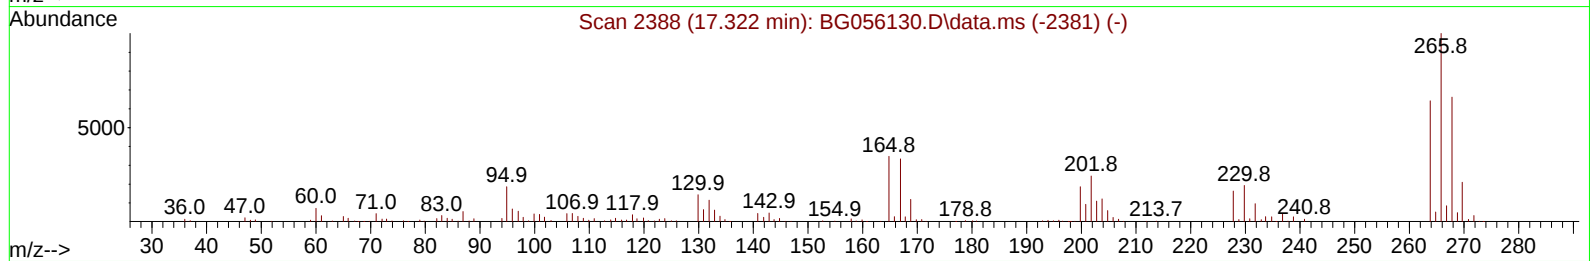
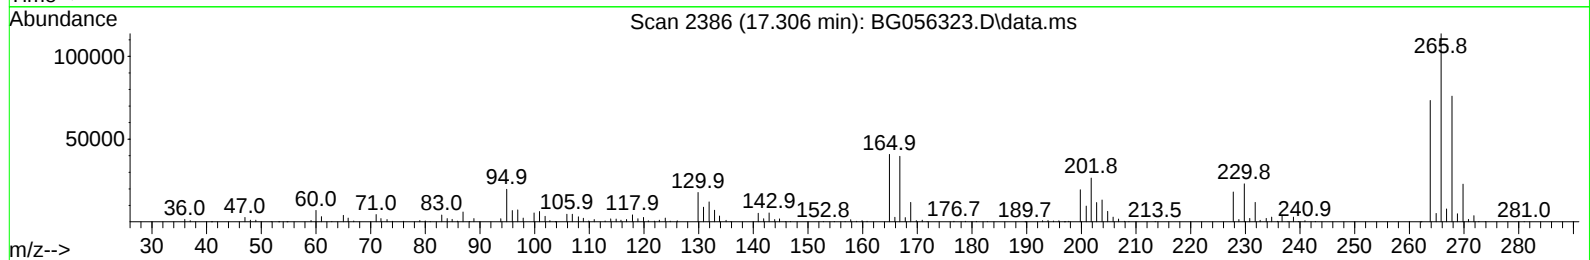


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056323.D
Acq On : 18 Jan 2023 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:49:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

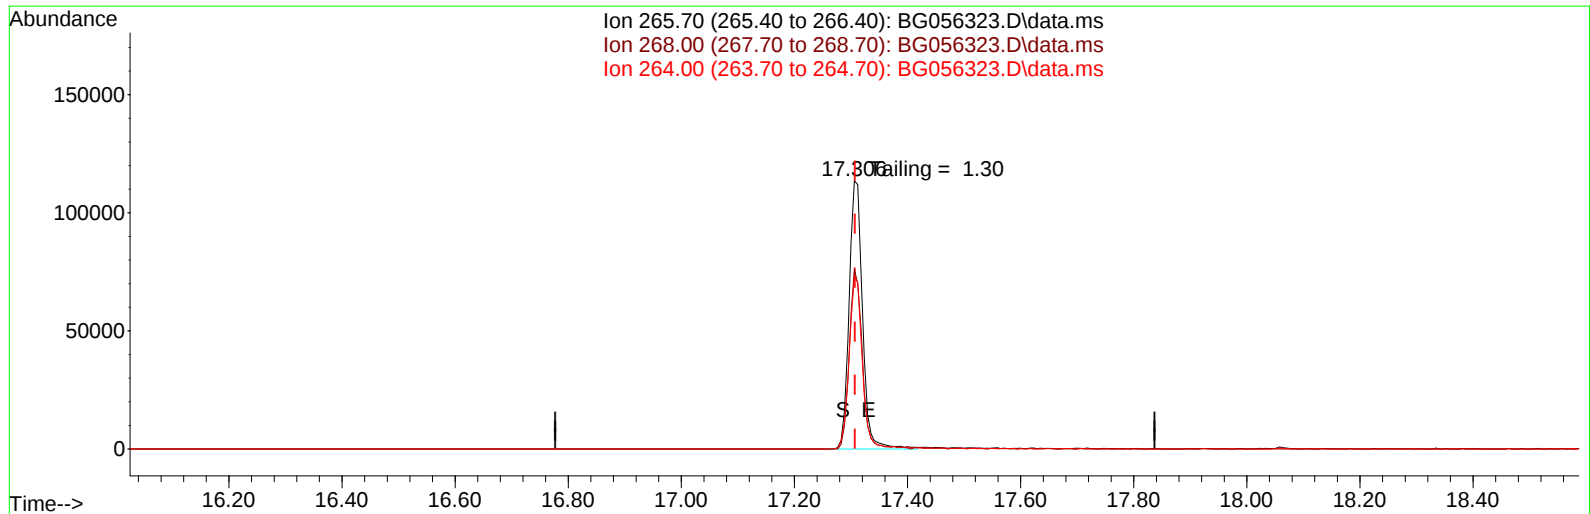

TIC: BG056323.D\data.ms

(70) Pentachlorophenol (C)




17.306min (-0.001) 381012.95 ng

response 187770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.90
264.00	64.30	64.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056323.D
Acq On : 18 Jan 2023 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:49:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

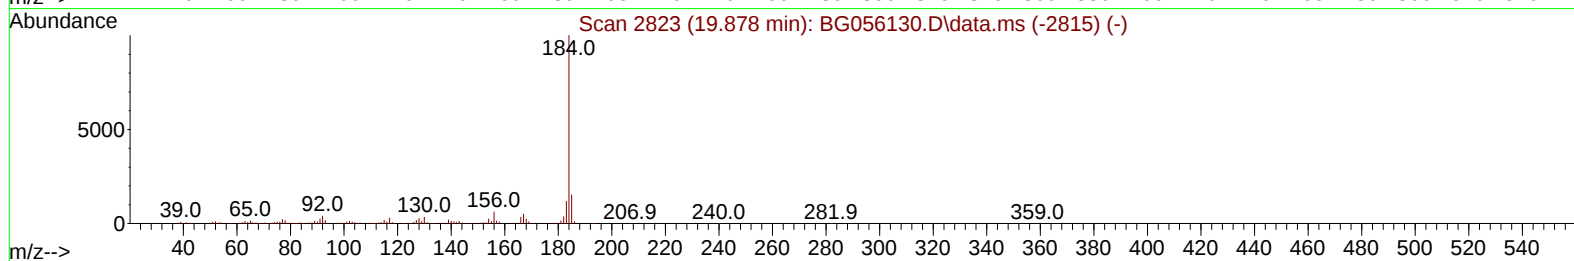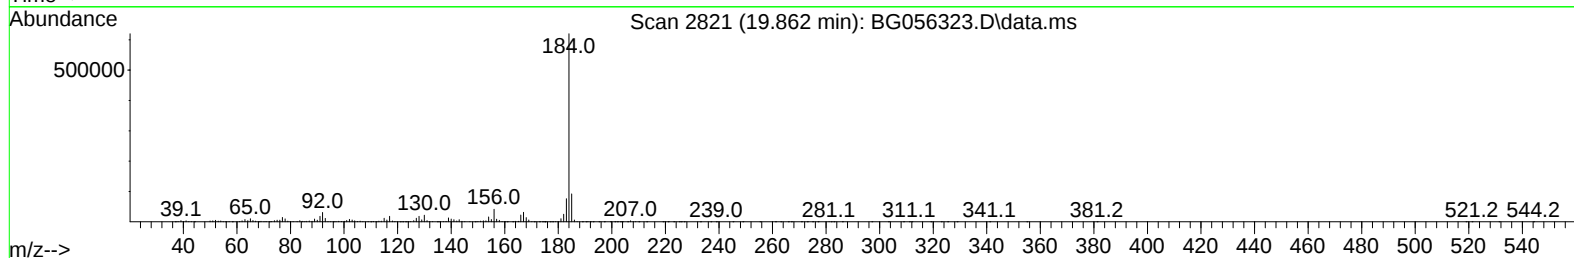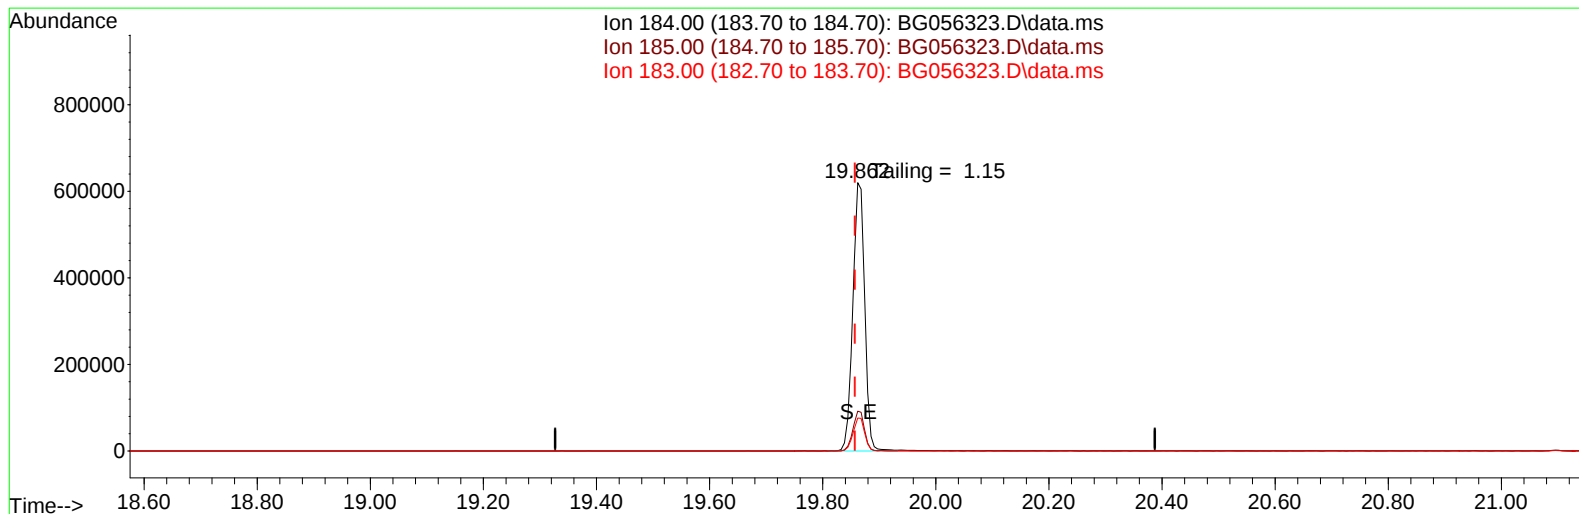

TIC: BG056323.D\data.ms

(77) Benzidine**19.862min (+ 0.005) 17250.87 ng****response 905608**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.85
183.00	11.70	12.31
0.00	0.00	0.00