

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
 Data File : BG056326.D
 Acq On : 18 Jan 2023 13:05
 Operator : CG/JU
 Sample : PB150306BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150306BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.345	342	350	359	rBB	147944	222761	5.46%	1.546%
2	5.827	425	432	441	rBV	629912	1019160	24.98%	7.071%
3	7.448	699	708	720	rBV	655882	1102410	27.02%	7.648%
4	8.306	848	854	861	rBB	120295	204145	5.00%	1.416%
5	9.481	1046	1054	1064	rBV	369704	661811	16.22%	4.592%
6	11.144	1329	1337	1344	rBV	159939	295568	7.24%	2.051%
7	13.547	1739	1746	1754	rBV	1474009	2312667	56.68%	16.045%
8	14.922	1973	1980	1989	rBB	346730	523833	12.84%	3.634%
9	16.402	2225	2232	2240	rBV	1143658	1729379	42.39%	11.998%
10	17.660	2439	2446	2453	rBV	484352	723750	17.74%	5.021%
11	20.233	2878	2884	2890	rBV	3083278	4079983	100.00%	28.307%
12	21.949	3170	3176	3187	rVB2	438446	765078	18.75%	5.308%
13	25.392	3753	3762	3773	rBV2	257679	772915	18.94%	5.362%




Sum of corrected areas: 14413460

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056326.D
Acq On : 18 Jan 2023 13:05
Operator : CG/JU
Sample : PB150306BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150306BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

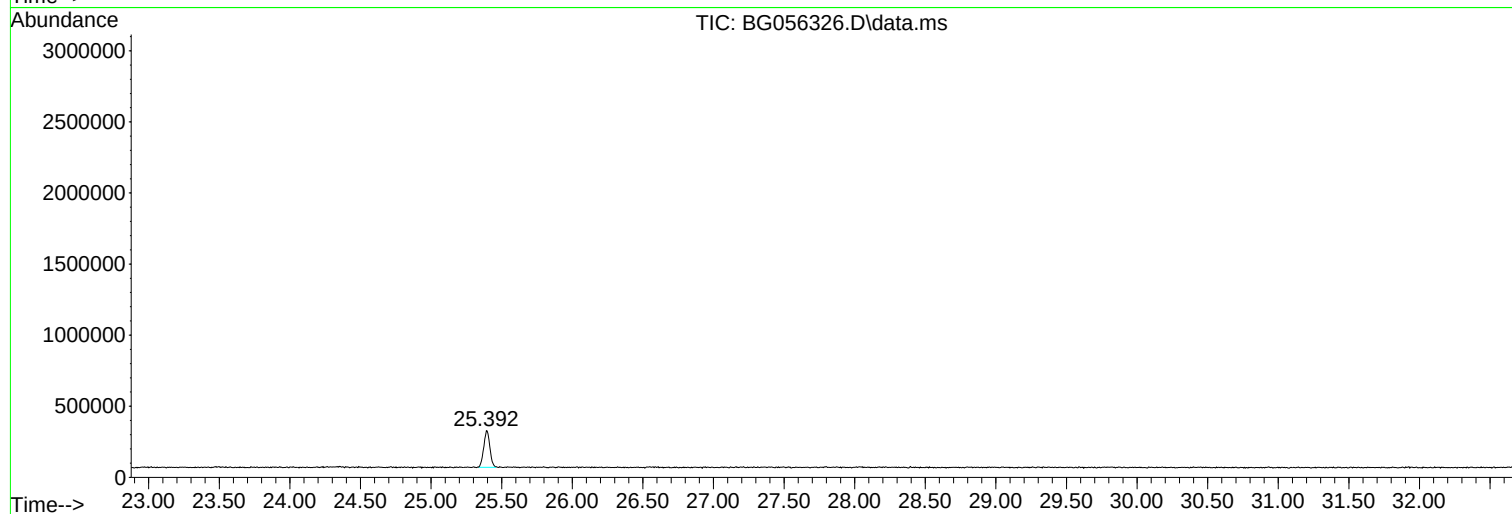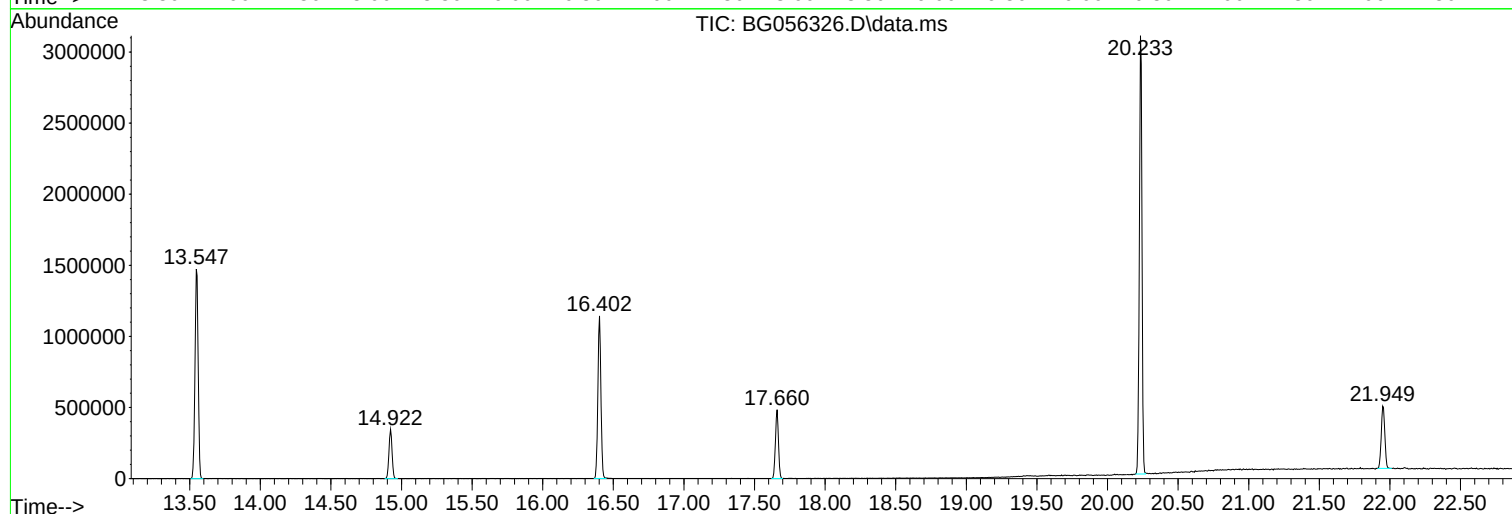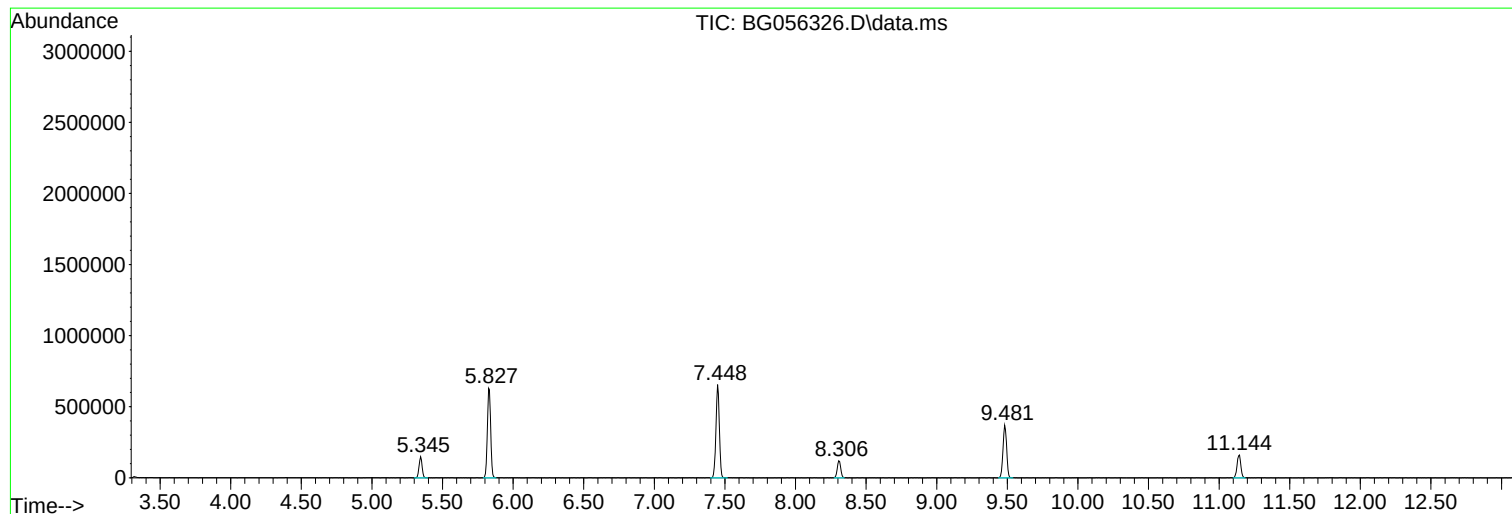

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056326.D
Acq On : 18 Jan 2023 13:05
Operator : CG/JU
Sample : PB150306BL
Misc :
ALS Vial : 4 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
PB150306BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
5.345	21.82 ng	222761	1,4-Dichlorobenzene-d4		8.306	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	50
2	4-Ethyl-3-octanol		158	C10H22O	019781-26-1	38
3	Propane, 1-ethoxy-2-methyl-		102	C6H14O	000627-02-1	35
4	Guanidine		59	CH5N3	000113-00-8	32
5	3-Hydroxy-3-methyl-2-butanone		102	C5H10O2	000115-22-0	25

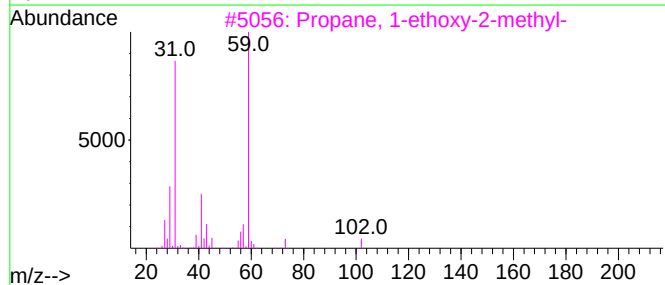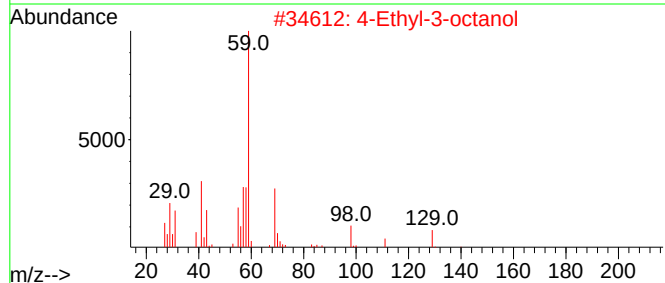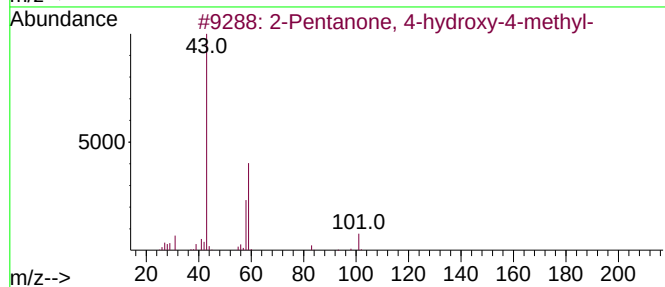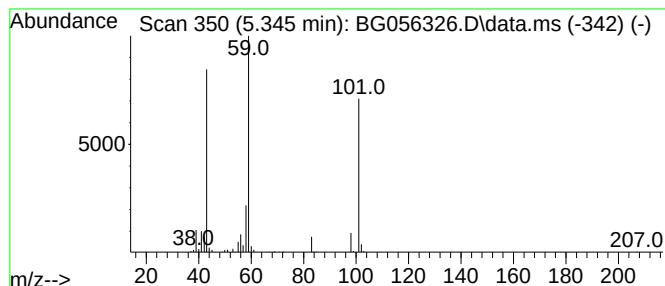

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056326.D
Acq On : 18 Jan 2023 13:05
Operator : CG/JU
Sample : PB150306BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150306BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.345	21.8	ng	222761	1	8.306	204145	20.0