


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056329.D
Acq On : 18 Jan 2023 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:31:30 2023

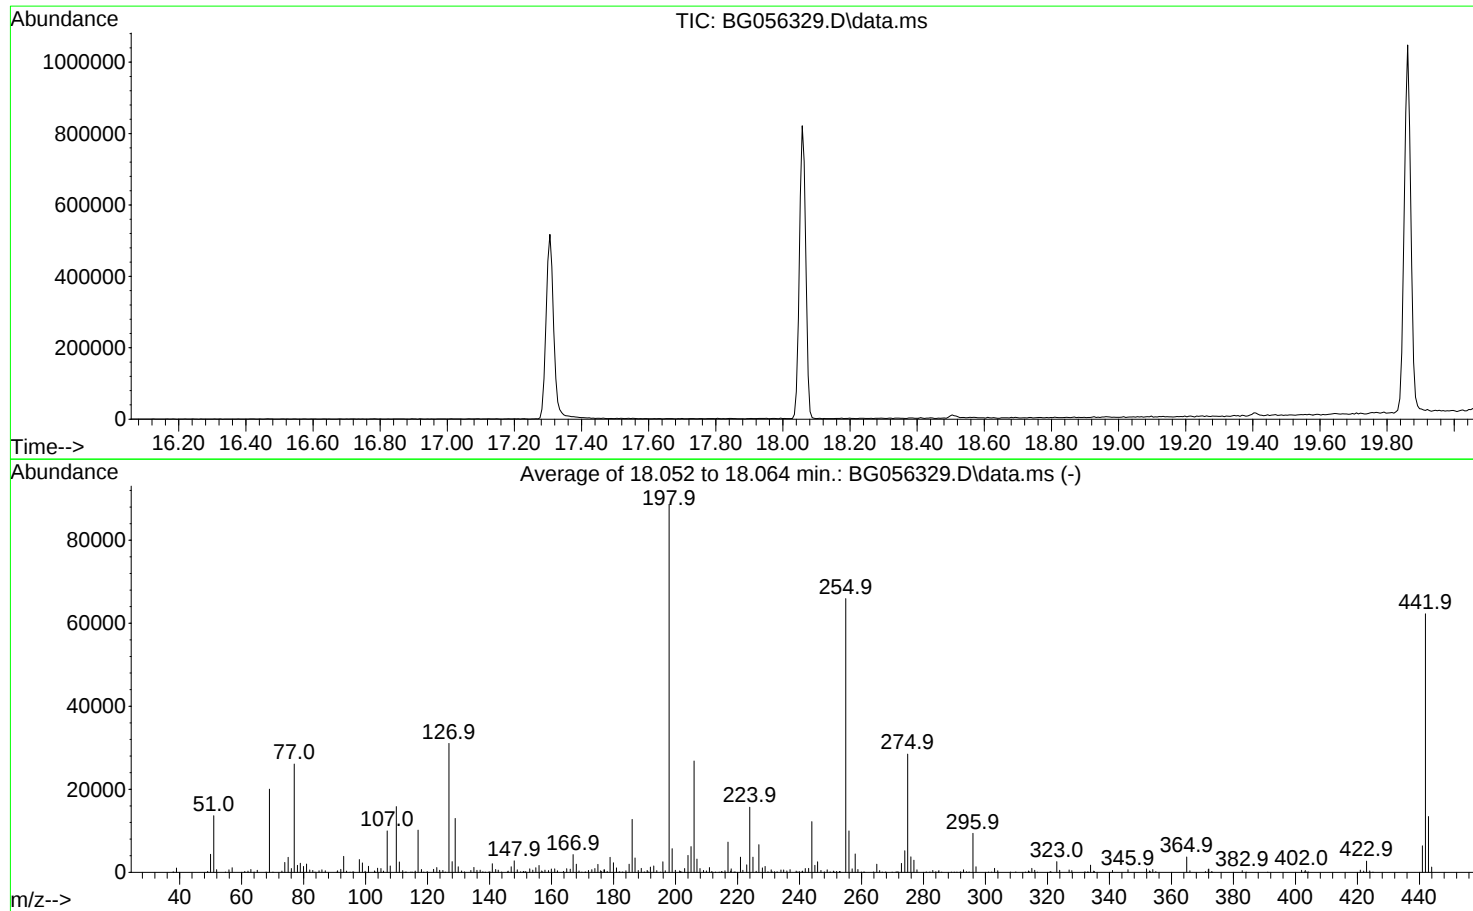




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.4	13612	PASS
68	69	0.00	2	0.3	70	PASS
69	198	0.00	100	22.6	20043	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	35.0	31061	PASS
197	198	0.00	2	0.4	355	PASS
198	198	100	100	100.0	88632	PASS
199	198	5	9	6.4	5693	PASS
275	198	10	60	32.1	28469	PASS
365	198	1	100	4.2	3693	PASS
441	198	0.01	100	7.2	6372	PASS
442	442	50	100	100.0	62301	PASS
443	442	15	24	21.6	13448	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
Data File : BG056329.D
Acq On : 18 Jan 2023 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 19 04:51:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

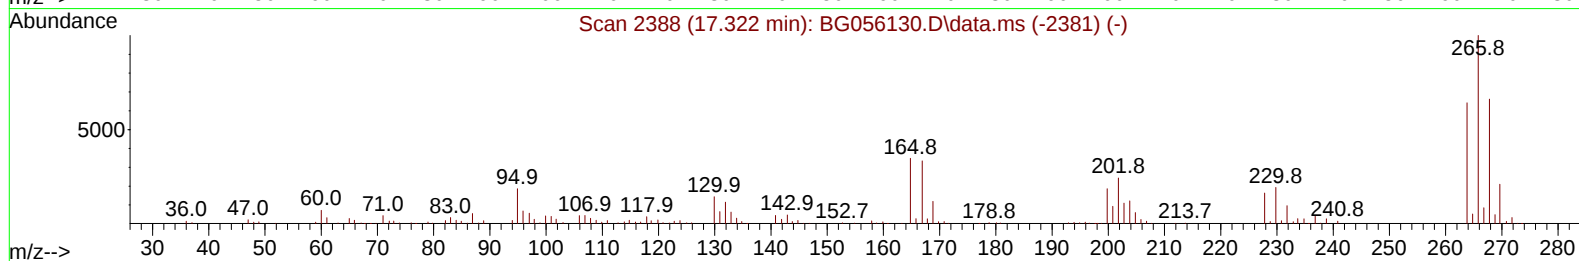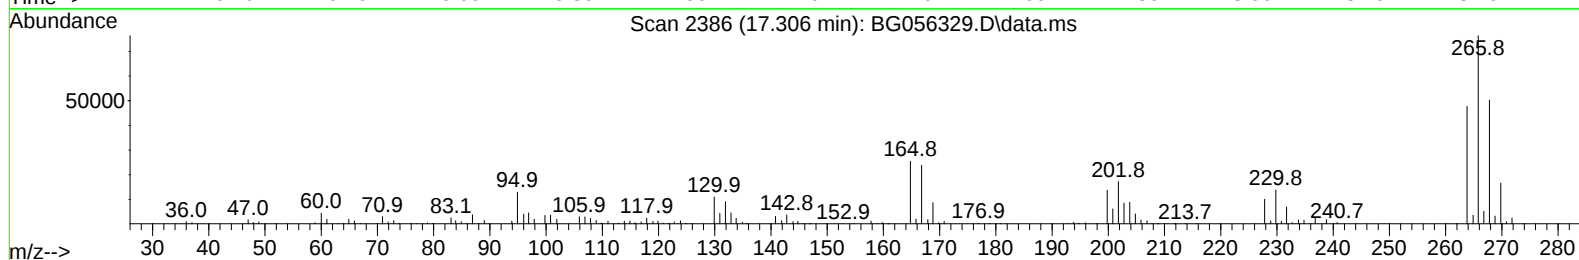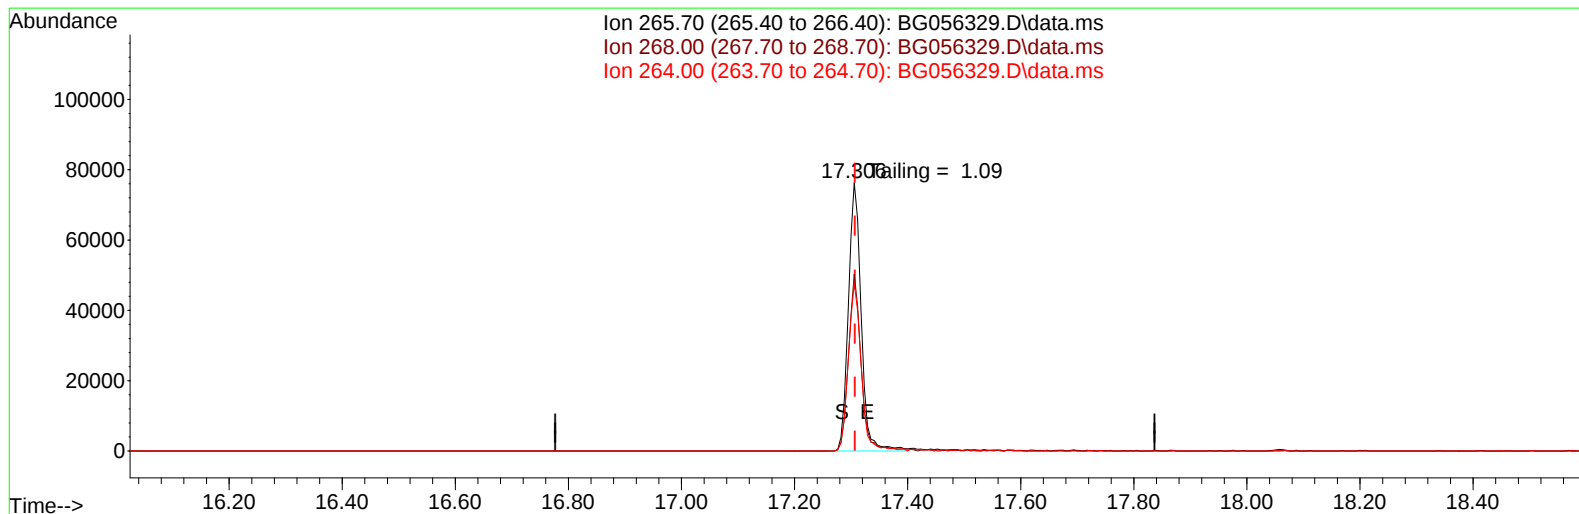

TIC: BG056329.D\data.ms

(70) Pentachlorophenol (C)

17.306min (-0.002) 23212.89 ng




response 120329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.85
264.00	64.30	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011823\
 Data File : BG056329.D
 Acq On : 18 Jan 2023 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 19 04:51:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 19 00:31:30 2023
 Response via : Initial Calibration

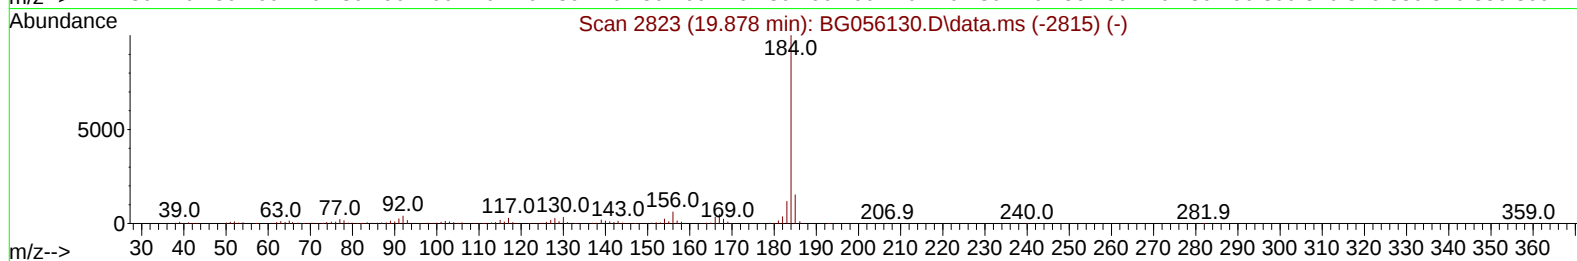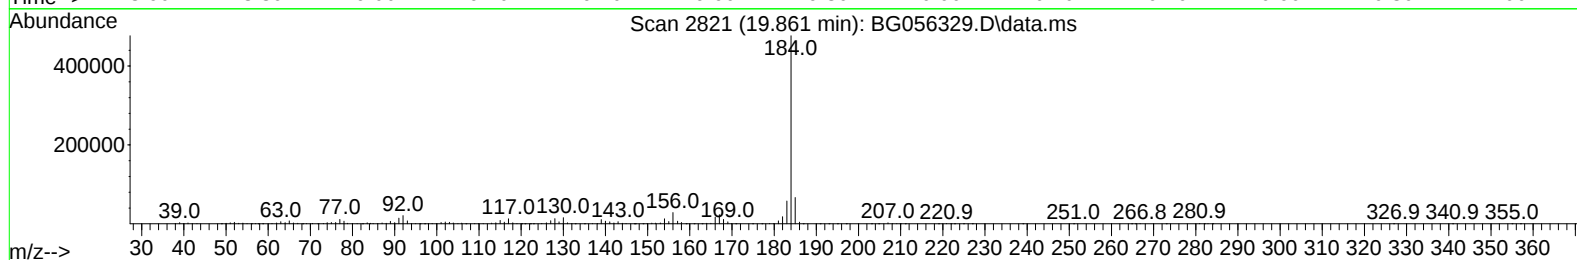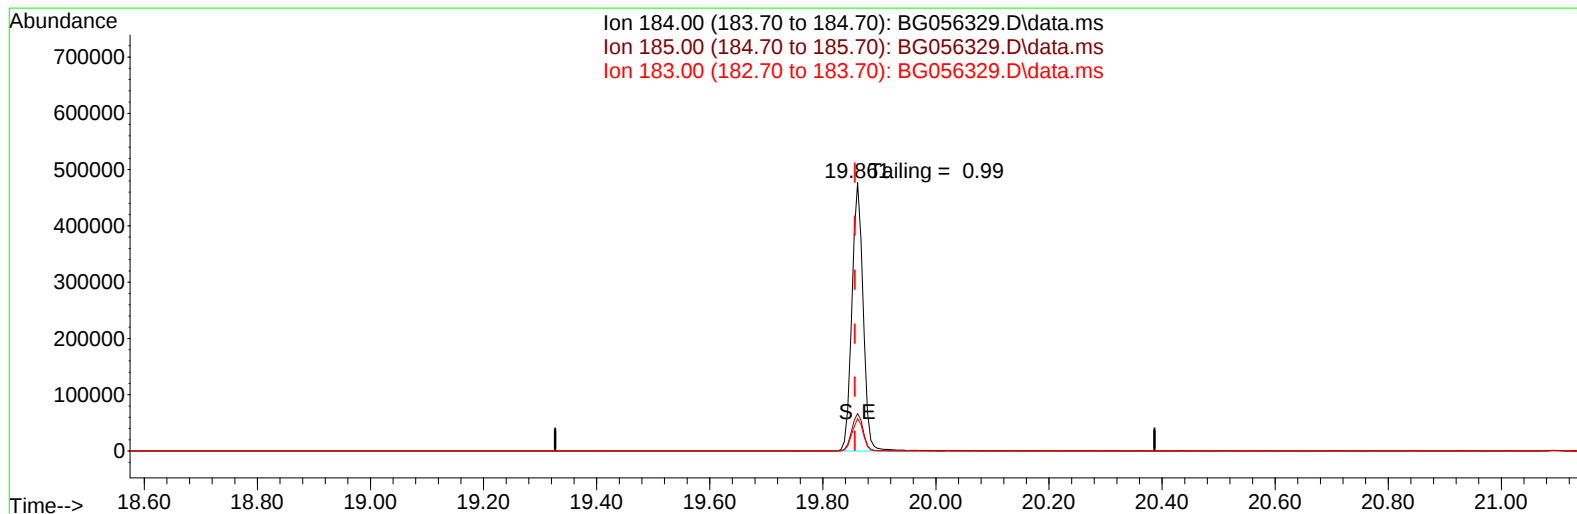

TIC: BG056329.D\data.ms

(77) Benzidine

19.861min (+ 0.004) 99824.65 ng

response 661176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.99
183.00	11.70	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2023	BNA_G	<u>BG056329.D</u>
Compound Name	Response	Retention Time
DDT	314454	21.095
DDD	9112	20.643
DDE	2314	20.143
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11426	325880	3.51

Instrument :
BNA_G
ClientSampleId :
DFTPP