




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052086.D
Acq On : 19 Jan 2022 23:35
Operator : CG/JU
Sample : N1179-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :Yogesh Patel 01/23/2022

Quant Time: Jan 20 02:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

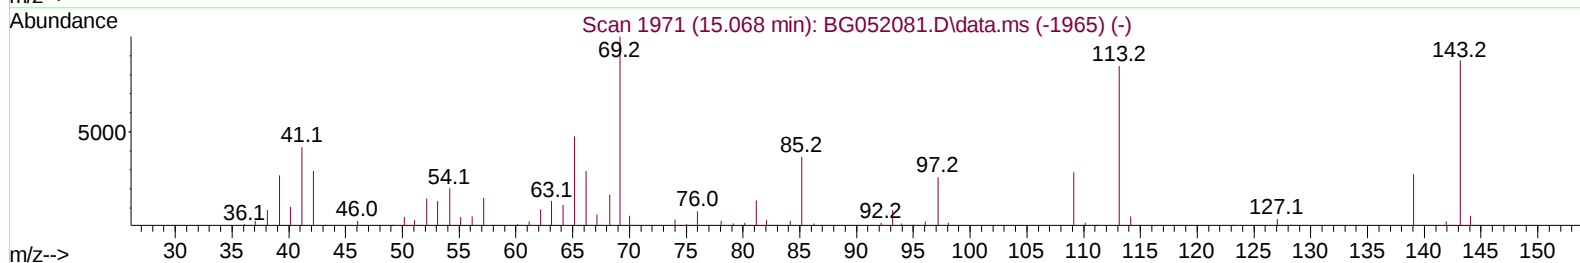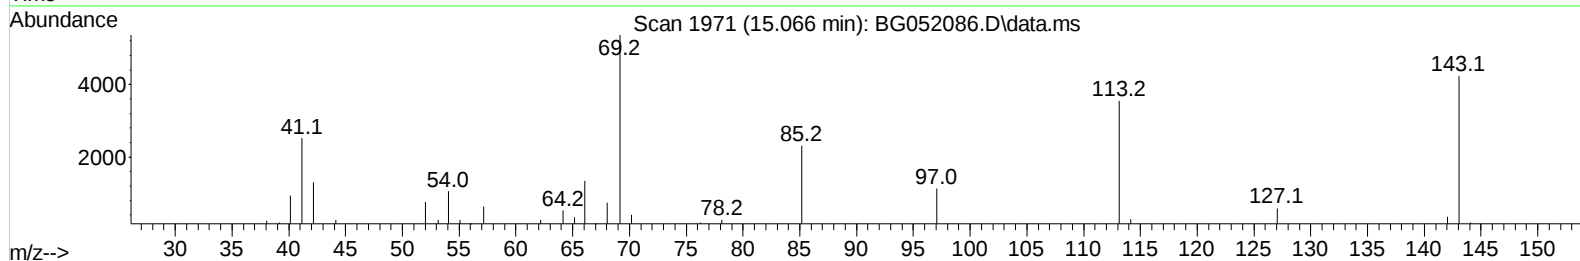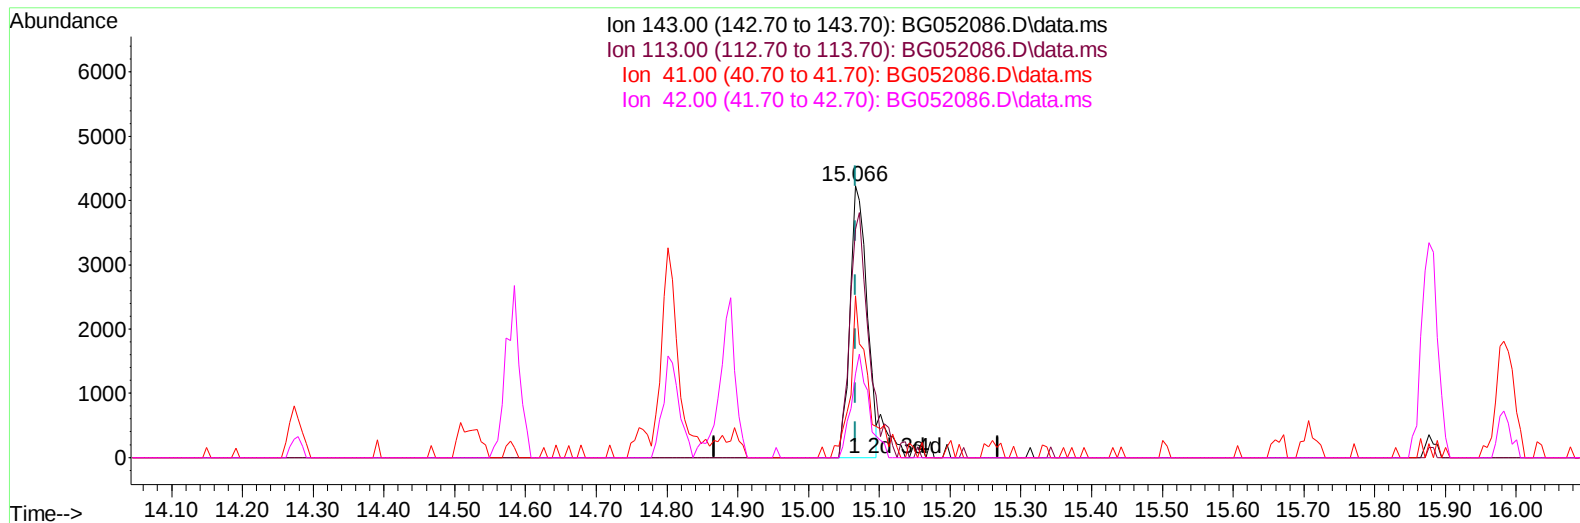

TIC: BG052086.D\data.ms

(54) 4-Nitrophenol-d4 (S)**15.066min (-0.001) 6.25 ng/u1****response 7024**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	84.10
41.00	44.40	59.47#
42.00	29.70	30.71




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052086.D
Acq On : 19 Jan 2022 23:35
Operator : CG/JU
Sample : N1179-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :Yogesh Patel 01/23/2022

Quant Time: Jan 20 02:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

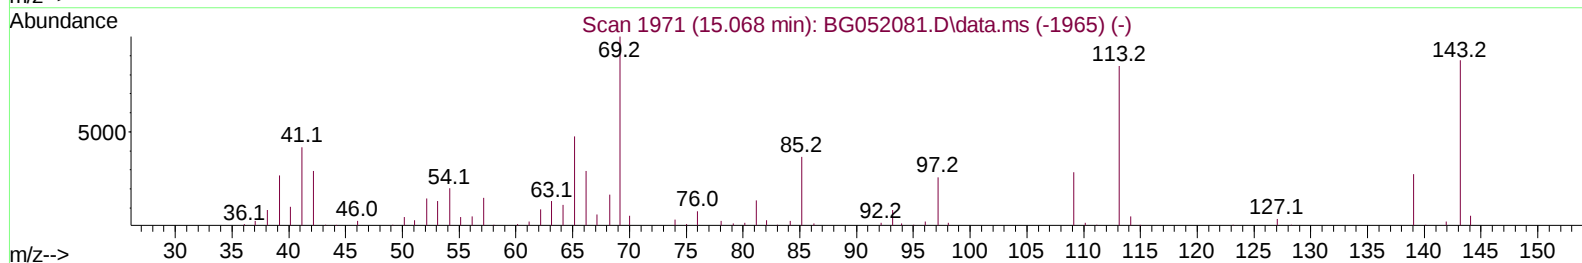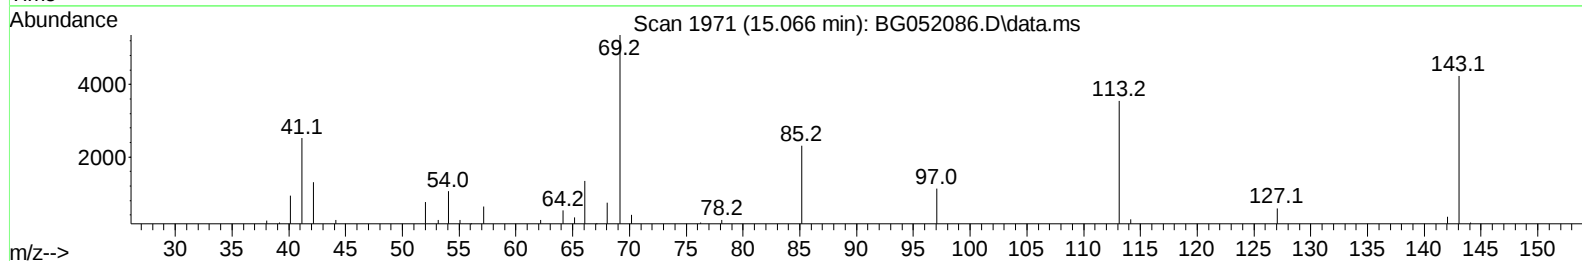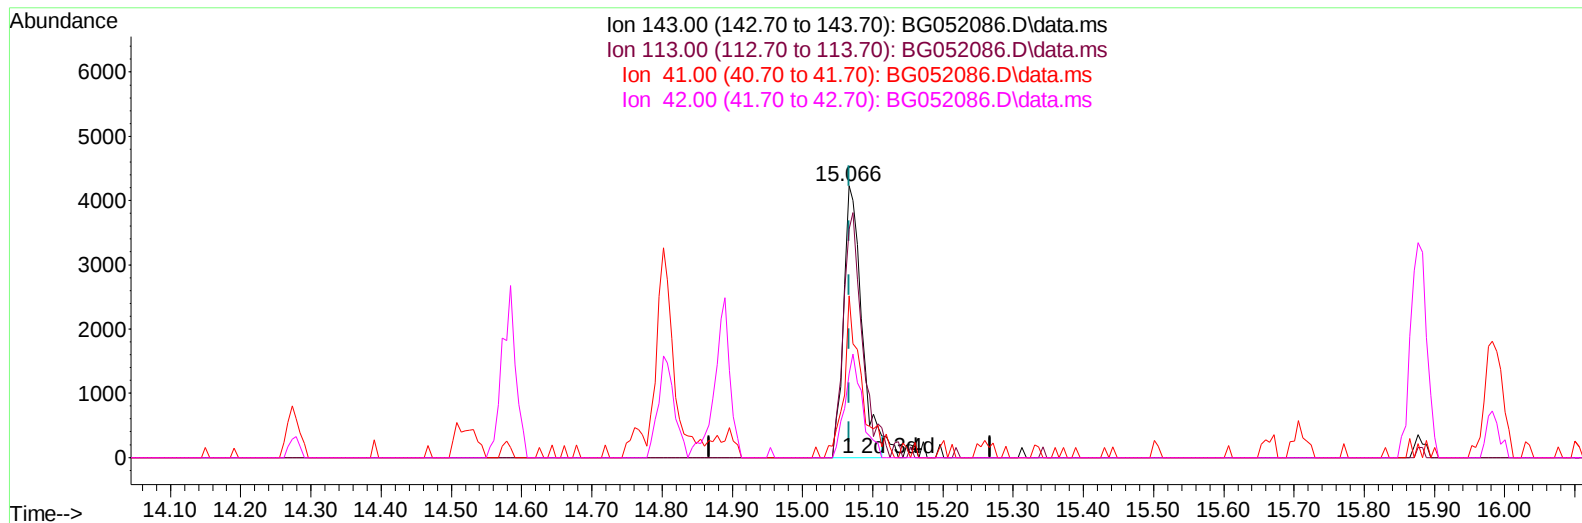

TIC: BG052086.D\data.ms

(54) 4-Nitrophenol-d4 (S)**15.066min (-0.001) 6.71 ng/ul m****response 7547**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	84.10
41.00	44.40	59.47#
42.00	29.70	30.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052086.D
 Acq On : 19 Jan 2022 23:35
 Operator : CG/JU
 Sample : N1179-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :Yogesh Patel 01/23/2022

Quant Time: Jan 20 02:03:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.246	152	27018	20.000	ng/ul	0.00
20) Naphthalene-d8	11.083	136	117212	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.890	164	81385	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.639	188	190187	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.957	240	185471	20.000	ng/ul	# 0.00
88) Perylene-d12	25.446	264	186834	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.570	96	3063	4.051	ng/uL	0.00
4) Pyridine-d5	4.010	84	8936	3.802	ng/ul	0.00
7) Phenol-d5	7.382	99	20439	7.729	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.547	67	49435	29.449	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.770	132	48582	27.749	ng/ul	0.00
15) 4-Methylphenol-d8	8.945	113	36516	17.764	ng/ul	0.00
21) Nitrobenzene-d5	9.415	128	32713	35.320	ng/ul	0.00
24) 2-Nitrophenol-d4	10.149	143	37569	36.677	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.696	165	64671	32.300	ng/ul	0.00
31) 4-Chloroaniline-d4	11.207	131	45526	16.327	ng/ul	0.00
46) Dimethylphthalate-d6	14.279	166	233721	34.743	ng/ul	0.00
49) Acenaphthylene-d8	14.584	160	289687	35.650	ng/ul	0.00
54) 4-Nitrophenol-d4	15.066	143	7547m	6.710	ng/ul	0.00
60) Fluorene-d10	15.877	176	207513	35.380	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.988	200	34512	28.765	ng/ul	0.00
73) Anthracene-d10	17.739	188	348741	38.654	ng/ul	0.00
81) Pyrene-d10	20.018	212	403103	37.764	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.205	264	374869	38.113	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052086.D
Acq On : 19 Jan 2022 23:35
Operator : CG/JU
Sample : N1179-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :Yogesh Patel 01/23/2022

Quant Time: Jan 20 02:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

