

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052069.D
 Acq On : 19 Jan 2022 11:37
 Operator : CG/JU
 Sample : N1100-14MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS6MEDL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :Yogesh Patel 01/23/2022

Quant Time: Jan 19 23:59:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.244	152	27160	20.000	ng/u1	0.00
20) Naphthalene-d8	11.081	136	123743	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.888	164	93543	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.637	188	200119	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.960	240	186068	20.000	ng/u1	# 0.00
88) Perylene-d12	25.444	264	193949	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.392	99	4047	1.522	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.551	67	2919	1.730	ng/u1	0.00
11) 2-Chlorophenol-d4	7.774	132	2860	1.625	ng/u1	0.00
15) 4-Methylphenol-d8	8.943	113	3596	1.740	ng/u1	0.00
21) Nitrobenzene-d5	9.419	128	1441m	1.474	ng/u1	0.00
24) 2-Nitrophenol-d4	10.153	143	1732	1.602	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.693	165	3789	1.793	ng/u1	0.00
31) 4-Chloroaniline-d4	11.204	131	5279	1.793	ng/u1	0.00
46) Dimethylphthalate-d6	14.277	166	12740	1.648	ng/u1	0.00
49) Acenaphthylene-d8	14.582	160	17443	1.868	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.875	176	12540	1.860	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.737	188	20869	2.198	ng/u1	0.00
81) Pyrene-d10	20.016	212	23356	2.181	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.197	264	21370	2.093	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.819	149	202162	32.601	ng/u1#	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052069.D
Acq On : 19 Jan 2022 11:37
Operator : CG/JU
Sample : N1100-14MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BGLS6MEDL

Quant Time: Jan 19 23:59:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :Yogesh Patel 01/23/2022

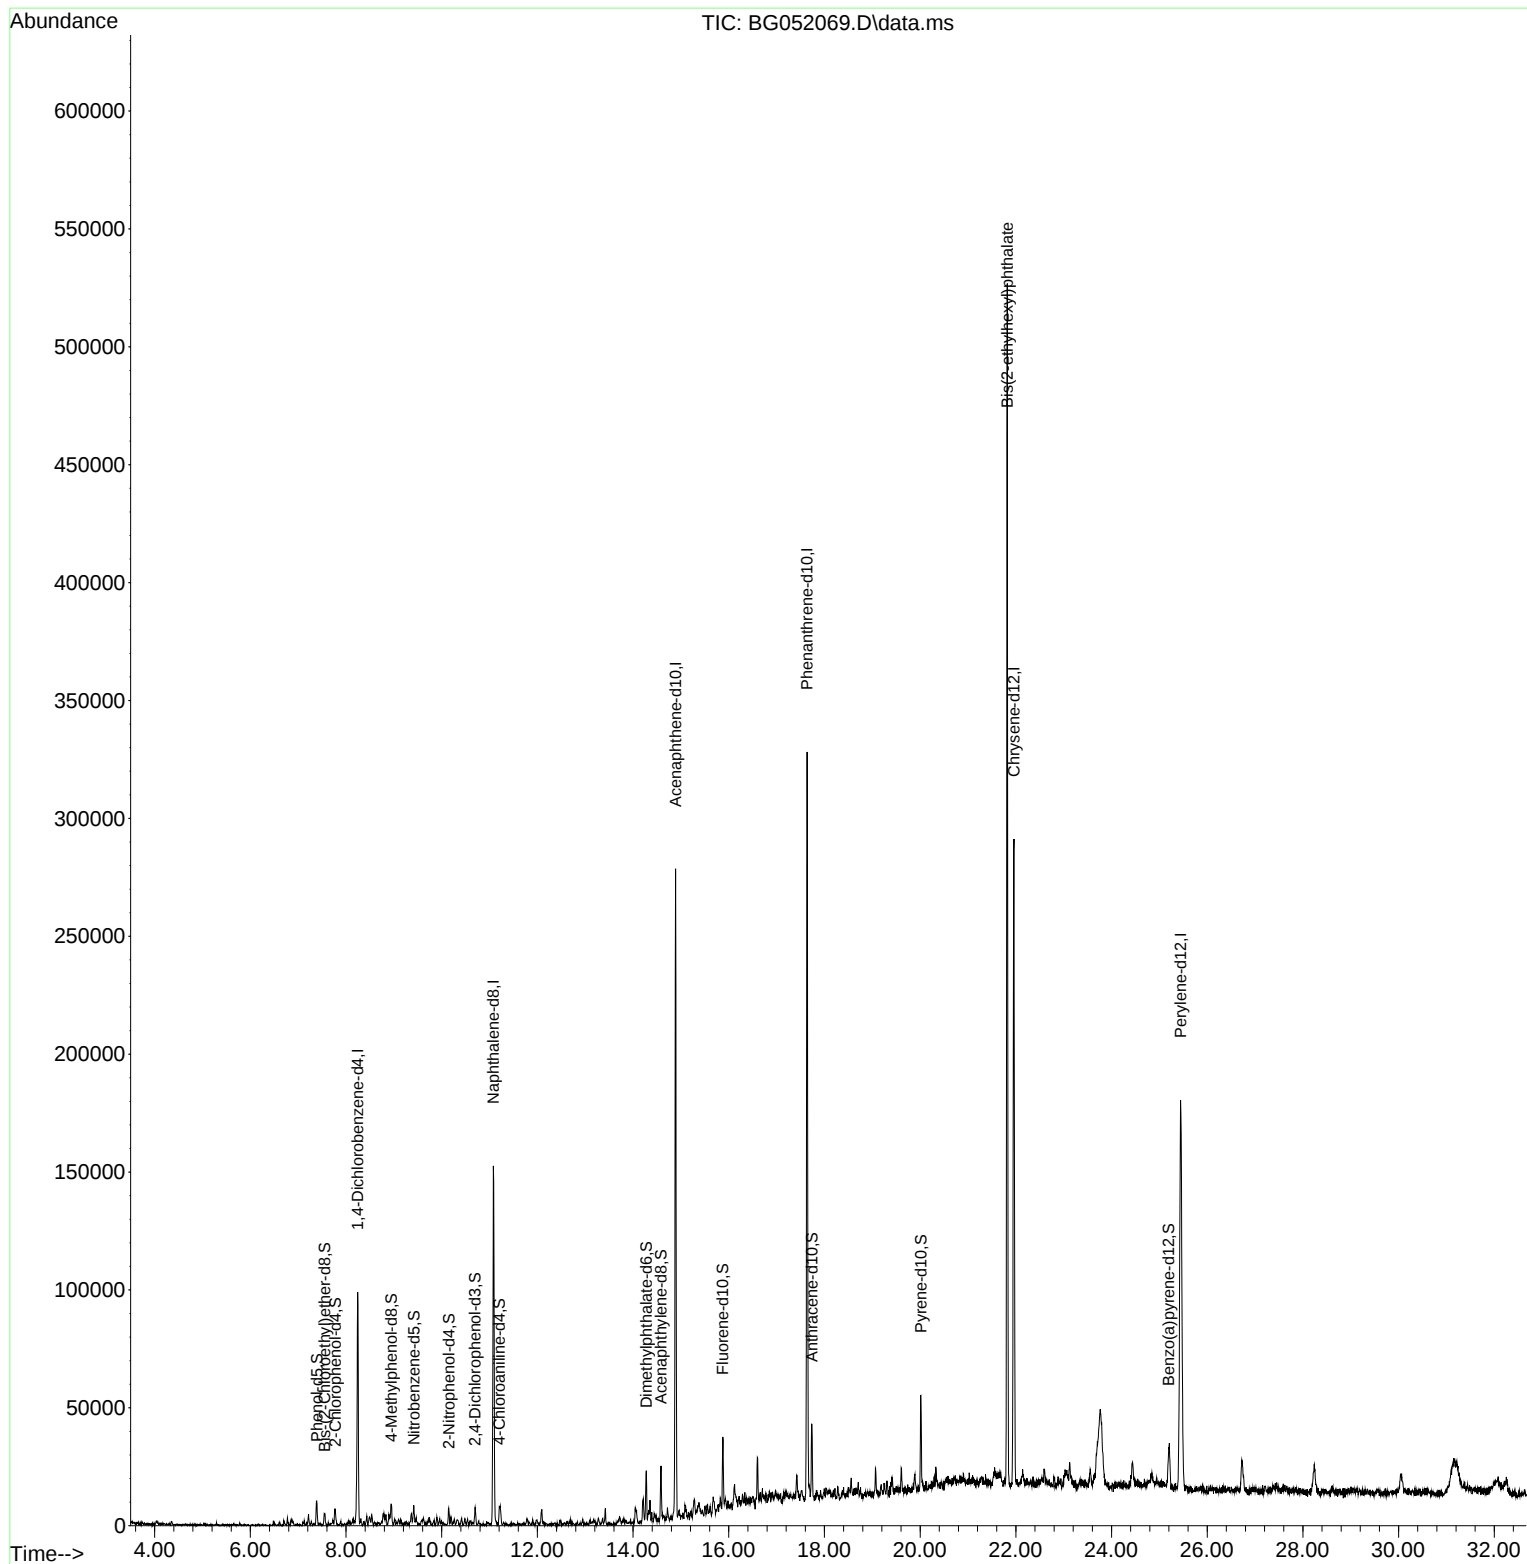

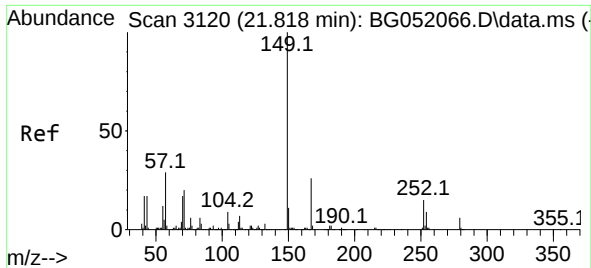

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 32.601 ng/ul
 RT: 21.819 min Scan# 3120
 Delta R.T. 0.003 min
 Lab File: BG052069.D
 Acq: 19 Jan 2022 11:37

Instrument :
 BNA_G
 ClientSampleId :
 BGLS6MEDL

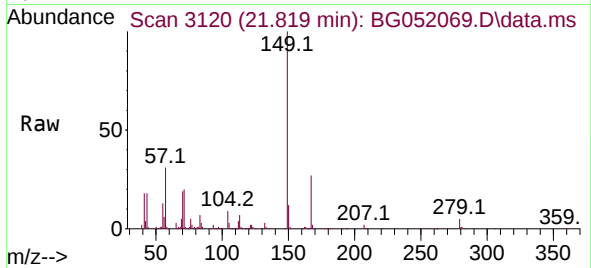

Tgt Ion:149 Resp: 202162
 Ion Ratio Lower Upper
 149 100
 167 27.5 21.1 31.7
 279 4.8 2.7 4.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :Yogesh Patel 01/23/2022

