

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052089.D
 Acq On : 20 Jan 2022 1:28
 Operator : CG/JU
 Sample : N1169-01ME
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7ME

Quant Time: Jan 20 02:04:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.245	152	29744	20.000	ng/ul	0.00
20) Naphthalene-d8	11.083	136	125663	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.889	164	90012	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.638	188	185290	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.956	240	182331	20.000	ng/ul	# 0.00
88) Perylene-d12	25.445	264	201402	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.569	96	2482	2.982	ng/uL	0.00
4) Pyridine-d5	4.004	84	10628	4.107	ng/ul	0.00
7) Phenol-d5	7.382	99	46494	15.971	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.546	67	28481	15.412	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.769	132	34712	18.010	ng/ul	0.00
15) 4-Methylphenol-d8	8.944	113	37341	16.501	ng/ul	0.00
21) Nitrobenzene-d5	9.414	128	18359	18.489	ng/ul	0.00
24) 2-Nitrophenol-d4	10.149	143	20491	18.659	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.695	165	38624	17.994	ng/ul	0.00
31) 4-Chloroaniline-d4	11.206	131	48446	16.206	ng/ul	0.00
46) Dimethylphthalate-d6	14.278	166	131653	17.695	ng/ul	0.00
49) Acenaphthylene-d8	14.584	160	169885	18.903	ng/ul	0.00
54) 4-Nitrophenol-d4	15.065	143	14421	11.593	ng/ul	0.00
60) Fluorene-d10	15.876	176	117469	18.109	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.982	200	12839	10.984	ng/ul	0.00
73) Anthracene-d10	17.738	188	182525	20.766	ng/ul	0.00
81) Pyrene-d10	20.018	212	210730	20.082	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.205	264	217610	20.524	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.821	149	700034	115.202	ng/ul#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052089.D
Acq On : 20 Jan 2022 1:28
Operator : CG/JU
Sample : N1169-01ME
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7ME

Quant Time: Jan 20 02:04:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

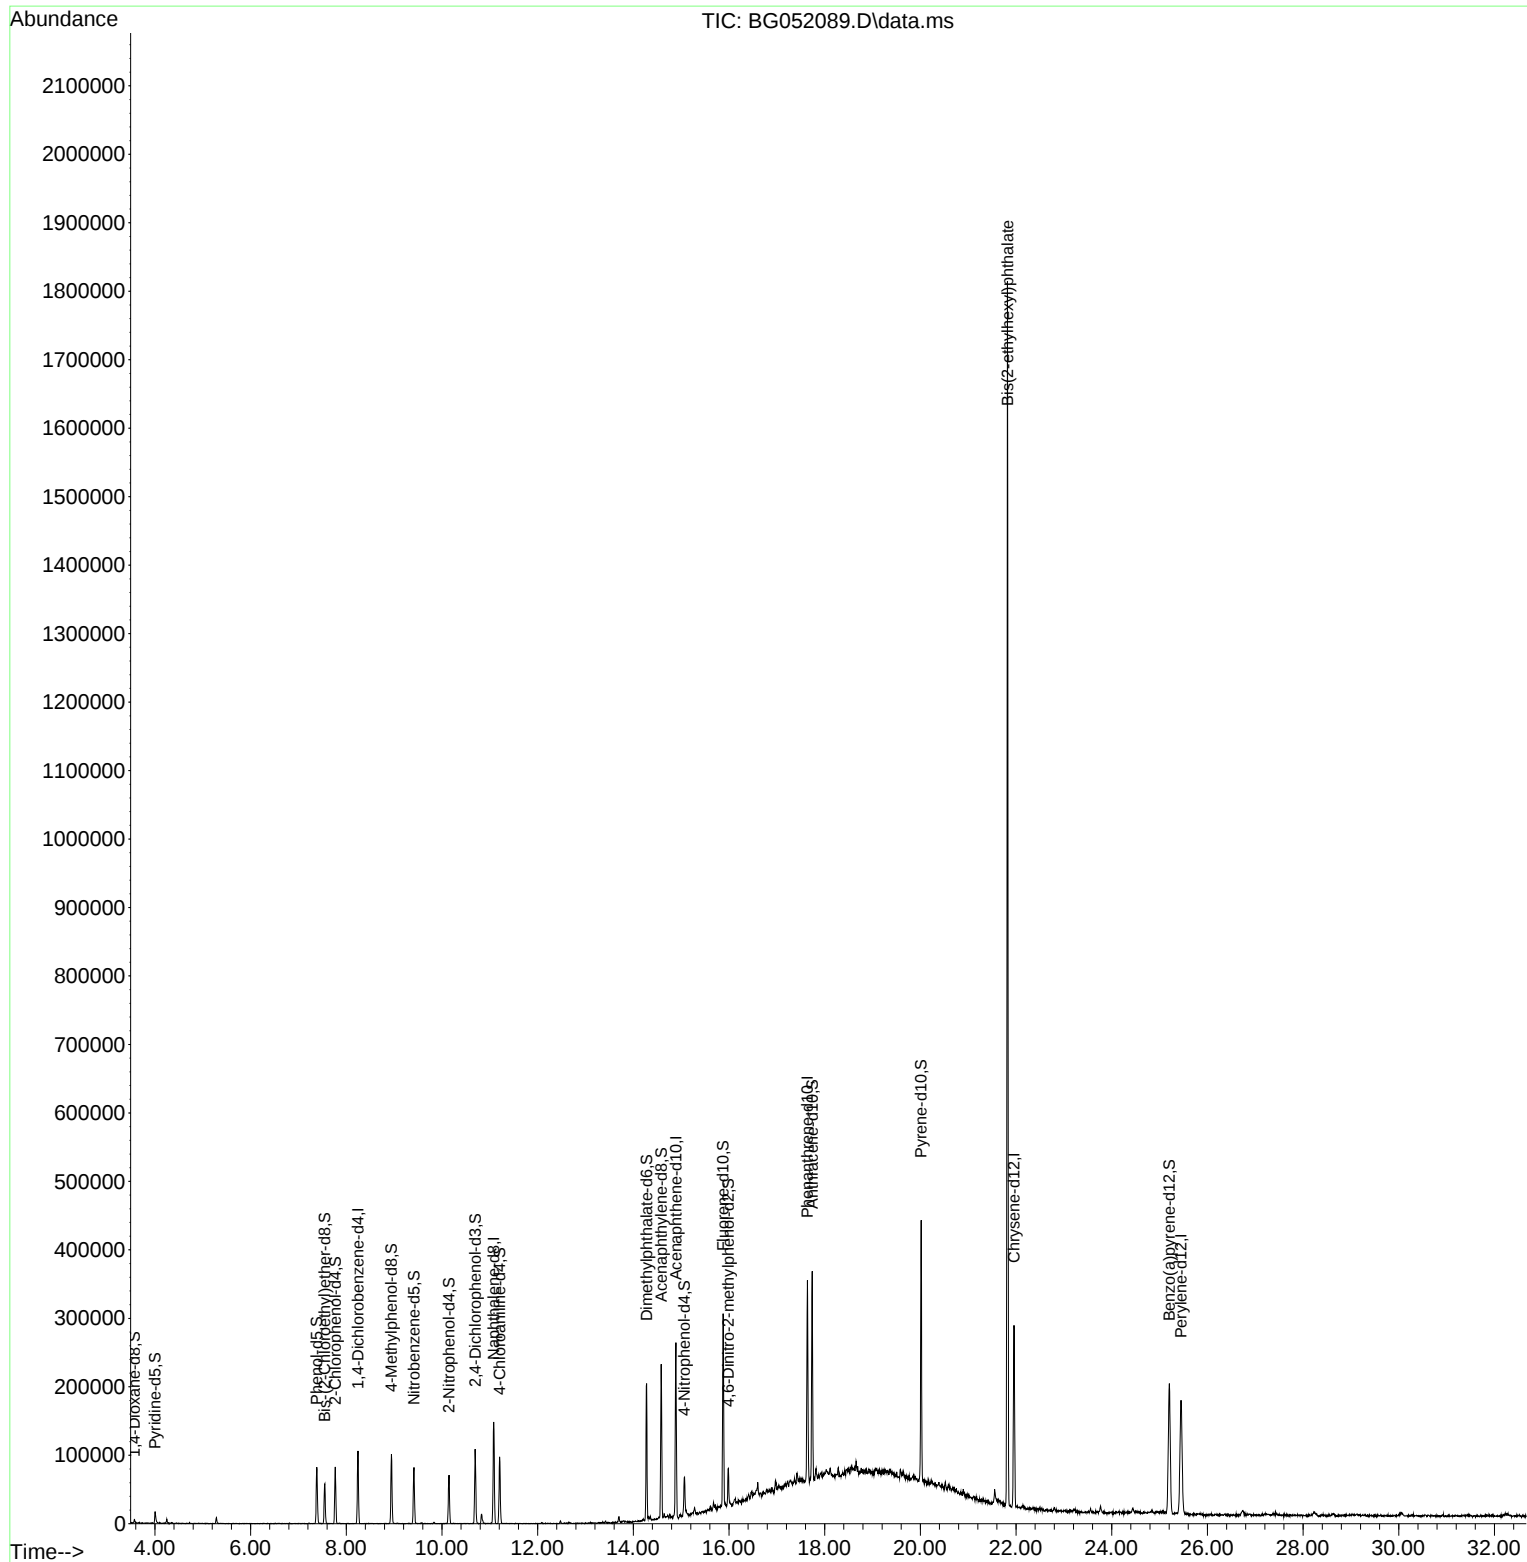

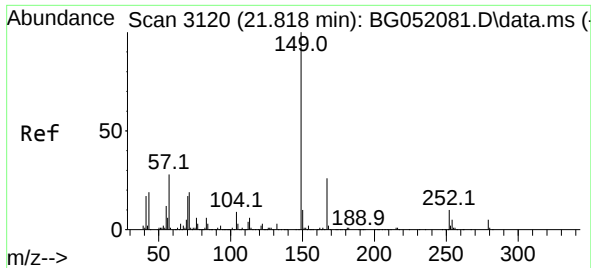

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 115.202 ng/ul
 RT: 21.821 min Scan# 31
 Delta R.T. 0.004 min
 Lab File: BG052089.D
 Acq: 20 Jan 2022 1:28

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7ME

Tgt Ion:149 Resp: 700034
 Ion Ratio Lower Upper
 149 100
 167 28.0 21.1 31.7
 279 5.1 2.7 4.1#

