

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052094.D
 Acq On : 20 Jan 2022 9:45
 Operator : CG/JU
 Sample : N1169-01MEDL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7MEDL

Quant Time: Jan 20 10:19:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.252	152	34328	20.000	ng/ul	0.00
20) Naphthalene-d8	11.089	136	144802	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.890	164	105214	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.639	188	219021	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.957	240	218761	20.000	ng/ul	# 0.00
88) Perylene-d12	25.452	264	240344	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.570	96	1078	1.122	ng/uL	0.00
4) Pyridine-d5	4.017	84	5555	1.860	ng/ul	0.01
7) Phenol-d5	7.389	99	27211	8.099	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.559	67	17837	8.363	ng/ul	0.00
11) 2-Chlorophenol-d4	7.776	132	19952	8.969	ng/ul	0.00
15) 4-Methylphenol-d8	8.951	113	21505	8.234	ng/ul	0.00
21) Nitrobenzene-d5	9.421	128	10580	9.247	ng/ul	0.00
24) 2-Nitrophenol-d4	10.155	143	11372	8.987	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.702	165	23505	9.503	ng/ul	0.00
31) 4-Chloroaniline-d4	11.213	131	28018	8.134	ng/ul	0.00
46) Dimethylphthalate-d6	14.279	166	78735	9.053	ng/ul	0.00
49) Acenaphthylene-d8	14.585	160	98494	9.376	ng/ul	0.00
54) 4-Nitrophenol-d4	15.072	143	6168	4.242	ng/ul	0.00
60) Fluorene-d10	15.877	176	69757	9.200	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.983	200	5591	4.046	ng/ul	0.00
73) Anthracene-d10	17.739	188	104888	10.095	ng/ul	0.00
81) Pyrene-d10	20.019	212	124789	9.912	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.206	264	128479	10.154	ng/ul	0.01


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.822	149	420427	57.666 ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052094.D
Acq On : 20 Jan 2022 9:45
Operator : CG/JU
Sample : N1169-01MEDL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7MEDL

Quant Time: Jan 20 10:19:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

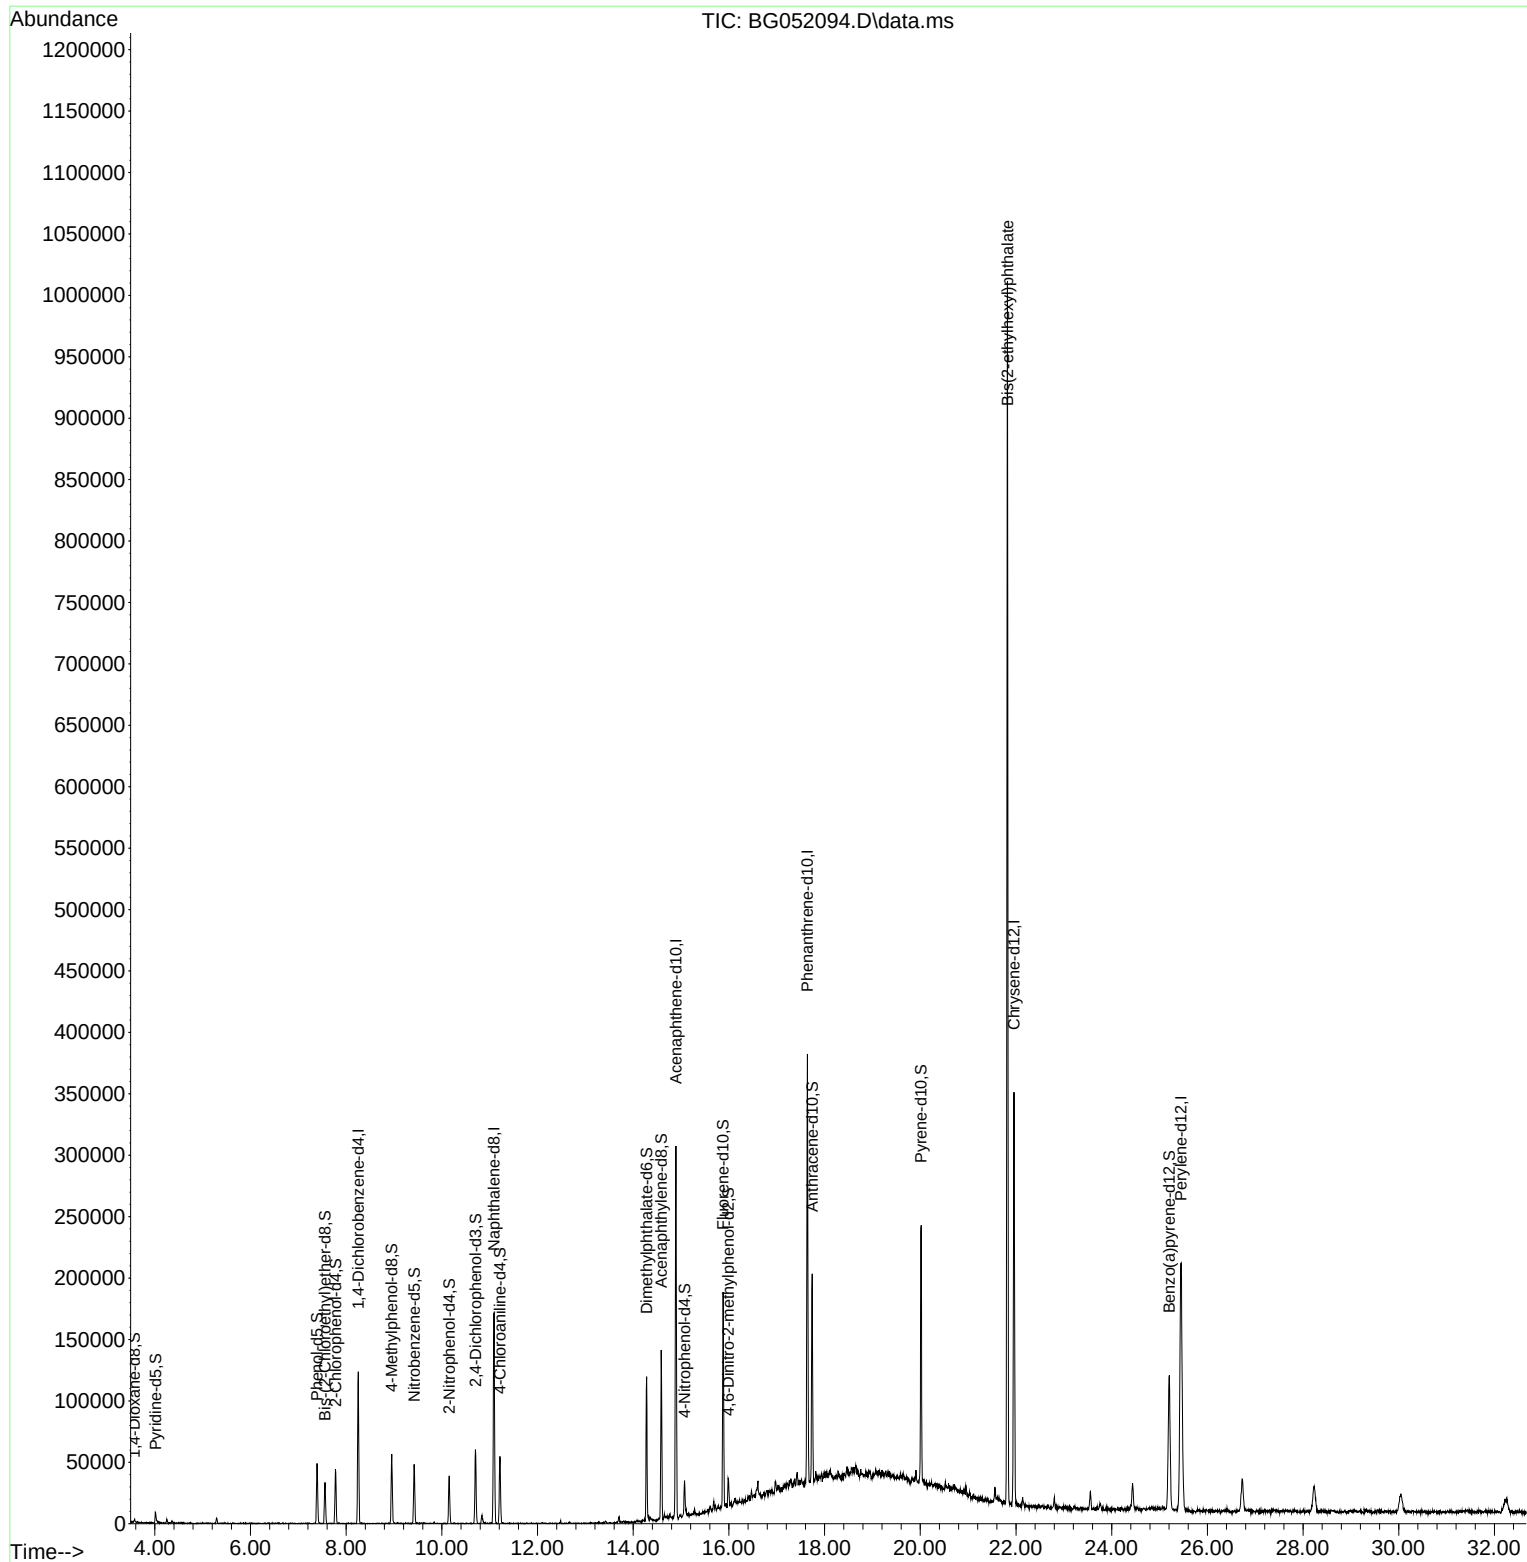

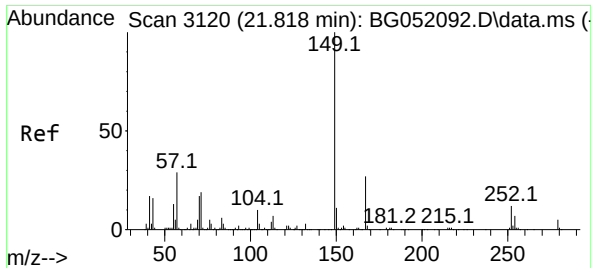

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 57.666 ng/ul
 RT: 21.822 min Scan# 31
 Delta R.T. 0.005 min
 Lab File: BG052094.D
 Acq: 20 Jan 2022 9:45

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7MEDL

Tgt Ion:149 Resp: 420427
 Ion Ratio Lower Upper
 149 100
 167 26.9 21.1 31.7
 279 4.8 2.7 4.1#

