

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052106.D
 Acq On : 20 Jan 2022 23:47
 Operator : CG/JU
 Sample : N1199-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F10

Quant Time: Jan 21 01:25:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.242	152	26823	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.079	136	117521	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.886	164	86644	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.635	188	202674	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.953	240	196085	20.000	ng/ul	# 0.00
88) Perylene-d12	25.436	264	199040	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.566	96	3220	4.290	ng/uL	-0.01
4) Pyridine-d5	4.001	84	17413	7.462	ng/ul	0.00
7) Phenol-d5	7.384	99	18874	7.189	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.549	67	46283	27.772	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.766	132	43756	25.174	ng/ul	-0.01
15) 4-Methylphenol-d8	8.941	113	34377	16.845	ng/ul	-0.01
21) Nitrobenzene-d5	9.411	128	28406	30.589	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.145	143	31979	31.137	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.692	165	58532	29.157	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.203	131	57589	20.599	ng/ul	-0.01
46) Dimethylphthalate-d6	14.275	166	217244	30.334	ng/ul	0.00
49) Acenaphthylene-d8	14.581	160	260864	30.154	ng/ul	0.00
54) 4-Nitrophenol-d4	15.068	143	7070	5.905	ng/ul	0.00
60) Fluorene-d10	15.873	176	190065	30.439	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.985	200	32653	25.539	ng/ul	0.00
73) Anthracene-d10	17.735	188	316171	32.885	ng/ul	0.00
81) Pyrene-d10	20.014	212	372479	33.006	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.196	264	350094	33.411	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.408	94	3986	1.488	ng/ul#	85
59) Diethylphthalate	15.679	149	12804	1.757	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052106.D
Acq On : 20 Jan 2022 23:47
Operator : CG/JU
Sample : N1199-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F10

Quant Time: Jan 21 01:25:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration




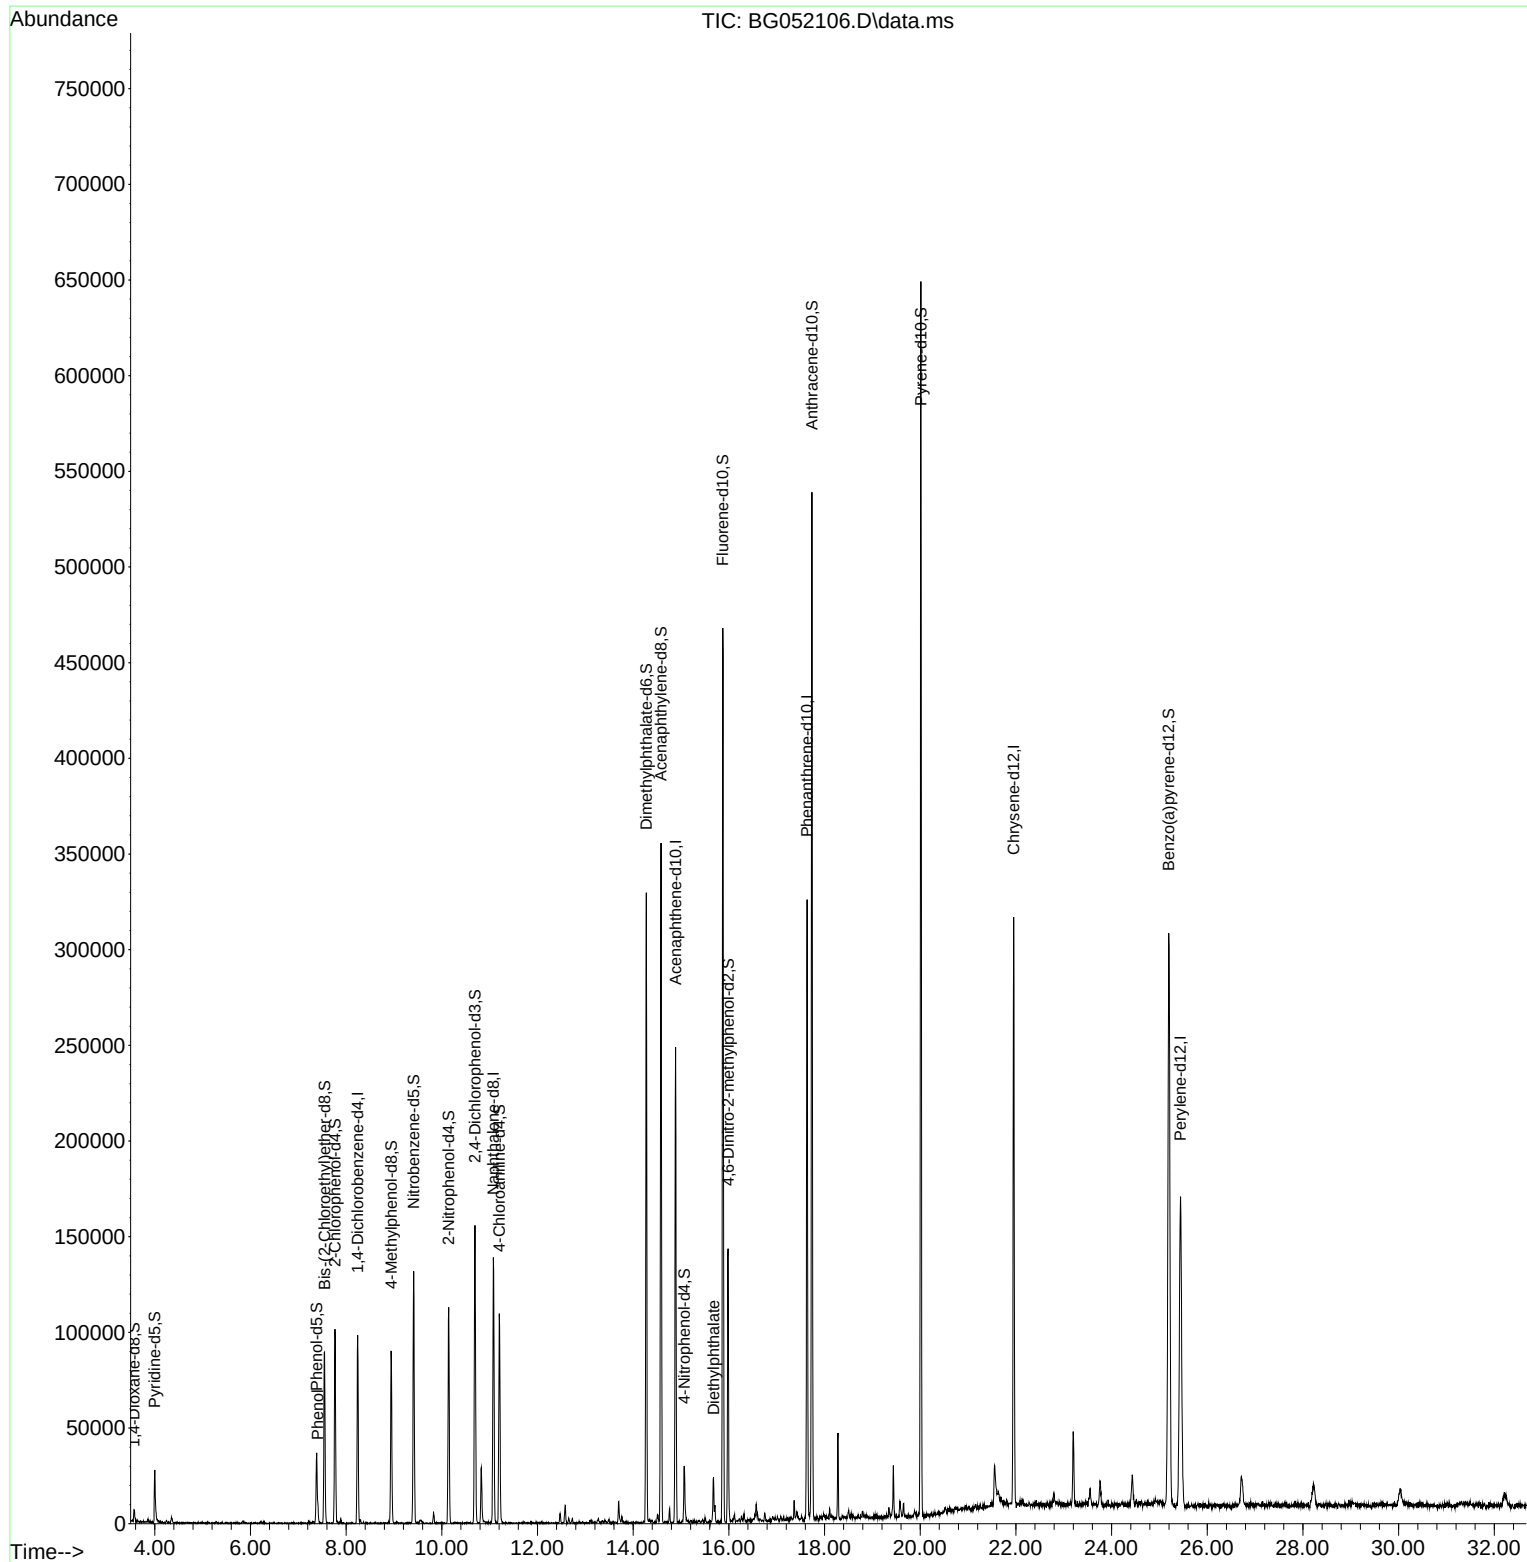


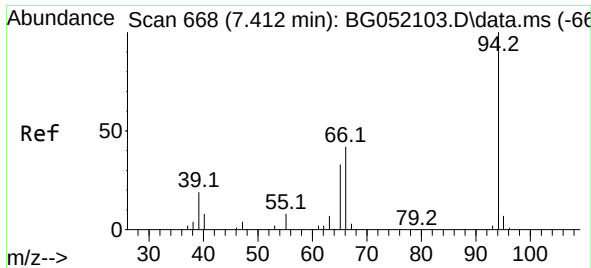

#8
Phenol
Concen: 1.488 ng/ul
RT: 7.408 min Scan# 60
Delta R.T. -0.011 min
Lab File: BG052106.D
Acq: 20 Jan 2022 23:47

Instrument :
BNA_G
ClientSampleId :
C0F10

Tgt Ion: 94 Resp: 3986
Ion Ratio Lower Upper
94 100
65 28.3 25.1 37.7
66 53.6 31.6 47.4#

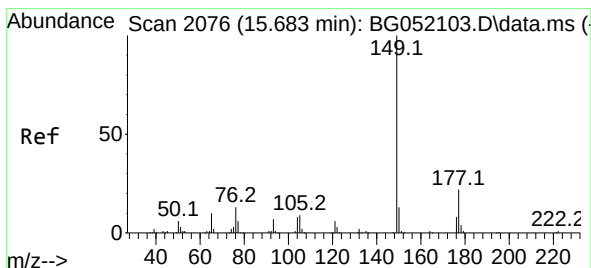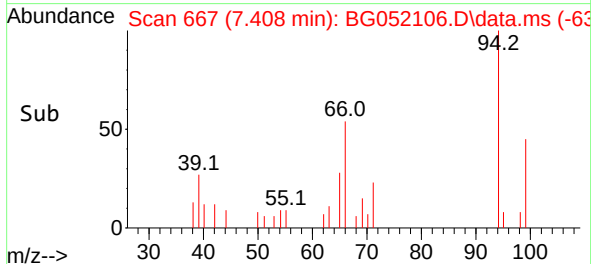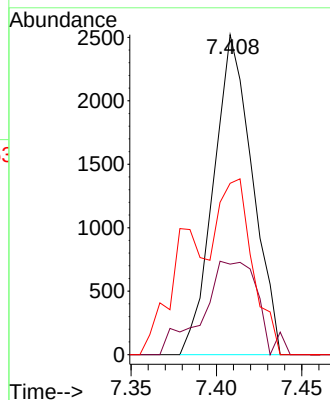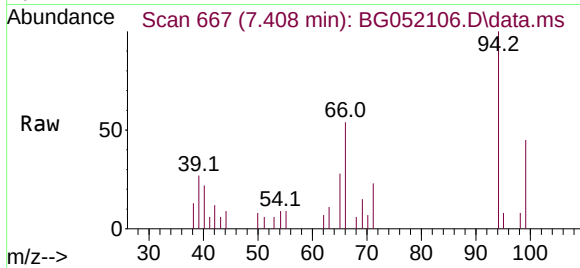

#59
Diethylphthalate
Concen: 1.757 ng/ul
RT: 15.679 min Scan# 2075
Delta R.T. -0.005 min
Lab File: BG052106.D
Acq: 20 Jan 2022 23:47

Tgt Ion: 149 Resp: 12804
Ion Ratio Lower Upper
149 100
177 25.8 16.8 25.2#
150 10.9 10.1 15.1

