

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052107.D
 Acq On : 21 Jan 2022 00:24
 Operator : CG/JU
 Sample : N1199-08
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F14

Quant Time: Jan 21 01:25:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.242	152	25245	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.085	136	108732	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.886	164	83139	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.635	188	190092	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.953	240	181445	20.000	ng/u1	# 0.00
88) Perylene-d12	25.437	264	181117	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.572	96	3501	4.955	ng/uL	0.00
4) Pyridine-d5	4.007	84	7021	3.197	ng/u1	0.00
7) Phenol-d5	7.379	99	22243	9.002	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.549	67	51947	33.119	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.772	132	49971	30.547	ng/u1	0.00
15) 4-Methylphenol-d8	8.941	113	39268	20.444	ng/u1	-0.01
21) Nitrobenzene-d5	9.411	128	33035	38.450	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.146	143	37423	39.383	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.692	165	68390	36.822	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.203	131	60923	23.554	ng/u1	-0.01
46) Dimethylphthalate-d6	14.275	166	251328	36.572	ng/u1	0.00
49) Acenaphthylene-d8	14.581	160	307842	37.085	ng/u1	0.00
54) 4-Nitrophenol-d4	15.068	143	8606	7.490	ng/u1	0.00
60) Fluorene-d10	15.879	176	221186	36.916	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.985	200	39295	32.768	ng/u1	0.00
73) Anthracene-d10	17.735	188	376537	41.756	ng/u1	0.00
81) Pyrene-d10	20.015	212	434968	41.654	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.202	264	404439	42.417	ng/u1	0.00
Target Compounds						
59) Diethylphthalate	15.679	149	18945	2.710	ng/u1	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052107.D
Acq On : 21 Jan 2022 00:24
Operator : CG/JU
Sample : N1199-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F14

Quant Time: Jan 21 01:25:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

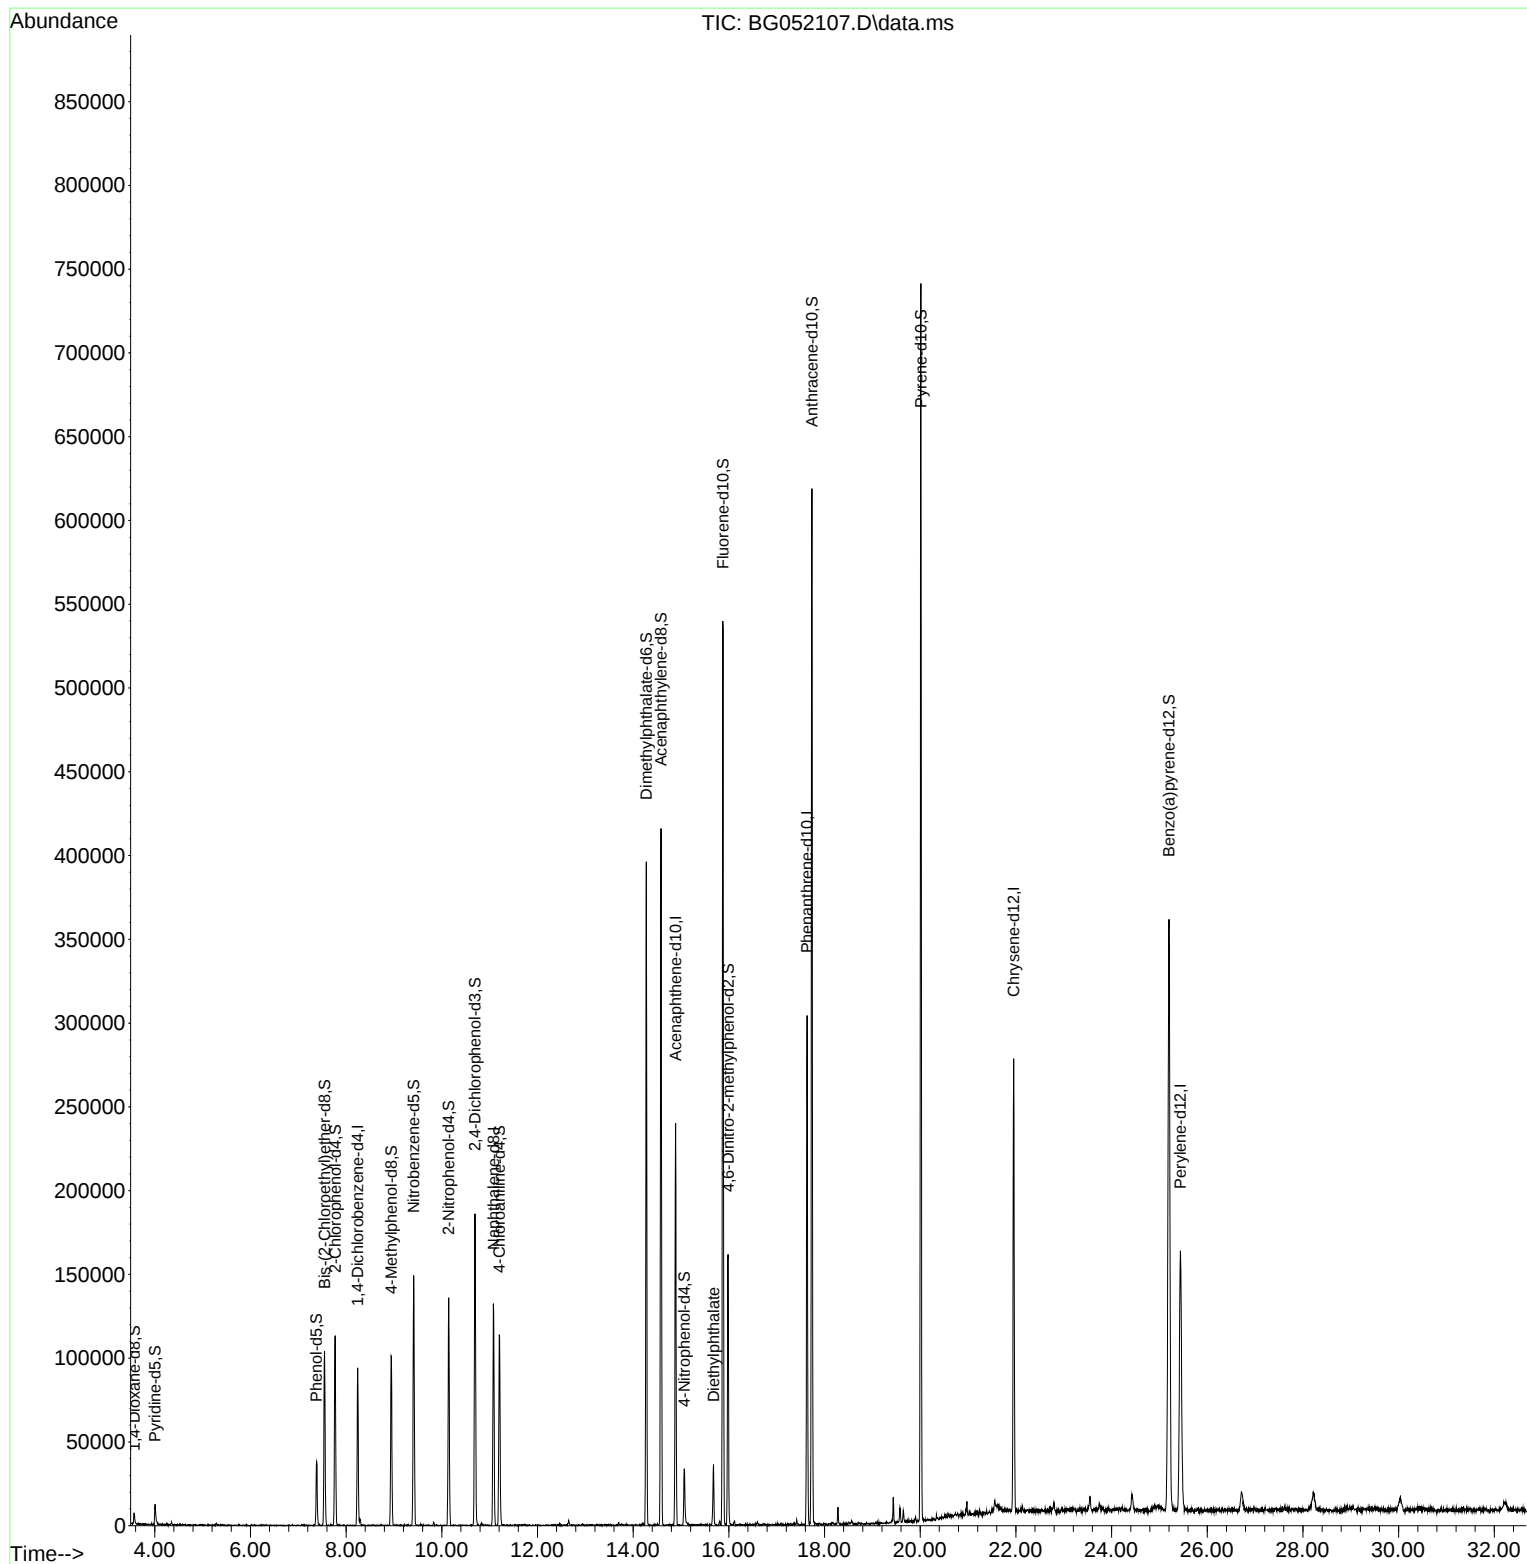

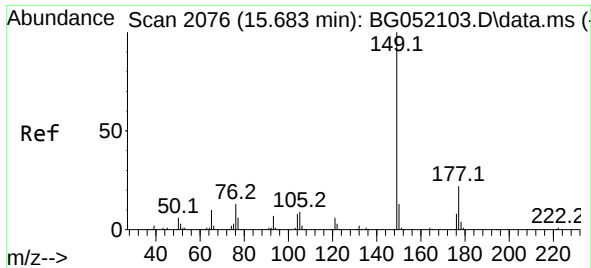

#59
 Diethylphthalate
 Concen: 2.710 ng/ul
 RT: 15.679 min Scan# 2075
 Delta R.T. -0.005 min
 Lab File: BG052107.D
 Acq: 21 Jan 2022 00:24

Instrument :
 BNA_G
 ClientSampleId :
 C0F14

Tgt Ion:149 Resp: 18945
 Ion Ratio Lower Upper
 149 100
 177 24.2 16.8 25.2
 150 10.6 10.1 15.1

