

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052109.D
 Acq On : 21 Jan 2022 1:40
 Operator : CG/JU
 Sample : N1199-10
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F39

Quant Time: Jan 21 02:48:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.246	152	25823	20.000	ng/u1	0.00
20) Naphthalene-d8	11.083	136	118931	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.884	164	85141	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.633	188	199130	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.957	240	191412	20.000	ng/u1	# 0.00
88) Perylene-d12	25.440	264	191346	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.570	96	2688	3.720	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.382	99	19308	7.640	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.547	67	48906	30.482	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.770	132	47014	28.096	ng/u1	0.00
15) 4-Methylphenol-d8	8.945	113	35647	18.144	ng/u1	0.00
21) Nitrobenzene-d5	9.415	128	32520	34.604	ng/u1	0.00
24) 2-Nitrophenol-d4	10.143	143	35435	34.093	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.696	165	66841	32.901	ng/u1	0.00
31) 4-Chloroaniline-d4	11.207	131	9647	3.410	ng/u1	0.00
46) Dimethylphthalate-d6	14.279	166	250884	35.649	ng/u1	0.00
49) Acenaphthylene-d8	14.584	160	302678	35.605	ng/u1	0.00
54) 4-Nitrophenol-d4	15.072	143	7054	5.995	ng/u1	0.00
60) Fluorene-d10	15.877	176	223250	36.384	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.983	200	37096	29.530	ng/u1	0.00
73) Anthracene-d10	17.733	188	369043	39.068	ng/u1	0.00
81) Pyrene-d10	20.012	212	426441	38.711	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.199	264	395429	39.255	ng/u1	0.00
Target Compounds						
59) Diethylphthalate	15.677	149	18216	2.544	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052109.D
Acq On : 21 Jan 2022 1:40
Operator : CG/JU
Sample : N1199-10
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F39

Quant Time: Jan 21 02:48:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

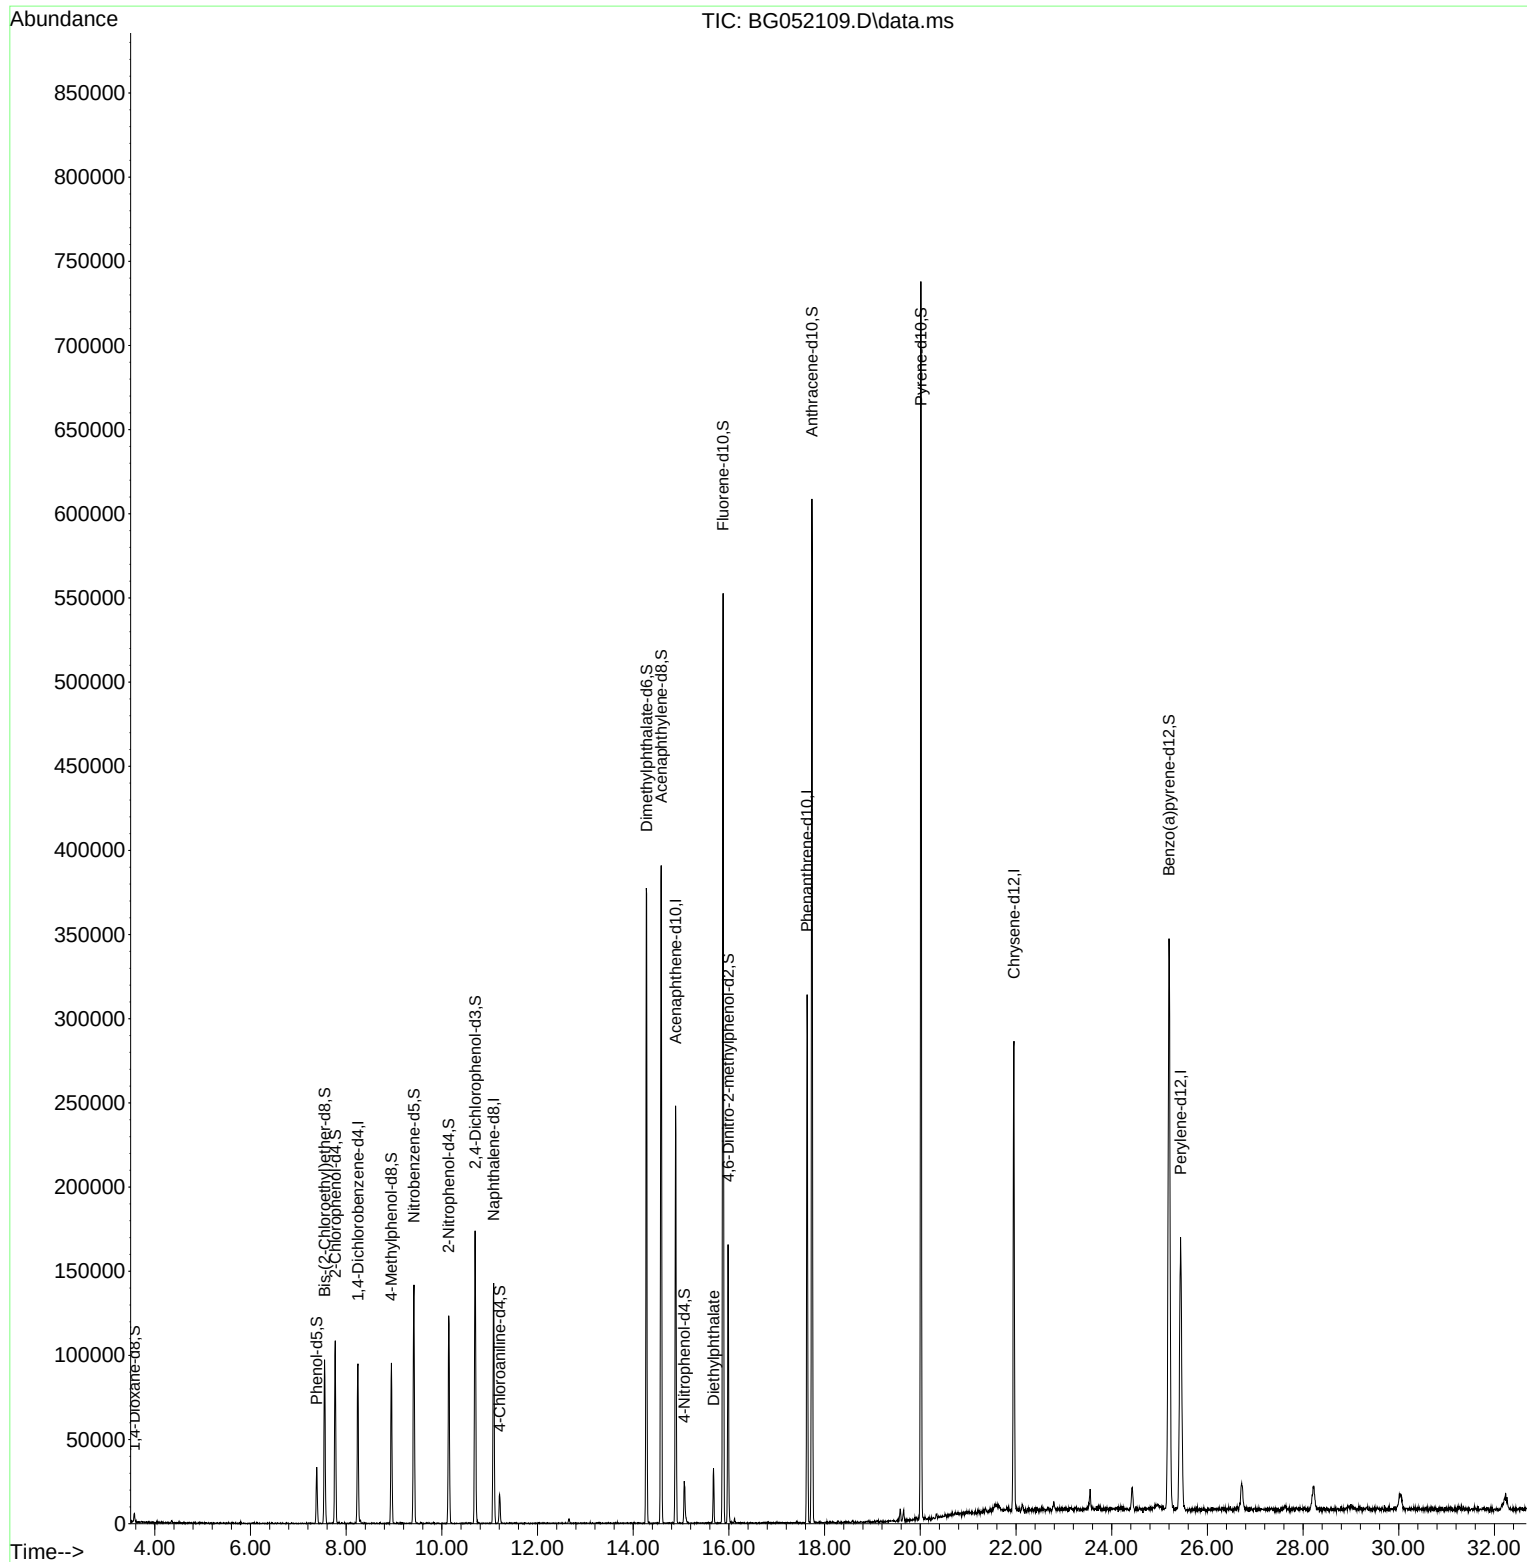

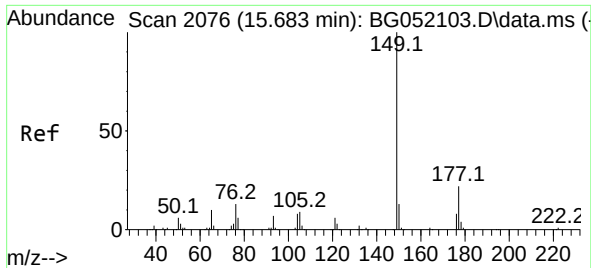

#59
 Diethylphthalate
 Concen: 2.544 ng/ul
 RT: 15.677 min Scan# 2075
 Delta R.T. -0.007 min
 Lab File: BG052109.D
 Acq: 21 Jan 2022 1:40

Instrument :
 BNA_G
 ClientSampleId :
 C0F39

Tgt Ion	Ratio	Lower	Upper
149	100		
177	23.4	16.8	25.2
150	10.7	10.1	15.1

