

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052069.D
 Acq On : 19 Jan 2022 11:37
 Operator : CG/JU
 Sample : N1100-14MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS6MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.038	87	93	97	rBV3	1915	4108	0.57%	0.105%
2	4.349	144	146	152	rBV2	1617	2831	0.39%	0.072%
3	6.481	506	509	512	rBV2	2133	1980	0.28%	0.051%
4	6.605	526	530	533	rBV2	1384	1888	0.26%	0.048%
5	6.699	542	546	551	rBV3	2305	3524	0.49%	0.090%
6	6.775	556	559	565	rBV	3353	4417	0.61%	0.113%
7	6.857	570	573	576	rBV4	2170	2904	0.40%	0.074%
8	7.216	631	634	640	rVV5	4813	6816	0.95%	0.174%
9	7.274	640	644	648	rVB3	1881	2674	0.37%	0.068%
10	7.386	658	663	670	rBV3	10283	18569	2.58%	0.474%
11	7.545	685	690	697	rBV3	5107	10671	1.49%	0.273%
12	7.774	724	729	734	rVB4	6362	11517	1.60%	0.294%
13	8.056	773	777	778	rVV2	1892	2125	0.30%	0.054%
14	8.138	785	791	792	rVV2	1878	2501	0.35%	0.064%
15	8.150	792	793	796	rVV2	2403	2471	0.34%	0.063%
16	8.244	800	809	816	rVV	98481	182614	25.42%	4.664%
17	8.308	816	820	826	rVB4	3081	4801	0.67%	0.123%
18	8.379	828	832	835	rVB	1631	2269	0.32%	0.058%
19	8.432	835	841	845	rBV2	4003	6276	0.87%	0.160%
20	8.490	845	851	856	rBV4	3410	8157	1.14%	0.208%
21	8.537	856	859	866	rVB4	4462	7191	1.00%	0.184%
22	8.778	896	900	902	rBV3	3869	6134	0.85%	0.157%
23	8.831	906	909	915	rVB4	4398	6795	0.95%	0.174%
24	8.896	915	920	922	rBV2	4557	6155	0.86%	0.157%
25	8.943	924	928	935	rVB4	8926	17765	2.47%	0.454%
26	9.013	935	940	943	rBV2	2512	3891	0.54%	0.099%
27	9.096	951	954	959	rBV4	1884	2885	0.40%	0.074%
28	9.137	959	961	964	rBV2	2075	2080	0.29%	0.053%
29	9.366	996	1000	1003	rVV3	3557	4509	0.63%	0.115%
30	9.413	1003	1008	1013	rVV2	7367	11230	1.56%	0.287%
31	9.466	1013	1017	1023	rVB2	3326	5687	0.79%	0.145%
32	9.583	1031	1037	1039	rBV4	1989	3624	0.50%	0.093%
33	9.618	1039	1043	1047	rVB3	2840	4730	0.66%	0.121%
34	9.736	1060	1063	1068	rVB3	2636	3436	0.48%	0.088%
35	9.842	1079	1081	1086	rVB4	2268	2311	0.32%	0.059%
36	9.900	1086	1091	1095	rBV2	3472	5464	0.76%	0.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052069.D
 Acq On : 19 Jan 2022 11:37
 Operator : CG/JU
 Sample : N1100-14MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS6MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	9.959	1095	1101	1104	rVV	2766	4018	0.56%	0.103%
38	10.000	1104	1108	1110	rVV2	1526	2203	0.31%	0.056%
39	10.147	1126	1133	1137	rBV4	7330	11987	1.67%	0.306%
40	10.194	1137	1141	1146	rVV2	3625	5253	0.73%	0.134%
41	10.265	1150	1153	1156	rVV3	2574	3241	0.45%	0.083%
42	10.329	1156	1164	1168	rVV5	2232	5721	0.80%	0.146%
43	10.417	1171	1179	1183	rBB5	3243	6200	0.86%	0.158%
44	10.482	1183	1190	1193	rBV3	3098	5301	0.74%	0.135%
45	10.541	1195	1200	1203	rVB2	2867	4333	0.60%	0.111%
46	10.593	1206	1209	1213	rVB4	1709	2608	0.36%	0.067%
47	10.699	1222	1227	1233	rVB2	7533	13239	1.84%	0.338%
48	10.776	1233	1240	1242	rBV2	1809	2416	0.34%	0.062%
49	11.081	1284	1292	1306	rVB	152477	276356	38.46%	7.059%
50	11.204	1306	1313	1314	rBV2	7805	9861	1.37%	0.252%
51	11.293	1323	1328	1332	rVB2	1318	2064	0.29%	0.053%
52	11.780	1405	1411	1417	rVB5	2681	5028	0.70%	0.128%
53	11.903	1428	1432	1440	rVB2	2606	4015	0.56%	0.103%
54	12.091	1457	1464	1468	rBV3	6721	12327	1.72%	0.315%
55	12.473	1525	1529	1533	rBV2	2440	3806	0.53%	0.097%
56	12.620	1550	1554	1557	rBV2	1543	2368	0.33%	0.060%
57	12.949	1605	1610	1613	rVB2	2406	3383	0.47%	0.086%
58	13.096	1631	1635	1636	rBV2	2212	2306	0.32%	0.059%
59	13.202	1652	1653	1658	rVB2	2054	1972	0.27%	0.050%
60	13.272	1661	1665	1672	rVV4	2970	5785	0.81%	0.148%
61	13.366	1676	1681	1684	rVV2	2756	4424	0.62%	0.113%
62	13.419	1684	1690	1695	rVV3	6995	9690	1.35%	0.247%
63	13.689	1732	1736	1739	rVV2	1797	3256	0.45%	0.083%
64	13.719	1739	1741	1747	rVB5	3190	5108	0.71%	0.130%
65	14.042	1792	1796	1797	rBV	6096	5557	0.77%	0.142%
66	14.212	1819	1825	1829	rBV4	10143	19567	2.72%	0.500%
67	14.277	1831	1836	1840	rVV2	21277	31755	4.42%	0.811%
68	14.330	1840	1845	1846	rVV4	4053	5972	0.83%	0.153%
69	14.353	1846	1849	1853	rVB2	8740	10634	1.48%	0.272%
70	14.388	1853	1855	1858	rBV2	3643	3283	0.46%	0.084%
71	14.441	1860	1864	1867	rBV2	3637	5734	0.80%	0.146%
72	14.582	1882	1888	1894	rBV	23742	38878	5.41%	0.993%
73	14.717	1906	1911	1918	rVB4	5508	8986	1.25%	0.230%
74	14.888	1929	1940	1947	rBV	275712	424454	59.07%	10.841%
75	14.964	1949	1953	1954	rBV3	2277	2287	0.32%	0.058%
76	15.040	1964	1966	1970	rVB5	2534	2506	0.35%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052069.D
 Acq On : 19 Jan 2022 11:37
 Operator : CG/JU
 Sample : N1100-14MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGSL6MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	15.082	1970	1973	1974	rBV2	5941	5925	0.82%	0.151%
78	15.158	1983	1986	1989	rVB5	3433	4063	0.57%	0.104%
79	15.199	1989	1993	1996	rBV5	3682	6865	0.96%	0.175%
80	15.281	2000	2007	2011	rBV6	8018	18939	2.64%	0.484%
81	15.504	2041	2045	2048	rBV5	4168	6840	0.95%	0.175%
82	15.546	2049	2052	2053	rBV2	3368	3407	0.47%	0.087%
83	15.610	2061	2063	2067	rVB5	3708	3836	0.53%	0.098%
84	15.675	2069	2074	2077	rBV4	7271	13421	1.87%	0.343%
85	15.875	2104	2108	2113	rBV	30646	46491	6.47%	1.187%
86	16.121	2146	2150	2161	rVB10	9733	25832	3.60%	0.660%
87	16.333	2184	2186	2190	rVB5	5520	6364	0.89%	0.163%
88	16.568	2223	2226	2228	rBV4	4631	7552	1.05%	0.193%
89	16.597	2228	2231	2236	rVB2	19077	28869	4.02%	0.737%
90	16.885	2278	2280	2283	rBV4	4138	4552	0.63%	0.116%
91	17.637	2402	2408	2414	rBV	315995	487486	67.85%	12.451%
92	17.731	2421	2424	2430	rVB2	30483	47165	6.56%	1.205%
93	19.064	2649	2651	2656	rVB4	10366	12570	1.75%	0.321%
94	19.387	2705	2706	2707	rBV	5243	2970	0.41%	0.076%
95	19.605	2740	2743	2747	rBV5	10129	14095	1.96%	0.360%
96	20.016	2808	2813	2819	rBV2	39892	62153	8.65%	1.587%
97	20.327	2864	2866	2869	rBV2	7588	7789	1.08%	0.199%
98	21.819	3114	3120	3130	rVB	510367	718516	100.00%	18.352%
99	21.960	3137	3144	3151	rBV	273815	485760	67.61%	12.407%
100	25.444	3728	3737	3752	rVB2	165852	538879	75.00%	13.764%




Sum of corrected areas: 3915221

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052069.D
Acq On : 19 Jan 2022 11:37
Operator : CG/JU
Sample : N1100-14MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS6MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

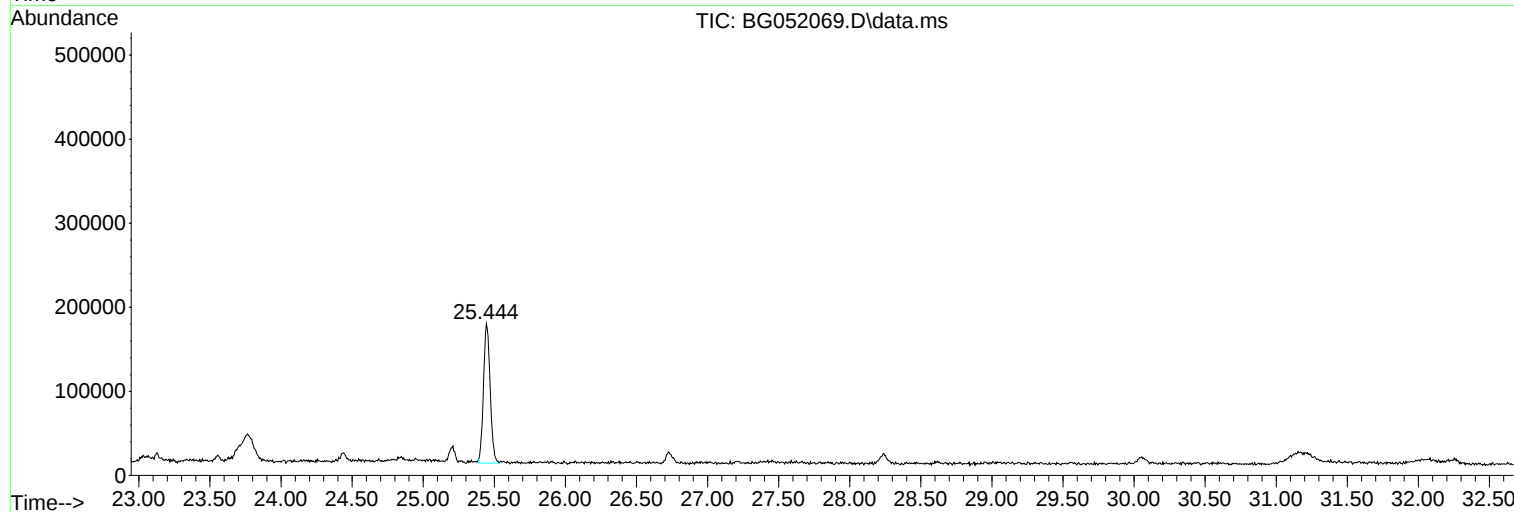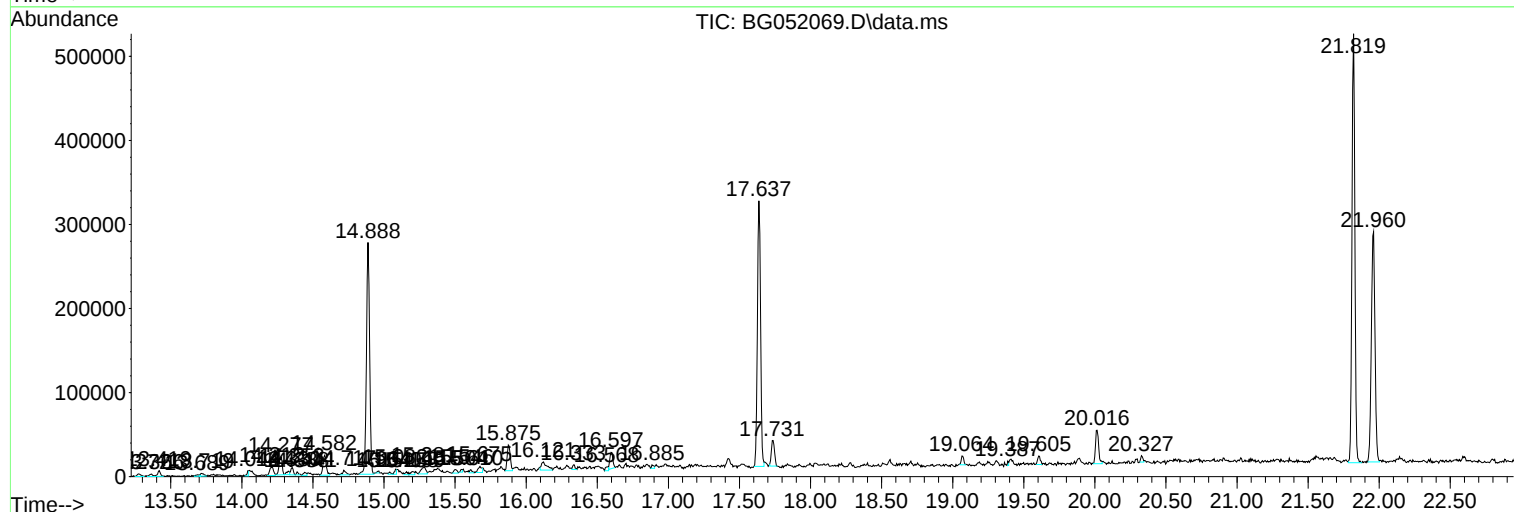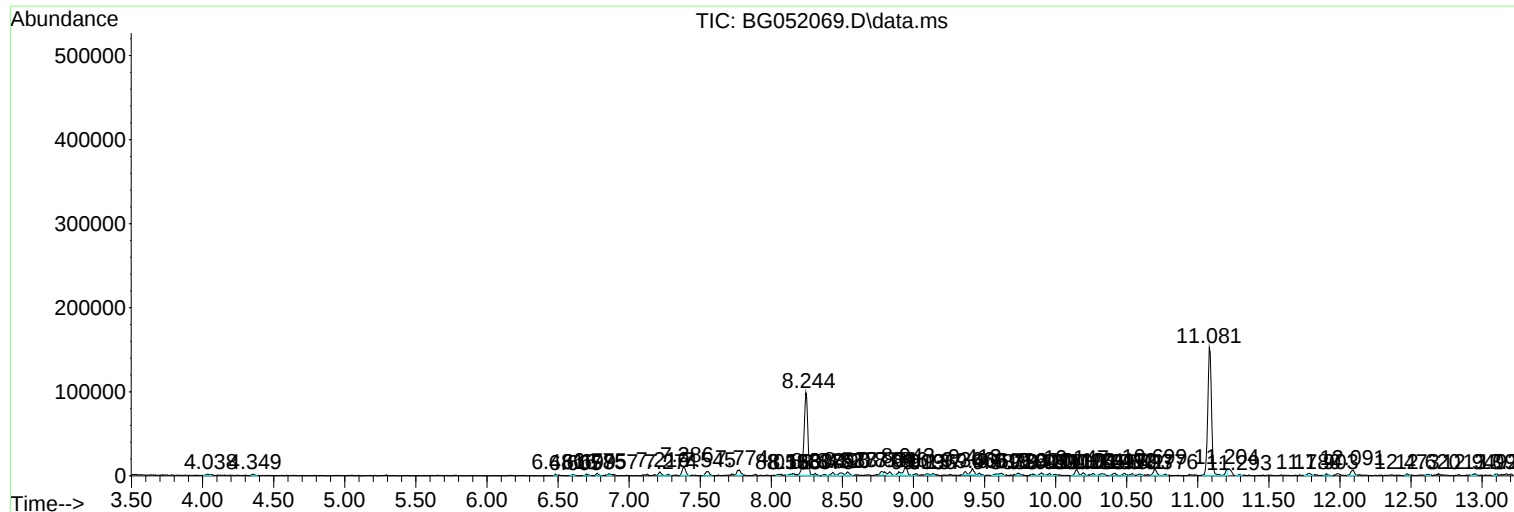

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052069.D
Acq On : 19 Jan 2022 11:37
Operator : CG/JU
Sample : N1100-14MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS6MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052069.D
Acq On : 19 Jan 2022 11:37
Operator : CG/JU
Sample : N1100-14MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS6MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc