

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052076.D
 Acq On : 19 Jan 2022 16:40
 Operator : CG/JU
 Sample : N1129-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.571	8	14	18	rBV2	3926	5411	0.87%	0.084%
2	3.911	68	72	73	rVB	1032	1201	0.19%	0.019%
3	4.005	84	88	93	rBV	16917	27738	4.48%	0.430%
4	4.111	103	106	111	rVB3	5400	7353	1.19%	0.114%
5	4.193	114	120	123	rVB2	1111	1432	0.23%	0.022%
6	4.246	125	129	133	rBV2	4028	5957	0.96%	0.092%
7	4.346	144	146	148	rBV2	1654	1767	0.29%	0.027%
8	4.569	179	184	188	rBV	1428	2141	0.35%	0.033%
9	4.716	205	209	212	rBV	815	1340	0.22%	0.021%
10	5.292	300	307	311	rBV2	6770	11907	1.92%	0.185%
11	5.374	316	321	325	rVV2	1524	2342	0.38%	0.036%
12	7.383	656	663	672	rVB	72994	131029	21.18%	2.033%
13	7.548	684	691	699	rBV	54947	88831	14.36%	1.378%
14	7.612	699	702	705	rVB2	917	1061	0.17%	0.016%
15	7.771	720	729	736	rBV	72342	121024	19.56%	1.878%
16	7.859	741	744	747	rVV	1101	1058	0.17%	0.016%
17	8.241	803	809	820	rVB	90073	155544	25.14%	2.414%
18	8.946	921	929	937	rBV2	72122	126476	20.44%	1.963%
19	9.069	944	950	954	rBB3	1746	3095	0.50%	0.048%
20	9.410	1002	1008	1017	rBV	73946	133055	21.50%	2.065%
21	9.563	1031	1034	1039	rBV2	1417	2323	0.38%	0.036%
22	9.833	1075	1080	1085	rBB3	2342	3495	0.56%	0.054%
23	10.144	1126	1133	1141	rBV2	65419	117993	19.07%	1.831%
24	10.291	1155	1158	1163	rVB	576	1055	0.17%	0.016%
25	10.696	1220	1227	1237	rBV	96795	173723	28.08%	2.696%
26	11.084	1285	1293	1300	rBV	135703	240400	38.85%	3.731%
27	11.131	1300	1301	1307	rVB2	1024	1084	0.18%	0.017%
28	11.207	1307	1314	1322	rBV	63595	122659	19.82%	1.903%
29	12.652	1555	1560	1566	rBV2	1507	2530	0.41%	0.039%
30	12.729	1568	1573	1578	rBV	1111	1803	0.29%	0.028%
31	13.698	1733	1738	1742	rBV4	4239	5914	0.96%	0.092%
32	13.763	1744	1749	1754	rVV2	2060	2981	0.48%	0.046%
33	14.274	1830	1836	1842	rBV	192795	276361	44.66%	4.289%
34	14.350	1846	1849	1854	rVB2	1117	1512	0.24%	0.023%
35	14.509	1873	1876	1880	rVB2	1214	1312	0.21%	0.020%
36	14.585	1882	1889	1898	rVB	214368	337541	54.55%	5.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052076.D
 Acq On : 19 Jan 2022 16:40
 Operator : CG/JU
 Sample : N1129-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	14.761	1916	1919	1923	rBV	2795	3457	0.56%	0.054%
38	14.891	1931	1941	1947	rBV	234570	367830	59.45%	5.708%
39	14.949	1949	1951	1955	rVB	1208	1224	0.20%	0.019%
40	15.067	1964	1971	1979	rBV2	48897	89951	14.54%	1.396%
41	15.202	1992	1994	1997	rVB2	1047	1175	0.19%	0.018%
42	15.255	2000	2003	2005	rBV2	1242	1084	0.18%	0.017%
43	15.284	2005	2008	2013	rVB3	1905	2331	0.38%	0.036%
44	15.507	2042	2046	2047	rBV2	1797	1201	0.19%	0.019%
45	15.654	2068	2071	2072	rBV	1572	1309	0.21%	0.020%
46	15.672	2072	2074	2078	rVV3	2023	2231	0.36%	0.035%
47	15.713	2078	2081	2084	rVV	1999	2282	0.37%	0.035%
48	15.878	2103	2109	2116	rBV	280851	418024	67.56%	6.487%
49	15.983	2121	2127	2134	rBV2	70505	102552	16.57%	1.591%
50	16.118	2145	2150	2153	rBV2	1199	1840	0.30%	0.029%
51	16.471	2206	2210	2212	rBV	1059	1484	0.24%	0.023%
52	16.547	2220	2223	2224	rBV2	1128	1233	0.20%	0.019%
53	16.577	2224	2228	2230	rVV4	2661	3944	0.64%	0.061%
54	16.594	2230	2231	2235	rVB2	3354	3394	0.55%	0.053%
55	16.653	2239	2241	2246	rVB	988	1270	0.21%	0.020%
56	16.753	2256	2258	2260	rBV	1674	1236	0.20%	0.019%
57	16.812	2264	2268	2272	rVB2	1960	2752	0.44%	0.043%
58	16.853	2272	2275	2278	rBV2	1601	1670	0.27%	0.026%
59	16.976	2293	2296	2298	rVB	1895	1914	0.31%	0.030%
60	17.017	2298	2303	2304	rBV	1082	1353	0.22%	0.021%
61	17.094	2312	2316	2319	rBV2	1072	1436	0.23%	0.022%
62	17.152	2323	2326	2329	rBV3	1002	1065	0.17%	0.017%
63	17.287	2346	2349	2352	rVB2	1476	1438	0.23%	0.022%
64	17.364	2358	2362	2366	rBV3	3701	5477	0.89%	0.085%
65	17.411	2369	2370	2371	rVV	2241	1208	0.20%	0.019%
66	17.452	2375	2377	2379	rVV	1120	1026	0.17%	0.016%
67	17.528	2382	2390	2392	rBV4	4567	8501	1.37%	0.132%
68	17.634	2402	2408	2414	rBV	309478	469322	75.85%	7.283%
69	17.681	2414	2416	2420	rVV2	19058	23051	3.73%	0.358%
70	17.734	2420	2425	2436	rVV2	299746	467965	75.63%	7.262%
71	17.834	2440	2442	2445	rVB	1616	1895	0.31%	0.029%
72	17.857	2445	2446	2448	rBV2	1527	1082	0.17%	0.017%
73	18.110	2485	2489	2493	rVB4	2066	3124	0.50%	0.048%
74	18.157	2495	2497	2501	rBV2	1955	2038	0.33%	0.032%
75	18.280	2514	2518	2523	rVB4	5489	6896	1.11%	0.107%
76	18.321	2523	2525	2527	rBV	1106	1147	0.19%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052076.D
 Acq On : 19 Jan 2022 16:40
 Operator : CG/JU
 Sample : N1129-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	18.392	2533	2537	2538	rBV4	1869	2629	0.42%	0.041%
78	18.503	2552	2556	2561	rVV4	10638	17534	2.83%	0.272%
79	18.568	2563	2567	2574	rVB6	4361	8323	1.35%	0.129%
80	18.709	2586	2591	2595	rBV5	5078	9275	1.50%	0.144%
81	18.744	2595	2597	2602	rVB4	3517	3715	0.60%	0.058%
82	18.797	2602	2606	2608	rBV4	2689	3676	0.59%	0.057%
83	19.003	2637	2641	2642	rBV3	2327	2670	0.43%	0.041%
84	19.114	2656	2660	2662	rBV4	2371	3444	0.56%	0.053%
85	19.273	2685	2687	2692	rBV5	1779	2028	0.33%	0.031%
86	19.367	2700	2703	2707	rVB4	3007	4310	0.70%	0.067%
87	19.437	2707	2715	2720	rBV7	10263	23172	3.74%	0.360%
88	19.578	2733	2739	2741	rBV7	6444	9698	1.57%	0.150%
89	19.678	2749	2756	2763	rVB	51348	81666	13.20%	1.267%
90	19.772	2770	2772	2776	rVB5	3375	3754	0.61%	0.058%
91	20.013	2807	2813	2823	rBV2	382780	618747	100.00%	9.602%
92	20.113	2828	2830	2832	rVB3	2546	1773	0.29%	0.028%
93	20.207	2844	2846	2847	rBV2	2938	2292	0.37%	0.036%
94	20.348	2868	2870	2871	rBV	3096	2048	0.33%	0.032%
95	21.564	3072	3077	3080	rBV4	26182	48421	7.83%	0.751%
96	21.811	3116	3119	3125	rBV4	9162	15973	2.58%	0.248%
97	21.958	3136	3144	3150	rBV	280056	524795	84.82%	8.144%
98	22.798	3285	3287	3296	rVB8	11541	20098	3.25%	0.312%
99	25.200	3688	3696	3705	rBV3	150387	426365	68.91%	6.616%
100	25.447	3728	3738	3751	rBV3	151479	471882	76.26%	7.323%




Sum of corrected areas: 6444148

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052076.D
Acq On : 19 Jan 2022 16:40
Operator : CG/JU
Sample : N1129-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

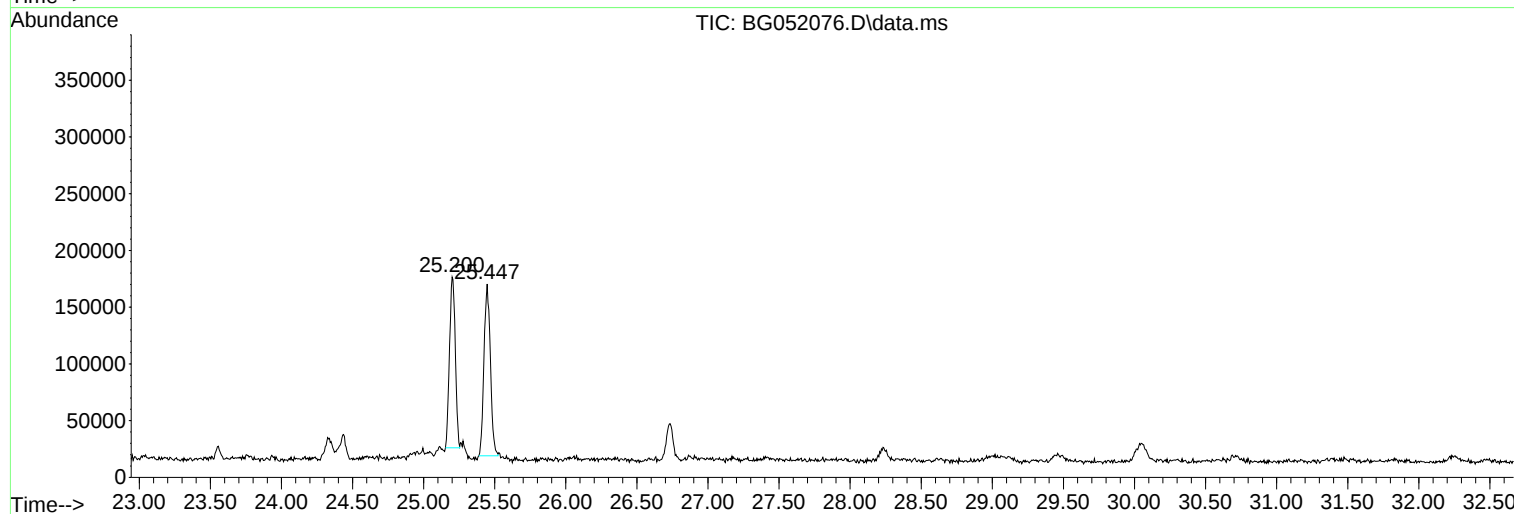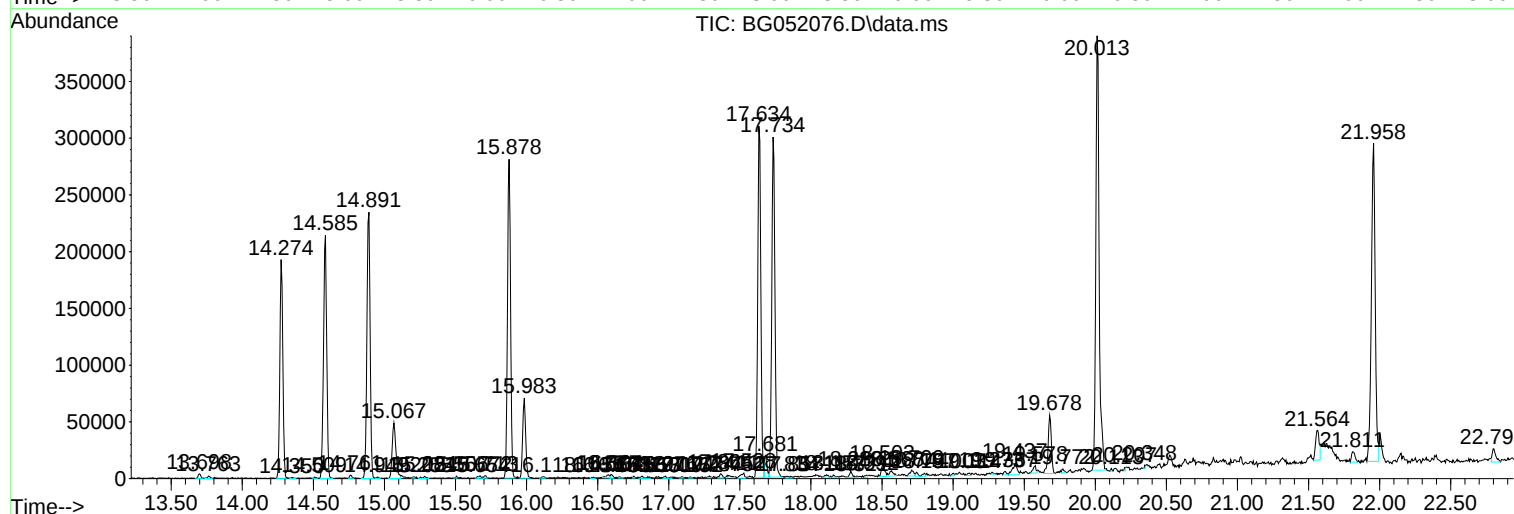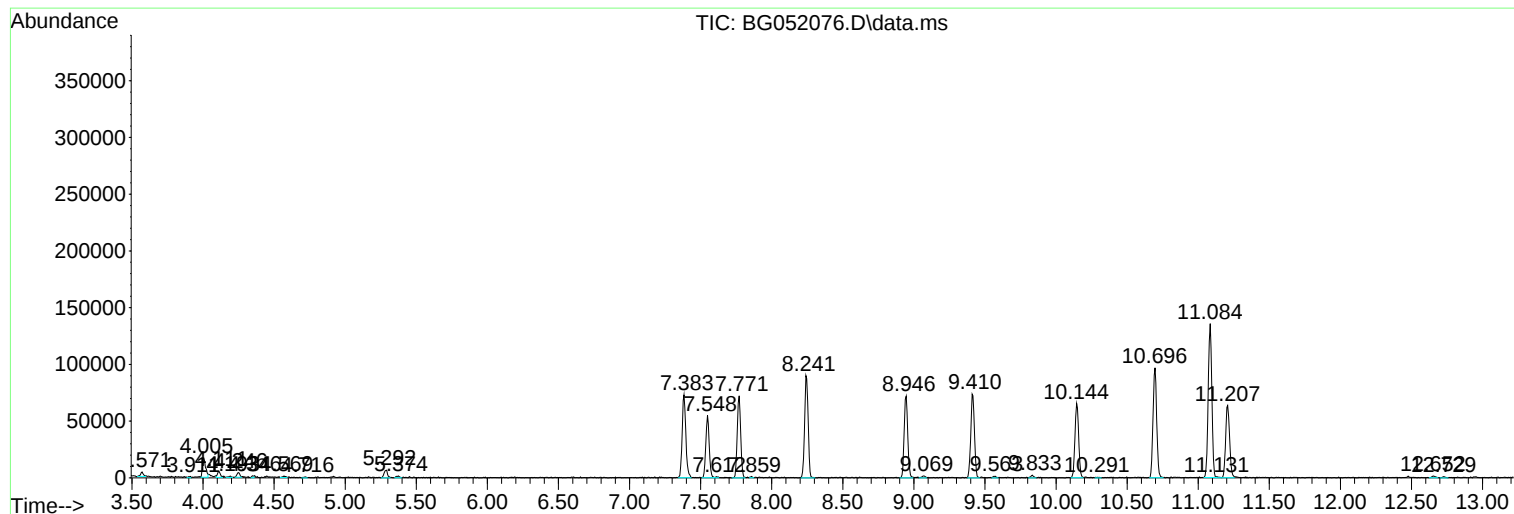

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052076.D
Acq On : 19 Jan 2022 16:40
Operator : CG/JU
Sample : N1129-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052076.D
Acq On : 19 Jan 2022 16:40
Operator : CG/JU
Sample : N1129-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc