

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052089.D
 Acq On : 20 Jan 2022 1:28
 Operator : CG/JU
 Sample : N1169-01ME
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	8	14	20	rBV2	5491	8794	0.35%	0.094%
2	4.004	84	88	97	rBV2	17077	28955	1.16%	0.310%
3	4.251	125	130	135	rVB2	6474	8969	0.36%	0.096%
4	5.285	300	306	313	rBV3	8720	13539	0.54%	0.145%
5	7.382	656	663	672	rBV	82588	148426	5.94%	1.589%
6	7.552	685	692	701	rVB	58386	97670	3.91%	1.046%
7	7.769	721	729	737	rBV	82965	137893	5.52%	1.476%
8	8.245	802	810	816	rBV	106127	178778	7.16%	1.914%
9	8.944	921	929	938	rVB	101392	172881	6.92%	1.851%
10	9.414	1002	1009	1016	rBV	82186	144209	5.77%	1.544%
11	9.831	1076	1080	1086	rVB2	1918	2734	0.11%	0.029%
12	10.149	1127	1134	1142	rBV	70868	127091	5.09%	1.361%
13	10.695	1220	1227	1238	rVB	108885	186724	7.48%	1.999%
14	10.830	1243	1250	1258	rBV2	13591	26506	1.06%	0.284%
15	11.083	1286	1293	1305	rVB	148751	270828	10.84%	2.899%
16	11.206	1305	1314	1321	rBV	97716	175188	7.01%	1.876%
17	12.093	1460	1465	1468	rVB3	1587	2883	0.12%	0.031%
18	12.475	1523	1530	1534	rBV2	4289	6349	0.25%	0.068%
19	13.421	1686	1691	1692	rBV3	3257	4237	0.17%	0.045%
20	13.697	1731	1738	1743	rBV6	8738	15171	0.61%	0.162%
21	13.791	1750	1754	1758	rVB5	2333	4226	0.17%	0.045%
22	14.278	1830	1837	1842	rBV	200566	299763	12.00%	3.209%
23	14.325	1842	1845	1847	rVV3	4633	6241	0.25%	0.067%
24	14.355	1847	1850	1854	rVB4	5625	6588	0.26%	0.071%
25	14.584	1882	1889	1895	rBV	224546	355429	14.23%	3.805%
26	14.642	1895	1899	1904	rBV5	6014	7743	0.31%	0.083%
27	14.719	1910	1912	1916	rVB4	4692	5717	0.23%	0.061%
28	14.760	1916	1919	1923	rBV3	6202	9010	0.36%	0.096%
29	14.889	1930	1941	1950	rBV	257405	420492	16.83%	4.502%
30	14.977	1952	1956	1957	rBV4	3981	5323	0.21%	0.057%
31	15.071	1964	1972	1983	rBV2	57639	124863	5.00%	1.337%
32	15.283	2003	2008	2011	rBV7	8505	13412	0.54%	0.144%
33	15.430	2030	2033	2035	rBV4	3159	4931	0.20%	0.053%
34	15.547	2050	2053	2054	rBV2	4489	5061	0.20%	0.054%
35	15.612	2061	2064	2069	rVB7	7494	11128	0.45%	0.119%
36	15.676	2071	2075	2079	rBV7	11137	17391	0.70%	0.186%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052089.D
 Acq On : 20 Jan 2022 1:28
 Operator : CG/JU
 Sample : N1169-01ME
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.782	2088	2093	2096	rBV6	4640	10487	0.42%	0.112%
38	15.876	2103	2109	2117	rBV	281710	443730	17.76%	4.750%
39	15.988	2122	2128	2137	rBV2	55677	96331	3.86%	1.031%
40	17.421	2369	2372	2376	rBV6	14650	23868	0.96%	0.256%
41	17.638	2404	2409	2416	rVB	295722	473678	18.96%	5.071%
42	17.738	2420	2426	2432	rVB	305109	463019	18.54%	4.957%
43	19.583	2737	2740	2744	rBV5	13833	22770	0.91%	0.244%
44	20.018	2808	2814	2819	rVB	380835	521111	20.86%	5.579%
45	21.551	3073	3075	3082	rVB8	16362	22805	0.91%	0.244%
46	21.762	3109	3111	3112	rBV2	4696	3490	0.14%	0.037%
47	21.821	3114	3121	3128	rVB	1788908	2497809	100.00%	26.741%
48	21.956	3138	3144	3151	rVB	266022	476773	19.09%	5.104%
49	22.455	3225	3229	3231	rBV5	4335	7079	0.28%	0.076%
50	22.667	3263	3265	3268	rBV4	3540	3280	0.13%	0.035%
51	23.125	3341	3343	3346	rBV4	4118	4672	0.19%	0.050%
52	23.284	3368	3370	3371	rVB2	4454	2849	0.11%	0.031%
53	23.301	3371	3373	3375	rBV3	3237	3095	0.12%	0.033%
54	23.342	3378	3380	3382	rBV3	3540	4273	0.17%	0.046%
55	23.560	3413	3417	3419	rBV5	5624	7457	0.30%	0.080%
56	23.601	3422	3424	3427	rBV3	2991	2856	0.11%	0.031%
57	23.765	3449	3452	3460	rVB7	9890	16188	0.65%	0.173%
58	24.917	3646	3648	3650	rBV3	3110	3045	0.12%	0.033%
59	25.117	3678	3682	3685	rBV5	2777	4215	0.17%	0.045%
60	25.205	3686	3697	3709	rVB2	190731	554198	22.19%	5.933%
61	25.451	3727	3739	3752	rVB2	165978	537183	21.51%	5.751%
62	26.021	3834	3836	3839	rBV3	2487	3095	0.12%	0.033%
63	26.438	3905	3907	3910	rVB4	3340	3346	0.13%	0.036%
64	26.597	3933	3934	3937	rBV3	3678	2656	0.11%	0.028%
65	26.679	3944	3948	3950	rBV5	3482	5483	0.22%	0.059%
66	26.738	3950	3958	3965	rVV5	7919	26499	1.06%	0.284%
67	26.832	3970	3974	3975	rBV4	2558	2687	0.11%	0.029%
68	27.190	4033	4035	4039	rBV4	2327	3296	0.13%	0.035%
69	27.596	4103	4104	4106	rBV2	3710	3117	0.12%	0.033%
70	27.954	4162	4165	4168	rBV5	2014	3084	0.12%	0.033%
71	28.001	4171	4173	4175	rBV3	3033	3084	0.12%	0.033%
72	28.083	4185	4187	4190	rVB4	2551	2803	0.11%	0.030%
73	28.112	4190	4192	4194	rBV3	3638	2867	0.11%	0.031%
74	28.500	4257	4258	4261	rBV3	2460	2725	0.11%	0.029%
75	29.493	4425	4427	4429	rVV3	2818	2613	0.10%	0.028%
76	29.516	4429	4431	4434	rVB4	2804	2709	0.11%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052089.D
Acq On : 20 Jan 2022 1:28
Operator : CG/JU
Sample : N1169-01ME
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7ME

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	32.183	4882	4885	4887	rBV4	2912	3143	0.13%	0.034%
78	32.595	4953	4955	4959	rVB5	3612	3588	0.14%	0.038%
79	32.636	4959	4962	4963	rVB2	2628	2546	0.10%	0.027%




Sum of corrected areas: 9340745

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052089.D
Acq On : 20 Jan 2022 1:28
Operator : CG/JU
Sample : N1169-01ME
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7ME

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

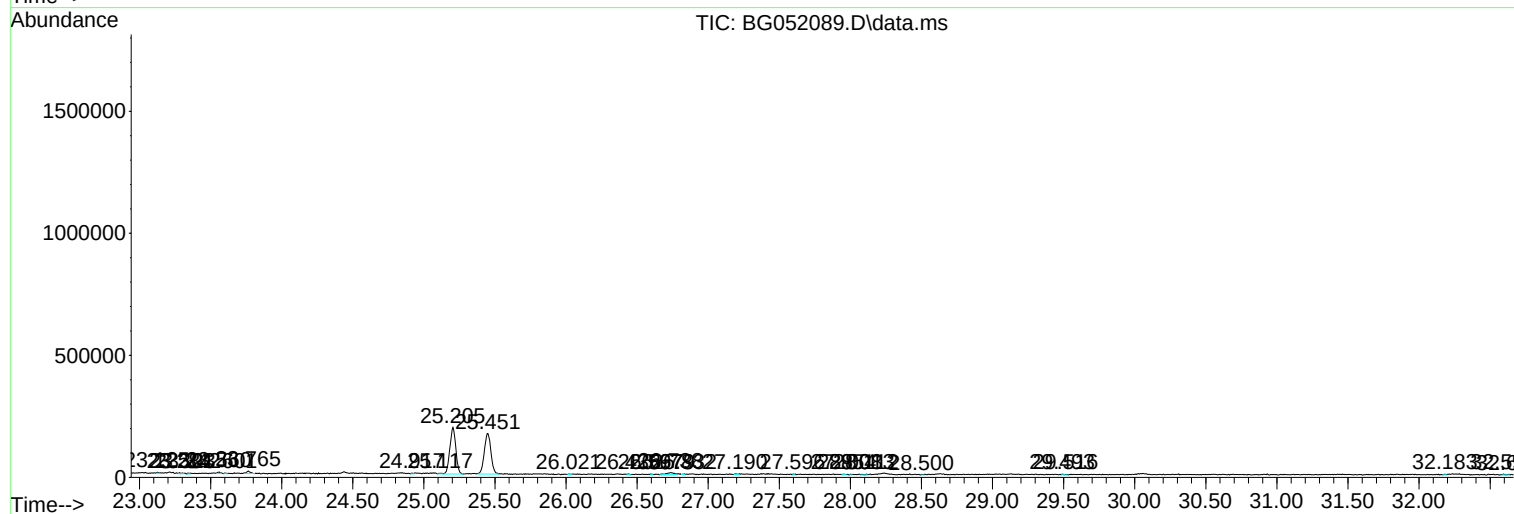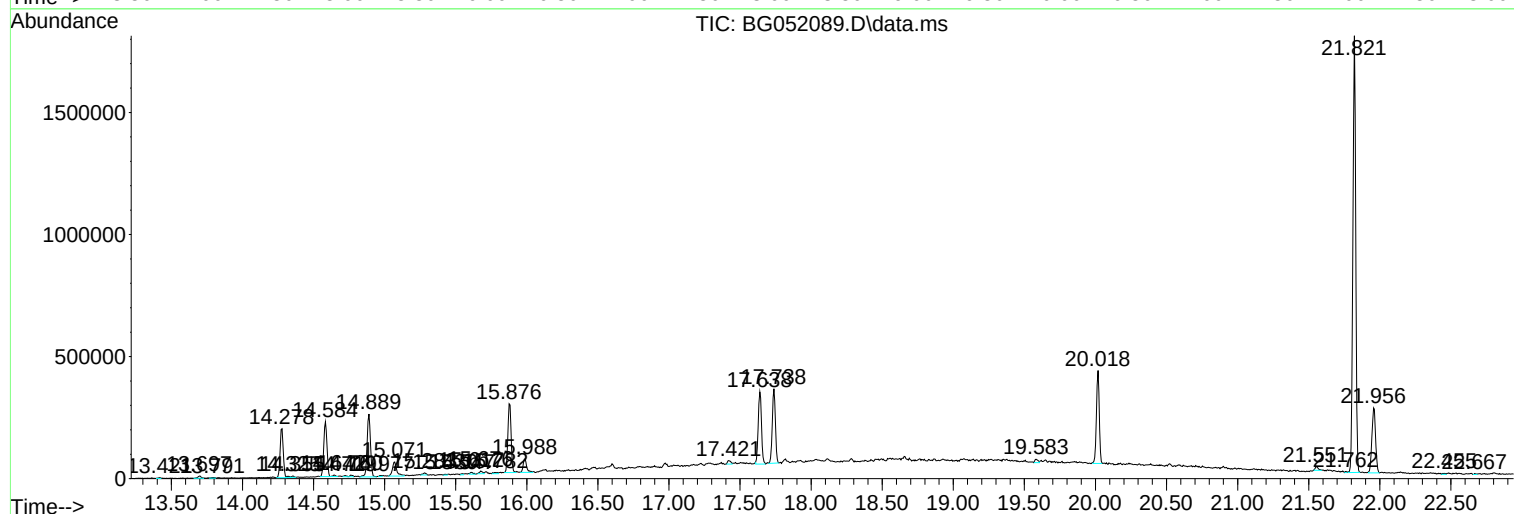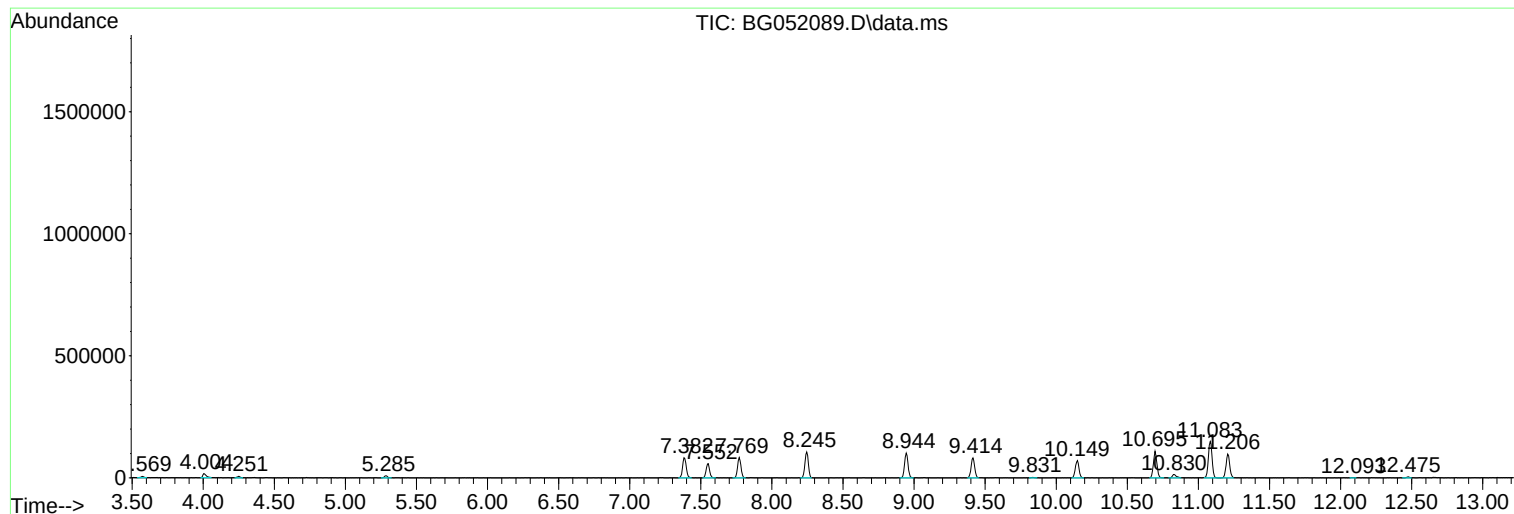

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052089.D
Acq On : 20 Jan 2022 1:28
Operator : CG/JU
Sample : N1169-01ME
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7ME

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052089.D
Acq On : 20 Jan 2022 1:28
Operator : CG/JU
Sample : N1169-01ME
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7ME

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc