

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052094.D
 Acq On : 20 Jan 2022 9:45
 Operator : CG/JU
 Sample : N1169-01MEDL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	11	15	22	rVB6	2988	4512	0.31%	0.063%
2	4.011	84	89	96	rBV2	8909	15065	1.02%	0.210%
3	4.252	126	130	135	rVB3	3669	5262	0.36%	0.073%
4	4.357	144	148	154	rVB3	2272	3616	0.24%	0.050%
5	5.291	303	307	313	rVB2	4631	7345	0.50%	0.102%
6	7.389	658	664	676	rBV2	48965	85253	5.77%	1.187%
7	7.553	686	692	700	rBV	33507	58918	3.99%	0.820%
8	7.776	723	730	737	rBV	44155	76329	5.17%	1.063%
9	8.252	804	811	818	rBV	123792	207228	14.03%	2.885%
10	8.951	924	930	940	rBV	56586	97985	6.63%	1.364%
11	9.421	1004	1010	1018	rVB	48162	86444	5.85%	1.203%
12	10.155	1127	1135	1143	rBV	38780	69552	4.71%	0.968%
13	10.702	1222	1228	1238	rVB	60192	107345	7.27%	1.494%
14	10.837	1245	1251	1262	rVB4	6732	13622	0.92%	0.190%
15	11.089	1287	1294	1302	rVB	171363	311098	21.06%	4.331%
16	11.213	1309	1315	1323	rBV2	54853	101865	6.89%	1.418%
17	12.482	1528	1531	1536	rVB3	2522	2769	0.19%	0.039%
18	13.704	1735	1739	1742	rVB5	4749	6830	0.46%	0.095%
19	14.197	1820	1823	1825	rVV3	1751	2387	0.16%	0.033%
20	14.279	1830	1837	1842	rBV	118446	177887	12.04%	2.476%
21	14.320	1842	1844	1847	rVV3	4173	4614	0.31%	0.064%
22	14.356	1847	1850	1854	rVV2	2950	4429	0.30%	0.062%
23	14.532	1877	1880	1883	rVV3	2310	3371	0.23%	0.047%
24	14.585	1883	1889	1895	rVB	138643	209267	14.16%	2.913%
25	14.649	1895	1900	1903	rBV5	4931	7406	0.50%	0.103%
26	14.685	1904	1906	1911	rVV6	1985	2980	0.20%	0.041%
27	14.767	1916	1920	1923	rBV2	4004	5337	0.36%	0.074%
28	14.890	1934	1941	1949	rVB	303998	483229	32.71%	6.727%
29	14.972	1949	1955	1957	rBV4	3711	6323	0.43%	0.088%
30	15.072	1963	1972	1980	rBV2	29788	58584	3.97%	0.816%
31	15.231	1996	1999	2001	rVV2	1913	2055	0.14%	0.029%
32	15.284	2003	2008	2013	rVB8	4893	8341	0.56%	0.116%
33	15.589	2059	2060	2063	rBV3	3080	3824	0.26%	0.053%
34	15.613	2063	2064	2069	rVB5	5130	5150	0.35%	0.072%
35	15.683	2072	2076	2079	rVV6	7997	11042	0.75%	0.154%
36	15.713	2079	2081	2086	rVB5	4690	6325	0.43%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052094.D
 Acq On : 20 Jan 2022 9:45
 Operator : CG/JU
 Sample : N1169-01MEDL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.877	2103	2109	2115	rBV	175278	261317	17.69%	3.638%
38	15.983	2123	2127	2133	rBV5	24333	44101	2.99%	0.614%
39	16.030	2133	2135	2136	rBV2	2481	1920	0.13%	0.027%
40	16.118	2144	2150	2151	rBV6	6068	8568	0.58%	0.119%
41	16.347	2188	2189	2193	rBV4	3454	3075	0.21%	0.043%
42	16.394	2195	2197	2198	rBV2	3162	2188	0.15%	0.030%
43	16.576	2224	2228	2229	rBV3	5704	7697	0.52%	0.107%
44	16.606	2231	2233	2238	rVB6	11525	11224	0.76%	0.156%
45	16.976	2292	2296	2300	rBV7	8340	13853	0.94%	0.193%
46	17.639	2403	2409	2417	rBV	349237	540142	36.56%	7.519%
47	17.739	2420	2426	2432	rVB2	169811	265399	17.96%	3.694%
48	19.907	2793	2795	2802	rVB8	9589	10852	0.73%	0.151%
49	20.019	2808	2814	2819	rVB	207751	305556	20.68%	4.253%
50	20.618	2915	2916	2918	rBV2	4585	3340	0.23%	0.046%
51	20.953	2971	2973	2977	rVB5	8538	9483	0.64%	0.132%
52	21.558	3073	3076	3080	rBV6	9536	11227	0.76%	0.156%
53	21.822	3114	3121	3129	rVB	995708	1477411	100.00%	20.566%
54	21.957	3136	3144	3151	rBV	337479	572698	38.76%	7.972%
55	22.116	3170	3171	3172	rBV	3322	1867	0.13%	0.026%
56	22.139	3172	3175	3181	rVB5	8067	12010	0.81%	0.167%
57	22.803	3284	3288	3293	rVB6	10095	14637	0.99%	0.204%
58	23.373	3383	3385	3387	rBV3	2293	2243	0.15%	0.031%
59	23.408	3389	3391	3395	rBV4	1775	2201	0.15%	0.031%
60	23.555	3410	3416	3422	rBV4	14362	26630	1.80%	0.371%
61	24.324	3545	3547	3548	rVB2	3358	2202	0.15%	0.031%
62	24.436	3556	3566	3572	rBV3	21583	49270	3.33%	0.686%
63	24.724	3614	3615	3619	rBV4	2216	2026	0.14%	0.028%
64	24.912	3645	3647	3649	rBV4	2653	1979	0.13%	0.028%
65	25.206	3686	3697	3710	rVB2	109488	314464	21.28%	4.377%
66	25.452	3726	3739	3753	rVB2	201333	676885	45.82%	9.423%
67	25.805	3798	3799	3803	rBV4	2138	2577	0.17%	0.036%
68	25.928	3818	3820	3824	rVB5	2248	2126	0.14%	0.030%
69	25.981	3826	3829	3832	rBV5	2757	3975	0.27%	0.055%
70	26.216	3868	3869	3872	rBV3	2268	2132	0.14%	0.030%
71	26.381	3896	3897	3901	rBV4	2090	2716	0.18%	0.038%
72	26.463	3909	3911	3915	rVB5	2093	1922	0.13%	0.027%
73	26.727	3948	3956	3966	rVB4	25929	79828	5.40%	1.111%
74	26.892	3982	3984	3986	rVB3	3138	2623	0.18%	0.037%
75	27.197	4034	4036	4039	rVB4	2531	2548	0.17%	0.035%
76	27.338	4057	4060	4061	rBV3	3026	2744	0.19%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052094.D
 Acq On : 20 Jan 2022 9:45
 Operator : CG/JU
 Sample : N1169-01MEDL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLW7MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	27.379	4064	4067	4068	rBV2	2713	2771	0.19%	0.039%
78	27.890	4152	4154	4160	rVB7	1910	2132	0.14%	0.030%
79	28.231	4200	4212	4223	rBV4	20969	80392	5.44%	1.119%
80	28.489	4254	4256	4258	rVB3	2431	2214	0.15%	0.031%
81	28.513	4258	4260	4263	rBV4	2035	2808	0.19%	0.039%
82	28.583	4270	4272	4276	rBV5	1844	2715	0.18%	0.038%
83	29.053	4351	4352	4354	rBV2	2263	2074	0.14%	0.029%
84	29.224	4376	4381	4382	rVB4	2508	3164	0.21%	0.044%
85	29.277	4389	4390	4392	rBV2	3805	2777	0.19%	0.039%
86	29.418	4413	4414	4417	rVB3	2747	1917	0.13%	0.027%
87	29.506	4428	4429	4434	rBV3	2570	2749	0.19%	0.038%
88	29.547	4434	4436	4438	rBV3	2812	3482	0.24%	0.048%
89	29.641	4450	4452	4456	rVB4	2406	2509	0.17%	0.035%
90	30.023	4510	4517	4518	rBV7	11135	18470	1.25%	0.257%
91	30.175	4542	4543	4547	rBV2	2006	2180	0.15%	0.030%
92	30.598	4613	4615	4617	rVB3	2181	1990	0.13%	0.028%
93	30.663	4625	4626	4628	rBV2	2183	1965	0.13%	0.027%
94	30.869	4659	4661	4665	rBV5	2606	3191	0.22%	0.044%
95	31.274	4727	4730	4732	rBV3	1997	2207	0.15%	0.031%
96	31.844	4824	4827	4829	rVB4	2878	2914	0.20%	0.041%
97	32.214	4884	4890	4891	rBV4	7593	8630	0.58%	0.120%
98	32.349	4911	4913	4914	rBV2	2292	1879	0.13%	0.026%
99	32.519	4939	4942	4943	rBV3	2609	2064	0.14%	0.029%
100	32.602	4953	4956	4959	rVB4	2448	3228	0.22%	0.045%




Sum of corrected areas: 7183667

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052094.D
Acq On : 20 Jan 2022 9:45
Operator : CG/JU
Sample : N1169-01MEDL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

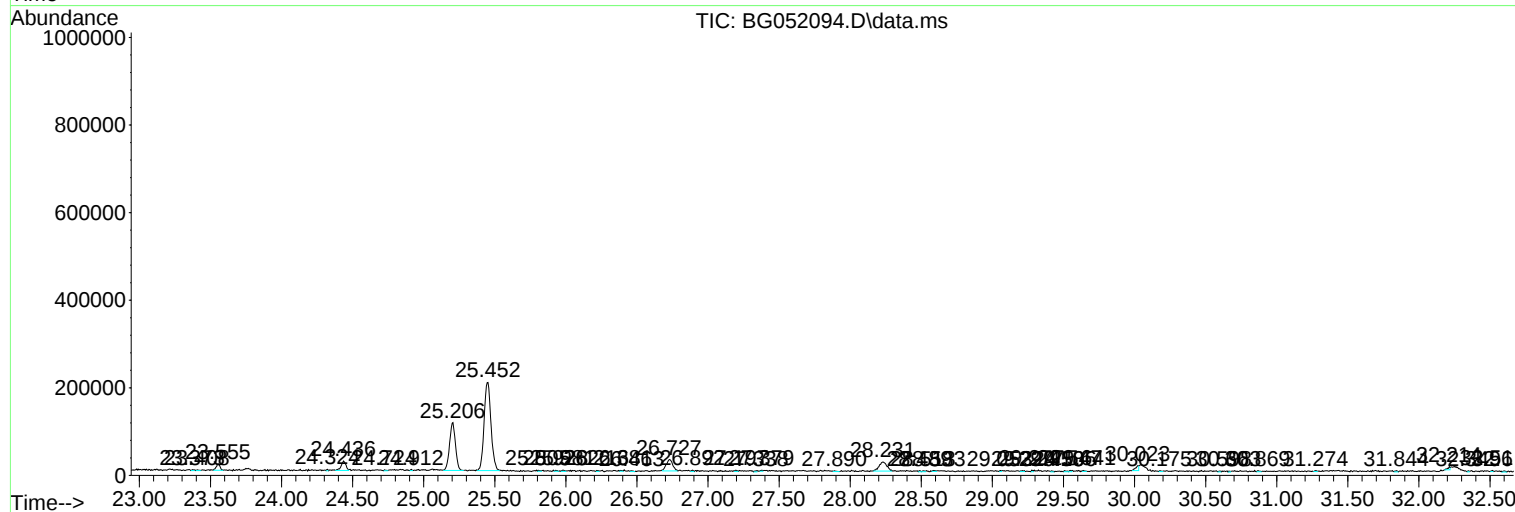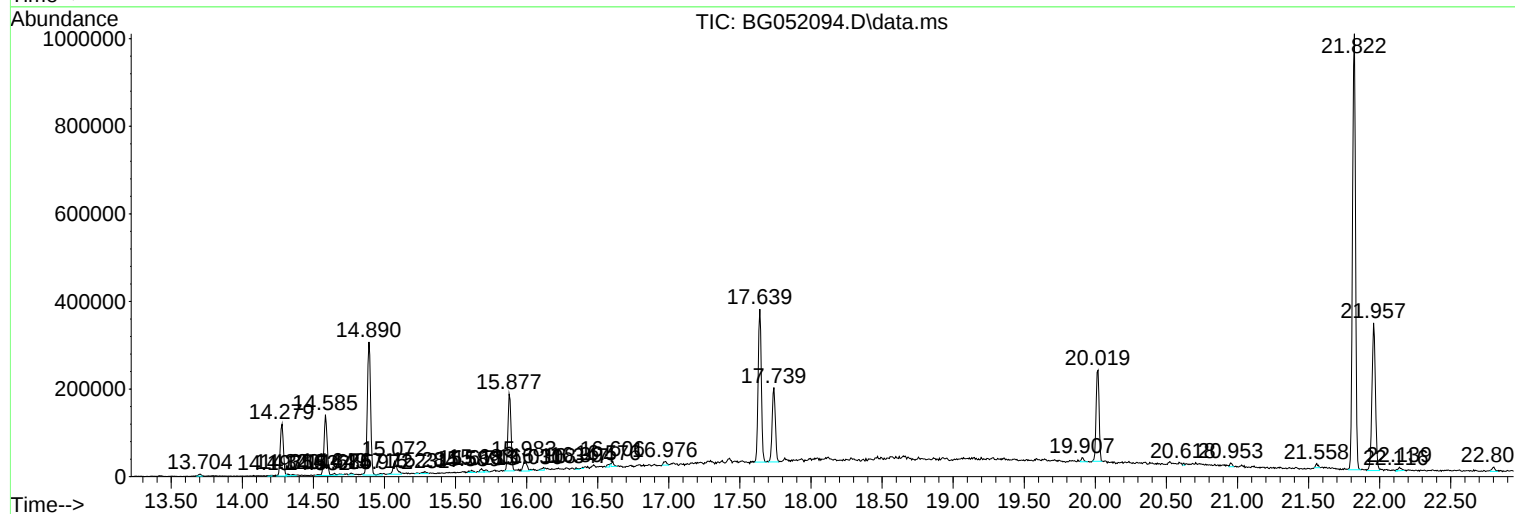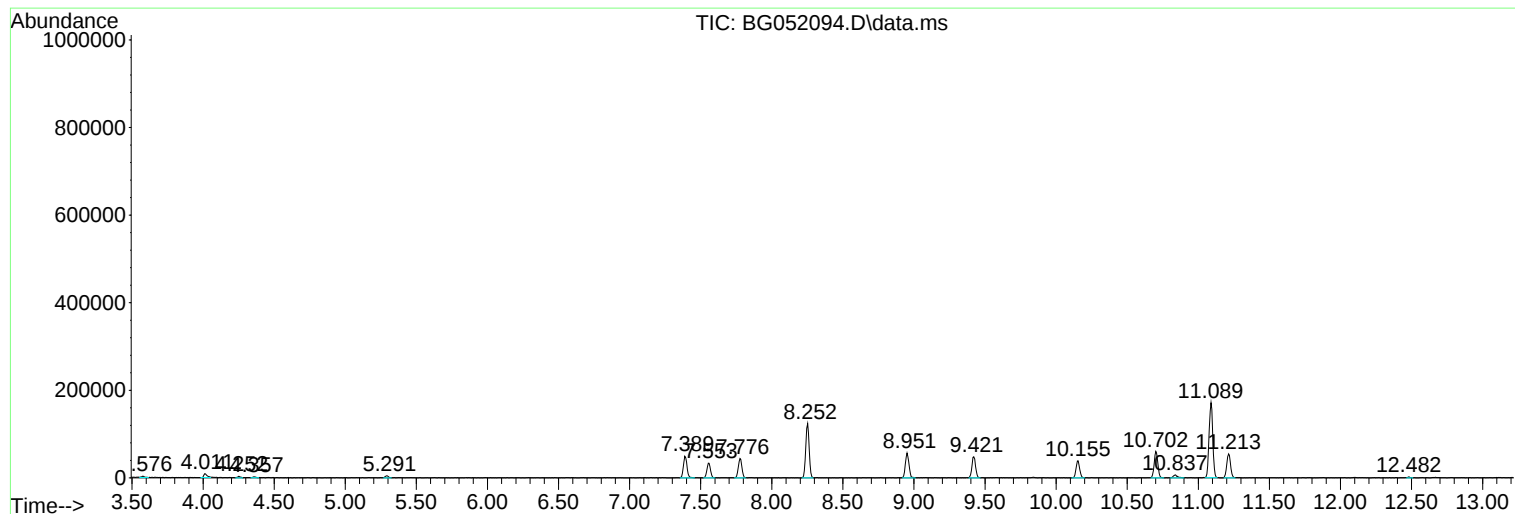

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052094.D
Acq On : 20 Jan 2022 9:45
Operator : CG/JU
Sample : N1169-01MEDL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7MEDL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
26.727	2.36 ng/ul	79828	Perylene-d12	25.452

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexacosane	366	C26H54	000630-01-3	83
2			Octadecane	254	C18H38	000593-45-3	78
3			5-Ethyl-5-methylnonadecane	310	C22H46	1000360-42-7	72
4			Heptadecane	240	C17H36	000629-78-7	72
5			Eicosane, 7-hexyl-	366	C26H54	055333-99-8	72

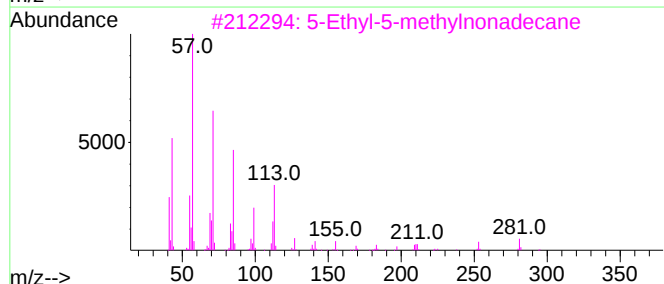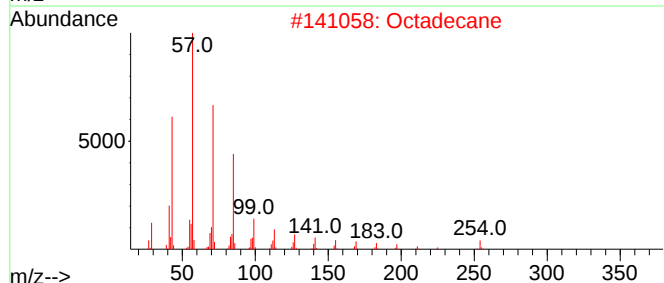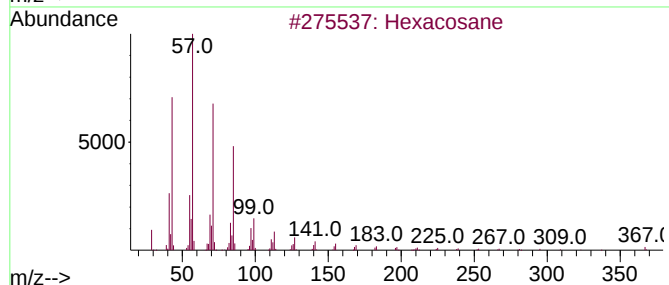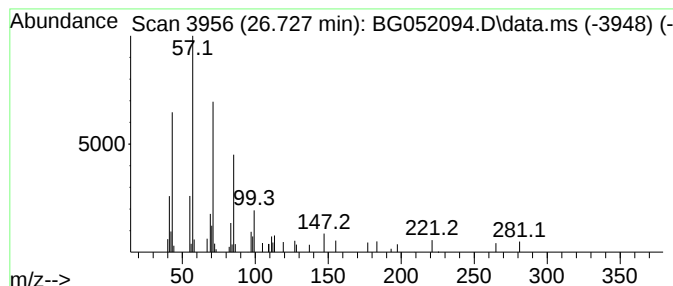

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052094.D
Acq On : 20 Jan 2022 9:45
Operator : CG/JU
Sample : N1169-01MEDL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7MEDL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
28.231	2.38 ng/ul	80392	Perylene-d12	25.452

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Octacosane, 2-methyl-	408	C29H60	001560-98-1	87
2		2-Methyltetracosane	352	C25H52	001560-78-7	87
3		Octacosane	394	C28H58	000630-02-4	86
4		Hentriacontane	437	C31H64	000630-04-6	86
5		Hexacosane	366	C26H54	000630-01-3	86

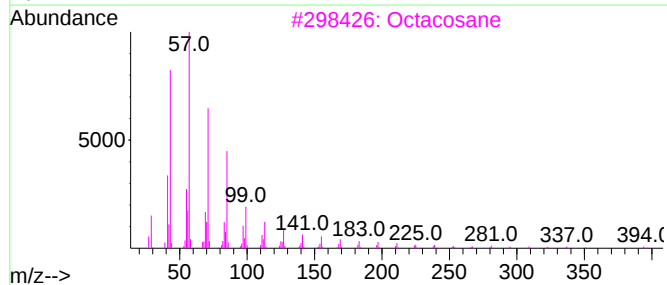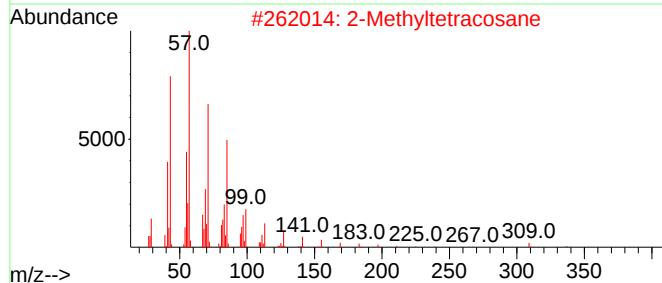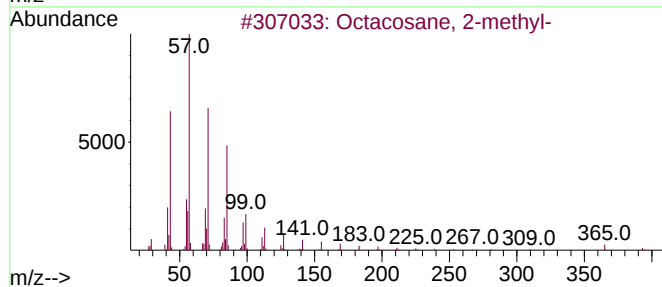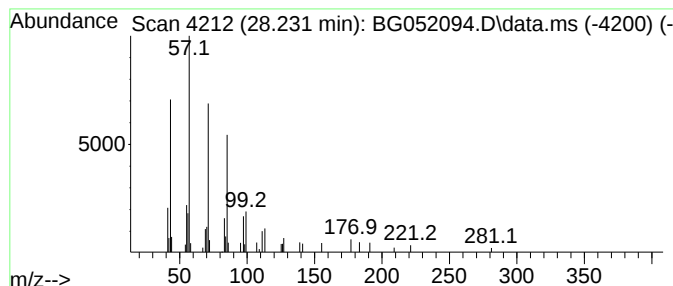

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052094.D
Acq On : 20 Jan 2022 9:45
Operator : CG/JU
Sample : N1169-01MEDL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLW7MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	26.727	2.4	ng/u1	79828	6	25.452	676885	20.0
(DEL) Alkane: S...	28.231	2.4	ng/u1	80392	6	25.452	676885	20.0